

Search
over 5,000 LC
applications at:



www.phenomenex.com/application

Chiral LC

Chiral LC Column Types.....	194
Polysaccharide Chiral Columns.....	293
Lux	293
Additional Chiral LC Columns	
Chiral CD-Ph	222
Chirex	223
Hypercarb.....	233
Sumichiral OA	337
Ultron ES	349

HPLC Column Selection

Column Selection Tree	195
Column Selection by Application	196
Column Selection by Manufacturer	197-199
Column Selection by Separation Mode.....	200
Column Selection by USP Specifications	201-204
Column Selection by Ph. Eur. Listing	205-209

HPLC Column Protection

Column Performance Check Standards	414-415
SecurityGuard Cartridge System.....	326

HPLC/UHPLC Columns

Aeris	210
Aqua.....	219
Asahipak	219
Axia Packed Columns	372
BioSep	220
Bondclone.....	222
Capcell Pak.....	222
Chiral CD-Ph.....	222
Chirex.....	223
Clarity	393
Columbus.....	225
Cosmosil	225
Curosil	225

Develosil	225
EnviroSep.....	225
EZ:faast.....	389
Gemini	226
Hamilton.....	233
Hypercarb	233
HyperClone.....	234
Hypersil	233
Hypersil BDS.....	233
IB-Sil.....	233
InertClone	236
Inertsil	233
Jupiter	237
Kinetex	240
Kromasil	269
LiChrosorb	269
LiChrospher	269
Luna	270
Luna Omega	284
Lux	293
Lux AMP	302
Merck KGaA.....	304
Nucleosil	304
Onyx	305
Phenogel	308
PhenoSphere	314
PhenoSphere-NEXT.....	314
PLgel, PLRP-S.....	314
PolymerX.....	315
PolySep-GFC-P	316
PREP/Preparative	371
Prodigy.....	317
Rezex	318

“ At first, I honestly didn't believe the marketing claim that their Core-Shell 5 μ particles had greater efficiency than fully porous 3 μ particles. But wow! Now I can issue my awesome, cutting edge chromatography, and QC can have their jumbo, 5 μ , abuse-proof particles. Everybody wins. ”

Chester Chan
Nexgen Pharma, USA

HPLC/UHPLC Columns (cont'd)

SecurityGuard	326
SecurityGuard ULTRA	331
Selectosil	332
Shodex.....	332
SphereClone	335
Spherex.....	336
Spherisorb	336
STAR-ION A300	337
Sumichiral OA Chiral	337
Synergi	338
Ultracarb	349
Ultremex.....	349
Ultron ES Chiral	349
Yarra	350
ZORBAX.....	359

HPLC Accessories and Consumables.....406-421

SecurityCAP LC Solvent Safety Products....324-325

Proteins/Peptides

Aeris	210
Aeris PREP.....	217
BioSep	220
Jupiter.....	237
Yarra.....	350
Yarra PREP	358

UHPLC Columns

Kinetex 1.3 μ m, 1.7 μ m and 2.6 μ m Core-Shell Technology Columns.....	240
Luna Omega 1.6 μ m Fully Porous Columns	284
Aeris Core-Shell Technology for RP-LC of Proteins & Peptides.....	210
Clarity Core-Shell Columns for Synthetic DNA/RNA	393
SecurityGuard ULTRA Column Protection	331



SecurityGuard Analytical Holder with Cartridge



SecurityGuard Ultra Holder with Cartridge



The opinions stated herein are solely those of the speaker and not necessarily those of any company or organization.


Chiral LC Column Types

LC Chiral Stationary Phase (CSP) Classification Diagram


Type	Description	Chemistry	Mechanism	Brands	Page
I	Brush (Pirkle)	Low molecular weight chiral selectors Ionic or covalent bonding	Attractive interactions Hydrogen bonding Charge transfer (π - π interaction) Dipole stacking	Chirex Sumichiral OA	199
					295
II	Helical Polymers	Cellulose and amylose derivatives	Attractive interactives Insertion complexes	Lux Cellulose and Amylose	257
III	Cavity	Cyclodextrins, Crown ether	Inclusion complexes	Chiral CD-Ph Sumichiral OA	198
					295
IV	Ligand Exchange	Amino acid-metal complex	Diastereomeric metal complex	Chirex Sumichiral OA	199 295
V	Protein	α -acid glycoprotein Bovine Serum Albumin	Hydrophobic interactions Polar interactions	Ultron ES	308
VI	Macrocyclic	Antibiotics Glycopeptides	Hydrogen bonding Charge transfer (π - π interaction) Inclusion complexation Ionic interactions Peptide bonding	None	

Other Types Carbon-Based (Hypercarb) and Ceramic-based (Ceramospher)


Type I Brush (Pirkle)

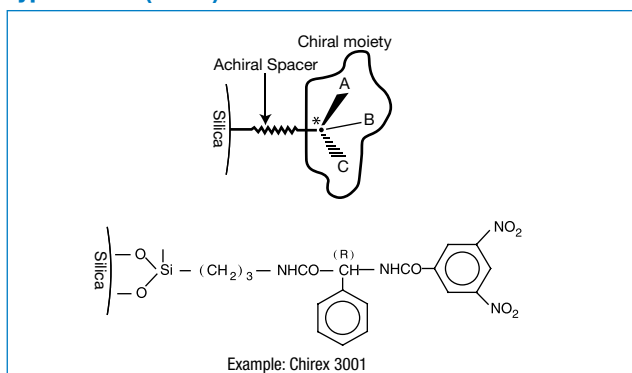


Type II Helical Polymers (Polysaccharide)

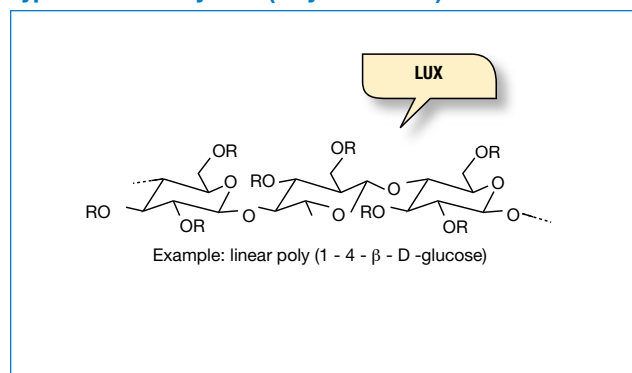


Type III Cavity

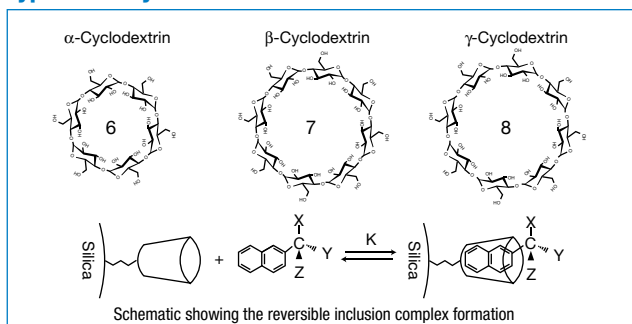

Type IV Ligand Exchange

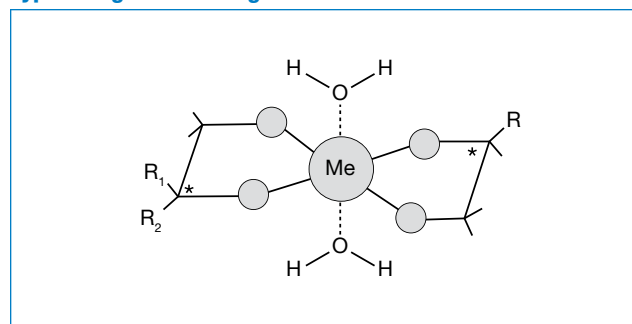

Type V Protein

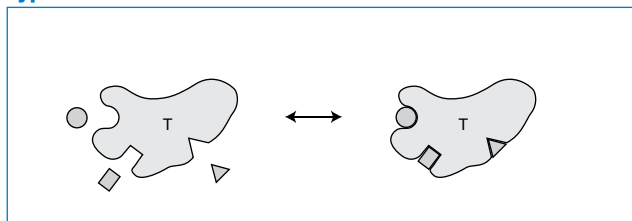

HPLC Column Selection Tree

Sample MW	Sample Solubility	Separation Mode	Our Recommended Column	Page		
MW < 5000	Organic-Soluble	Hexane-Soluble	Normal Phase Adsorption	Kinetex HILIC _____ 240 Luna Silica(2) _____ 270		
			Normal Phase Bonded	Luna CN, NH ₂ , HILIC _____ 270		
		Methanol Methanol/H ₂ O Soluble	Reversed Phase Bonded	Kinetex C18, EVO C18, XB-C18, C8, Phenyl-Hexyl, Biphenyl, F5, Polar C18 _____ 240 Synergi Max-RP, Fusion-RP _____ 338		
	Luna C8(2), C18(2) _____ 270 Luna Omega C18, Omega PS C18, Omega C18 Polar _____ 284 Gemini C18, NX-C18, C6-Phenyl _____ 226 Lux _____ 293					
	THF-Soluble	Gel Permeation GPC	Phenogel 50 Å, 100 Å _____ 308			
	Aqueous-Soluble	Non ionic	Reversed Phase	Kinetex C18, EVO C18, XB-C18, C8, Phenyl-Hexyl, Biphenyl, F5, Polar C18 _____ 240 Synergi Polar-RP, Hydro-RP _____ 338 Luna C8(2), C18(2), Luna PFP(2) _____ 270 Luna Omega C18, Omega PS C18, Omega Polar C18 _____ 284 Gemini C18, NX-C18 _____ 226 Onyx C18 _____ 305 Lux _____ 293		
			Chiral	Lux _____ 293		
		Ionic	Ion Pairing / Reversed Phase	Kinetex C18, EVO C18, XB-C18, C8, Polar C18 _____ 240 Synergi Max-RP, Hydro-RP _____ 338 Luna C8(2), C18(2) _____ 270 Luna Omega C18, Omega PS C18, Omega Polar C18 _____ 284 Gemini C18, NX-C18 _____ 226 Onyx C18 _____ 305		
				Ion-Exchange	Luna SCX, NH ₂ _____ 270 PhenoSphere SAX _____ 314 Clarity Oligo-SAX _____ 394	
			HILIC	Kinetex HILIC _____ 240 Luna HILIC, NH ₂ , Si(2) _____ 270		
			Chiral	Lux _____ 293 Chirex _____ 223		
			Peptides	Reversed Phase	Aeris PEPTIDE _____ 210 Jupiter Proteo _____ 237 Kinetex EVO C18 _____ 240 Luna Omega PS C18 _____ 284	
		MW > 5000	Organic-Soluble	Gel Permeation Chromatography (GPC)	Unknown MW Range	Phenogel Linear (2) _____ 308 Shodex GPC _____ 332
					Known MW Range	Specific Pore: Phenogel _____ 308 Shodex GPC _____ 332
			Aqueous-Soluble	Gel Filtration Aqueous GFC/SEC	pH 2-7.5	Yarra SEC Series _____ 354 BioSep-SEC-S Series _____ 220
pH > 7.5					PolySep-GFC-P _____ 316	
Ion-Exchange				Cation-Exchange	Shodex IEC CM-825 _____ 332	
	Anion-Exchange		Clarity Oligo-SAX _____ 394 Shodex IEC DEAE _____ 332			
Aqueous-Soluble	Reversed Phase		pH 2-9	Aeris WIDEPOR C4, XB-C8, XB-C18 _____ 210 Jupiter 300 C4, C5, C18 _____ 237		
			pH > 9	Hamilton PRP-3 _____ Inquire		
Aqueous-Soluble	Hydrophobic Interaction (HIC)		Shodex HIC _____ 332			

HPLC Column Selection by Application

This table is to aid you in selecting the right column for your application. For application notes or method development assistance please call your technical representative.

Amino Acids	Page
Phenomenex EZ:faast (GC and LC/MS)	390
Phenomenex Chirex (chiral)	223
Phenomenex Lux (chiral)	293
Phenomenex Kinetex EVO C18 (Fmoc or OPA derivatized)	240
Anions	
Phenomenex Luna NH ₂	270
Phenomenex STAR-ION A300	337
Phenomenex Lux (chiral)	293
Phenomenex PhenoSphere SAX	314
Hamilton PRP	233
Shodex IC	332
Phenomenex Clarity Oligo-SAX	373
Phenomenex Rezex ROA-Organic Acid	318
Antibiotics	
Phenomenex Kinetex	240
Phenomenex Gemini / Gemini NX	226
Phenomenex Luna	270
Phenomenex Luna Omega	284
Phenomenex Synergi	338
Biotechnology/Life Sciences	
Phenomenex Aeris WIDEPORE	210
Phenomenex Aeris PEPTIDE	210
Phenomenex Clarity	373
Phenomenex Jupiter 300/Jupiter Proteo	237
Phenomenex BioSep-SEC-S	250
Phenomenex Yarra SEC	350
Phenomenex PolySep-GFC-P	316
Phenomenex Luna SCX	270
Phenomenex Luna Omega PS C18	284
Phenomenex Luna NH ₂	270
Shodex GFC, KW	332
Carbohydrates	
Phenomenex Rezex	318
Phenomenex Luna NH ₂	270
Shodex SUGAR	332
Cations	
Phenomenex Luna SCX	270
Hamilton PRP	233
Enantiomers (Chiral)	
Phenomenex Lux	293
Phenomenex Chirex	223
Environmental (Carbamates, PAH's, Explosives)	
Phenomenex Zebron (GC)	83
Phenomenex Kinetex	240
Phenomenex Gemini / Gemini NX	226
Phenomenex Luna	270
Phenomenex Luna Omega	284
Phenomenex Synergi	338
Foods, Flavors and Fragrances	
Phenomenex Rezex	318
Phenomenex Kinetex	240
Phenomenex Gemini / Gemini NX	226
Phenomenex Luna	270
Phenomenex Luna Omega	284
Phenomenex Lux (chiral)	293
Phenomenex Synergi	338
Phenomenex Zebron (GC)	83

Nucleosides and Nucleotides	Page
Phenomenex Kinetex EVO C18	240
Phenomenex Luna NH ₂ , SCX	270
Phenomenex Luna Omega Polar C18, Luna Omega PS C18	284
Phenomenex Synergi Polar-RP	338
Phenomenex PhenoSphere SAX	314
Oligonucleotides	
Phenomenex Clarity Oligo-XT	373
Phenomenex Clarity Oligo-RP	373
Phenomenex Clarity Oligo-MS	373
Phenomenex Clarity Oligo-SAX	373
Phenomenex Aeris WIDEPORE	210
Organic Acids	
Phenomenex Luna Omega PS C18	284
Phenomenex Rezex	318
Phenomenex Synergi Hydro-RP	338
Peptides/Proteins	
Phenomenex Aeris WIDEPORE	210
Phenomenex Aeris PEPTIDE	210
Phenomenex Jupiter 300/Jupiter Proteo	237
Phenomenex Luna SCX, NH ₂	270
Phenomenex Yarra SEC	350
Phenomenex BioSep-SEC-S	220
Phenomenex Luna Omega PS C18	284
Pesticides, Herbicides, and Dioxins	
Phenomenex Kinetex	240
Phenomenex Gemini / Gemini NX	226
Phenomenex Synergi	338
Phenomenex Luna	270
Phenomenex Luna Omega	284
Phenomenex Zebron (GC)	83
Pharmaceuticals	
Phenomenex Kinetex	240
Phenomenex Gemini / Gemini NX	226
Phenomenex Synergi	338
Phenomenex Luna	270
Phenomenex Luna Omega	284
Phenomenex Lux (chiral)	293
Phenomenex Chirex (chiral)	223
Polymers, Plastics, Rubber	
Phenomenex Zebron (GC)	83
Phenomenex Phenogel	308
Shodex Asahipak GF	219
Vitamins	
Phenomenex Kinetex	240
Phenomenex Gemini / Gemini NX	226
Phenomenex Synergi	338
Phenomenex Luna	270
Phenomenex Luna Omega	284
Taxanes	
Phenomenex Kinetex F5	240
Phenomenex Luna PFP(2)	270
Textiles/Dyes	
Phenomenex Kinetex	240
Phenomenex Gemini / Gemini NX	226
Phenomenex Synergi	338
Phenomenex Luna	270
Phenomenex Luna Omega	284
Phenomenex Phenogel GPC	308

HPLC Column Selection by Manufacturer

In recognizing the tremendous difficulty the chromatographer has in choosing from literally hundreds of columns and to aid in your selection of alternative materials from different manufacturers, an HPLC column selection guide is presented below.

This selection is, neither in terms of manufacturers nor in terms of their products, a complete list, and the accuracy of the data is not guaranteed.

Column	Phenomenex Alternative*	Phenomenex Recommended Alternative**
Agilent Technologies / Varian / Polymer Labs		
Advanced Bio SEC	Yarra	BioSep
Advanced Bio RP	Aeris	Jupiter
Bio SEC	BioSep-SEC-S	Yarra
Chiradex	Lux	Chirex
HC-C18(2)	Luna C18(2)	Synergi Hydro-RP
MetaSil	Prodigy	Luna
MetaSil AQ C18	Aqua C18	Synergi Hydro-RP
Microsorb	Luna	Synergi
Microsorb 300 Å	Jupiter 300	Aeris WIDEPORE
PL-Aquagel-OH	PolySep GFC-P	Shodex OHpak SB-800H
PLgel	Phenogel	Phenogel
PL Hi-PLEX	Rezex	Rezex
PLRP-S	PolymerX RP-1	Gemini NX-C18
PLRP-S 300 Å	Hamilton PRP-3	Aeris WIDEPORE
PlusPore	Phenogel	Phenogel
Polaris C18 Amide, C8 Ether	Luna Omega Polar C18	Synergi Fusion-RP
Poroshell 300	Aeris WIDEPORE	Aeris WIDEPORE
Poroshell 120	Kinetex	Kinetex
Pursuit	Luna	Synergi
Pursuit DiPhenyl	Kinetex Biphenyl	Gemini C6-Phenyl
Taxsil (1, 2, 3)	Luna PFP(2)	Kinetex F5
TC-C18(2)	Synergi Hydro-RP	Luna C18(2)
ZORBAX Eclipse-XDB	Luna	Kinetex
ZORBAX Eclipse Plus	Gemini	Kinetex EVO C18
ZORBAX Rapid Resolution HT	Kinetex	Luna Omega
ZORBAX PrepHT	Luna(3) 10 µm	Luna 10 µm <i>PREP</i>
ZORBAX Rx	HyperClone	Luna
ZORBAX SB 80 Å	Kinetex XB-C18	Luna
ZORBAX SB 300 Å	Jupiter 300	Aeris WIDEPORE
ZORBAX SB Aq	Synergi Hydro-RP	Synergi Hydro-RP
ZORBAX GF (BioSeries)	BioSep-SEC-S	Yarra
ZORBAX Extend-C18	Gemini NX-C18	Kinetex EVO C18
ZORBAX 300 Extend	Jupiter 300	Aeris WIDEPORE
ZORBAX Bonus RP	Synergi Fusion-RP	Synergi Hydro-RP
ZORBAX Oligo	Clarity Oligo-RP	Clarity Oligo-MS
ZORBAX Carbohydrate	Luna NH ₂	Rezex
Hichrom Ltd.		
Alltima	Luna	Luna Omega
Alltima HP	Luna	Kinetex
Apex	Luna	Kinetex
Apollo	Luna	Kinetex
Genesis	Luna	Gemini
Prevail	Synergi	Luna
Vydac	Jupiter	Aeris
Bio-Rad		
Aminex	Rezex	Rezex
Macro-Prep	—	Shodex IEC
UNOsphere	—	Shodex IEC

Column	Phenomenex Alternative*	Phenomenex Recommended Alternative**
Chiral Technologies/DAICEL Corporation		
CHIRALCEL AY-H	Lux Amylose-2	Lux Cellulose-2
CHIRALCEL OD-H	Lux Cellulose-1	Lux Cellulose-2
CHIRALCEL OJ-H	Lux Cellulose-3	Lux Cellulose-4
CHIRALCEL OX-H	Lux Cellulose-4	Lux Cellulose-2
CHIRALCEL OZ-H	Lux Cellulose-2	Lux Cellulose-4
CHIRALPAK AD-H	Lux Amylose-1	Lux Amylose-2
CHIRALPAK IA	Lux i-Amylose-1	—
CHIRALPAK IC	Lux i-Cellulose-5	—
E.S. Industries		
Aquasep	Synergi Fusion-RP	Synergi Hydro-RP
Chromegabond	Nucleosil	Luna
Chromegabond HC	Ultrapak ODS (30)	Synergi Hydro-RP
Chromegabond BAS	Synergi Fusion-RP	Synergi Hydro-RP
Chromegabond WR	Luna	Gemini
Epic	Synergi 2.5 µm	Kinetex
Epic Polar	Kinetex Biphenyl	Synergi Hydro-RP
FluoroSep-RP Phenyl	Luna Phenyl-Hexyl	Kinetex Phenyl-Hexyl
FluoroSep-RP Octyl	—	Kinetex C8
Gammabond C1	PhenoSphere C1	Develosil TMS-UG (C1)
Gammabond C8, C18	Luna C8(2), C18(2)	Kinetex C8, C18
Gammabond PVP	—	Asahipak ODS-50
Gammabond SCX	—	Shodex IEC CM-825
Gammabond WCX	—	Asahipak ES-502C 7C
Protec-RP	Synergi Fusion-RP	Synergi Hydro-RP
GL Sciences		
Inertsil ODS-Prep-100 Å	Luna 10 µm <i>PREP</i> C18(2)	Luna 10 µm C18(2)
Inertsil ODS(2)	Prodigy ODS(2)	Luna C18(2)
Inertsil ODS(3)	Prodigy ODS(3)	Luna C18(2)
Inertsil ODS(4)	Kinetex XB-C18	Synergi Max-RP
Inertsil Peptide C18	Aeris PEPTIDE	Luna Omega PS C18
Inertsil 300 Å WP300 C8	Jupiter C5	Aeris WIDEPORE C8
InertSustain	Gemini NX-C18	Kinetex EVO C18
InertSustain AQC18	Luna Omega Polar C18	Kinetex Polar C18

* Alternative - This category indicates an alternative column which will likely give a similar selectivity.

** Recommended Alternative - This category indicates an alternative column which may yield somewhat different selectivity but may also lead to improved resolution.

HPLC Column Selection by Manufacturer

This selection is, neither in terms of manufacturers nor in terms of their products, a complete list, and the accuracy of the data is not guaranteed.

Column	Phenomenex Alternative*	Phenomenex Recommended Alternative**
MAC-MOD/Bischoff/ACT/Advanced Materials Technology		
ACE C18	Gemini NX-C18	Kinetex XB-C18
ACE-AQ	Synergi Fusion-RP	Luna Omega Polar C18
ACE-300 A	Jupiter 300	Aeris WIDEPORE
ACE Excel	Gemini NX-C18	Kinetex EVO
ACE Ultracore	Kinetex	Luna Omega
HALO	Kinetex	Luna Omega
HALO Bioclass	Aeris	Luna Omega PS C18
HALO Glycan	—	Luna NH ₂
HALO Peptide ES-C18	Aeris WIDEPORE XB-C18	Aeris PEPTIDE XB-C18
HALO Protein	Aeris WIDEPORE	Aeris WIDEPORE
HALO Penta-HILIC	Kinetex HILIC	Luna HILIC
Hydrobond	Synergi Fusion-RP	Luna Omega Polar C18
Pronto Pearl	Luna Omega	Kinetex
ProntoSIL 120 Å	Luna C18(2)	Kinetex
ProntoSIL 300 Å	Jupiter 300	Aeris WIDEPORE
ProntoSIL Aq 120 Å	Synergi Hydro-RP	Develosil RP-Aqueous(C30)
ProntoSIL Aq PLUS	Synergi Hydro-RP	Luna Omega Polar C18
ProntoSIL SH 120 Å	Gemini NX-C18	Luna C18(2)
ProntoSIL ACE-EPS	Synergi Hydro-RP	Luna Omega Polar C18
ProntoSIL Chiral AX	—	Chirex
ProntoSIL C30	Develosil C30	Luna Phenyl-Hexyl
Partisil	Luna	Synergi
Partisphere	Luna	Synergi
Ultrasphere	Luna	Synergi
Restek		
Allure	Ultracarb ODS (30)	Luna C18(2)
Force	Luna Omega	Kinetex
Pinnacle DB	HyperClone	Luna C18(2)
Pinnacle Ultra C18	Ultracarb ODS (20)	Luna C18(2)
Pinnacle II	HyperClone BDS	Luna C18(2)
Roc	Luna	Luna Omega
Raptor	Kinetex	Synergi
Ultra Aqueous	Synergi Hydro-RP	Luna Omega Polar C18
Ultra II	Kinetex	Synergi
Viva	Aeris WIDEPORE	Jupiter
Supelco / Sigma-Aldrich / MilliporeSigma		
Antibodix	—	Clarity Oligo-WAX
Ascentis	Synergi	Gemini NX-C18
Ascentis Express	Kinetex	Luna Omega
Ascentis Peptide	Aeris WIDEPORE	Aeris PEPTIDE
Astec	Lux	—
BIOshell	Aeris WIDEPORE	Jupiter
Discovery Bio	Jupiter 300	Aeris WIDEPORE
Discovery HSF5	Luna PFP(2)	Kinetex F5
Discovery HSC18	Luna C18(2)	Kinetex C18
Discovery C18	Luna C18(2)	Kinetex C18
Discovery RP C16 Amide	Synergi Fusion-RP	Synergi Fusion-RP
Discovery (C18, C16)	Synergi Hydro-RP	Luna Omega
Proteomix	—	Clarity Oligo-WAX
Supelco ABZ, ABZ+	Luna C8(2)	Luna C18(2)
Supelco LC-18-T	Prodigy (3)	Luna C18(2)
Supelco LC-18-S	Prodigy (3)	Luna C18(2)
Supelco LC-F	Luna PFP(2)	Kinetex F5
Supelco LC-PAH	—	Synergi Hydro-RP
Supelcosil LC	PhenoSphere-NEXT	Synergi Hydro-RP

Column	Phenomenex Alternative*	Phenomenex Recommended Alternative**
Supelco / Sigma-Aldrich / MilliporeSigma (cont'd)		
Supelcogel	Rezex	Rezex
Supelcogel ODP-50	Asahipak ODP-50	Luna C18(2)
Supelcosil LC-DB	HyperClone BDS	Synergi Hydro-RP
Supelcosil LC-304/308/318	Jupiter 300	Aeris WIDEPORE
Supelcosil LC-NH ₂ -NP	—	Luna NH ₂
Supelcosil LC-PCN	Luna CN	Develosil CN-UG
Supelcosil LC-SAX	PhenoSphere SAX	Clarity SAX
Supelcosil LC-SCX	PhenoSphere SCX	Luna SCX
Titan	Luna Omega	Kinetex
Thermo Fisher Scientific / Thermo Scientific Dionex		
Acclaim 120	Luna	Kinetex
Acclaim 300	Jupiter	Aeris WIDEPORE
Acclaim HILIC-10	Luna HILIC	Kinetex HILIC
Acclaim PA	Synergi Fusion-RP	Luna Omega Polar C18
Acclaim PA 2	Synergi Fusion-RP	Luna Omega Polar C18
Acclaim OA	Synergi Hydro-RP	Synergi Fusion-RP
Acclaim Surfactant	—	Gemini
Accucore	Kinetex	Luna Omega PS C18
Accucore Vanquish C18+	Kinetex EVO	Luna Omega PS C18
AminoPac PA	—	Asahipak IEC/ES
Aquasil	Synergi Hydro-RP	Develosil ODS-MG
BetaBasic	Luna	Kinetex
BioBasic SEC	BioSep-SEC-S	Yarra
BioBasic IEX	Shodex IEC	Clarity Oligo-WAX
BioBasic RP	Jupiter 300	Aeris WIDEPORE
BETASIL	Prodigy (3)	Luna
BetaMax	Luna	Gemini
BETASIL Phenyl-Hexyl	Luna Phenyl-Hexyl	Kinetex Phenyl-Hexyl
Carbamate	Synergi Fusion-RP	Synergi Hydro-RP
CarboPac (MA, PA)	—	Rezex
Deltabond	Luna C18(2)	Synergi Max-RP
DNAPac	Asahipak IEC	Clarity Oligo-WAX
DNASwift	—	Clarity Oligo-RP
Fluophase	Luna PFP(2)	Kinetex F5
Hypercarb	—	Gemini
HyperREZ XP	Rezex	Rezex
Hypersil GOLD	Luna	Kinetex
Hypersil GOLD aQ C18	Luna Omega Polar C18	Synergi Hydro-RP
Hypersil Green	—	Synergi Hydro-RP
Hypersil	HyperClone	Synergi Max-RP
HyPURITY	Luna	Kinetex
HyPURITY ADVANCE	Synergi Fusion-RP	Luna Omega
HyPURITY AQUASTAR	Synergi Fusion-RP	Luna Omega
Ionpac AS series	STAR-ION A300	Shodex IC series
IonPac CS series	Shodex IC series	Hamilton PRP-X200
IonPac ICE AS series	Rezex ROA	Rezex ROA
IonPac IonSwift	—	Star-Ion
OmniPac	—	Luna SCX
Prism RP	Synergi Hydro-RP	Luna Omega Polar C18, PS C18
ProPac	—	Shodex IEC
Synchronis	Luna	Kinetex

* Alternative - This category indicates an alternative column which will likely give a similar selectivity.

** Recommended Alternative - This category indicates an alternative column which may yield somewhat different selectivity but may also lead to improved resolution.

HPLC Column Selection by Manufacturer

This selection is, neither in terms of manufacturers nor in terms of their products, a complete list, and the accuracy of the data is not guaranteed.

Column	Phenomenex Alternative*	Phenomenex Recommended Alternative**
Waters		
ACQUITY APC	—	Phenogel
ACQUITY BEH	Kinetex	Synergi 2.5 µm
ACQUITY CSH	Kinetex EVO C18	Kinetex XB-C18
ACQUITY Protein BEH SEC	Yarra	Yarra
ACQUITY UPC2	—	Kinetex
Atlantis	Synergi Fusion-RP	Synergi Hydro-RP
BioSuite IEX	Shodex IEC	—
BioSuite SEC	BioSep-SEC-S	Yarra
BioSuite RPC	—	Jupiter 300
Carbamate	—	Synergi Hydro-RP
Carbohydrate	PhenoSphere NH ₂	Luna NH ₂
CORTECS	Kinetex	Kinetex
Deltapak 100A	—	Luna
Deltapak 300A	Jupiter 300	Aeris WIDEPORE
GST	—	Luna HILIC
IC-pak	Hamilton PRP-X100	STAR-ION A300
µBondapak	Bondclone	Synergi Hydro-RP
µPorasil	Bondclone Silica	Luna Silica
µStyragel	Phenogel	Phenogel
Novapak 4 µm	—	Synergi Hydro-RP
OST	Clarity Oligo-RP	Clarity Oligo-MS
Protein-Pak IEC	Shodex IEC	—
Protein-Pak SW	BioSep-SEC-S	Yarra
PrST	Aeris WIDEPORE	Jupiter 3 µm C18
PST	Aeris PEPTIDE	Luna Omega PS C18
Resolve	PhenoSphere	Luna
Spherisorb	SphereClone	Synergi Hydro-RP
Sugar-pak	Rezex	Rezex
SunFire	Luna	Kinetex
Symmetry C18, C8	Luna C18(2), C8(2)	Synergi Max-RP
Symmetry Shield C18, C8	Synergi Fusion-RP	Synergi Hydro-RP
Styragel	Phenogel	Phenogel
UltraStyragel	Phenogel	Phenogel
Ultrahydrogel	PolySep-GFC-P	Shodex OHPak SB
XBridge	Gemini NX-C18	Kinetex EVO C18
XSelect	Luna Omega PS C18	Kinetex
XTerra MS	Gemini	Kinetex EVO C18
XTerra RP	Gemini	Kinetex EVO C18

* Alternative - This category indicates an alternative column which will likely give a similar selectivity.

** Recommended Alternative - This category indicates an alternative column which may yield somewhat different selectivity but may also lead to improved resolution.

HPLC Column Selection by Separation Mode

This table is to aid you in selecting the right column from Phenomenex for the separation mode you desire. For specific application notes or method development assistance please call your Phenomenex technical consultant.

Separation Mode	Page
Adsorption Chromatography	
Phenomenex Kinetex HILIC	240
Phenomenex Luna Silica	270
Chiral Chromatography	
Phenomenex Lux	293
Phenomenex Chirex	223
Shinwa Ultron ES	349
Shiseido Chiral CD-Ph	222
Sumika Sumichiral OA	337
Gel Filtration Chromatography	
Phenomenex Yarra SEC (silica)	350
Phenomenex BioSep SEC/GFC (silica)	220
Phenomenex PolySep GFC-P (polymer)	316
Asahipak GF and GS	219
Shodex GFC OHPak SB, Sugar KS, Protein KW	332
Gel Permeation Chromatography	
Phenomenex Phenogel	308
Shodex Asahipak GF	219
Shodex GPC, KF	332
Hydrophilic Interaction Chromatography	
Phenomenex Kinetex HILIC	240
Phenomenex Luna HILIC	270
Phenomenex Luna NH ₂	270
Hydrophobic Interaction Chromatography	
Shodex HIC	332
Ion-Exclusion Chromatography	
Phenomenex Rezex	318
Shodex RSpak, SUGAR	332
Ion-Exchange Chromatography	
Phenomenex Clarity Oligo-SAX	393
Phenomenex Luna SCX, Luna NH ₂	270
Phenomenex PhenoSphere SAX	314
Phenomenex Rezex	318
Macherey-Nagel Nucleosil SAX, SB	304
Shiseido Capcell UG-SCX	222
Shodex Asahipak ES	219
Shodex IEC	332
Shodex RSpak KC-811	332
Ion Chromatography	
Phenomenex STAR-ION A300	337
Hamilton PRP	233
Shodex IC	332
Ligand Exchange Chromatography	
Phenomenex Rezex	318
Shodex SUGAR	332
Multi-Mode Chromatography	
Phenomenex Luna SCX	270
Phenomenex Luna NH ₂	270
Shodex Asahipak GS	219

Separation Mode	Page
Normal Phase Chromatography	
Phenomenex Kinetex HILIC	240
Phenomenex Luna CN, NH ₂ , Silica	270
Phenomenex Prodigy	317
Merck KGaA LiChrospher	269
Nomura Chemical Develosil	225
Shodex Asahipak	219
Reversed Phase Chromatography	
Phenomenex Aeris	210
Phenomenex Bondclone	222
Phenomenex Clarity	393
Phenomenex Gemini	226
Phenomenex Gemini NX	226
Phenomenex HyperClone	234
Phenomenex Jupiter	237
Phenomenex Kinetex	240
Phenomenex Luna	270
Phenomenex Luna Omega	284
Phenomenex Onyx	305
Phenomenex PhenoSphere	314
Phenomenex PhenoSphere-NEXT	314
Phenomenex PolymerX	315
Phenomenex Prodigy	317
Phenomenex SphereClone	335
Phenomenex Synergi	338
Agilent Technologies ZORBAX StableBond, Rx, XDB	359
GL Sciences Inertsil	233
Hamilton PRP	233
Macherey-Nagel Nucleosil	304
Merck KGaA LiChrospher, Superspher	269
Nacalai Tesque Cosmosil	225
Nomura Chemical Develosil UG series	225
Shiseido Capcell SG, UG, MG, ACR, AQ	222
Shodex Asahipak ODP, C4P	219
Shodex RSpak	332
Waters Spherisorb	336

HPLC Column Selection by USP Listing

For each United States Pharmacopeia (USP) column specification, you will find listed the most suitable Phenomenex column.

It is widely understood that all HPLC packings are not alike, and no single column can perform a myriad of desired separations. HPLC packings differ in hydrophobicity, surface coverage, surface area, pore size and particle shape.

The USP does give chromatographers the flexibility to make adjustments to Monographs. As you can read below, column manufacturers or sources and materials stated in USP Monographs are only recommendations. Chromatographers can and should change and adapt the Monograph's specifications to yield the most satisfactory analytical results.

USP Column Classification	Recommended Phenomenex Column	Particle Shape	Page
L1 Octadecyl silane chemically bonded to porous or non-porous silica or ceramic microparticles, 1.5 to 10 µm in diameter, or a monolithic rod.	Gemini® NX-C18	Spherical	226
	Kinetex® C18	Core-Shell	240
	Kinetex EVO C18	Core-Shell	240
	Kinetex Polar C18	Core-Shell	240
	Kinetex XB-C18	Core-Shell	240
	Luna® C18(2)	Spherical	270
	Luna Omega C18	Spherical	284
	Luna Omega PS C18	Spherical	284
	Luna Omega Polar C18	Spherical	284
	Gemini C18	Spherical	226
	Synergi™ Hydro-RP	Spherical	338
	Synergi Fusion-RP	Spherical	338
	Onyx™ C18	Monolith	305
	Jupiter® C18	Spherical	237
	Clarity® Oligo-RP	Spherical	393
	Clarity Oligo-MS	Core-Shell	393
	Clarity Oligo-XT	Core-Shell	393
Aeris™ WIDEPORE XB-C18	Core-Shell	210	
Aeris PEPTIDE XB-C18	Core-Shell	210	
L2 Octadecyl silane chemically bonded to silica gel of a controlled surface porosity that has been bonded to a solid spherical core, 30 to 50 µm in diameter.			
L3 Porous silica particles, 1.5 to 10 µm in diameter, or a monolithic silica rod.	Kinetex HILIC	Core-Shell	240
	Luna Silica(2)	Spherical	270
	Onyx Silica	Monolith	305
L4 Silica gel of controlled surface porosity bonded to a solid spherical core, 30 to 50 µm in diameter.			
L5 Alumina of controlled surface porosity bonded to a solid spherical core, 30 to 50 µm in diameter.			
L6 Strong cation-exchange packing: sulfonated fluorocarbon polymer coated on a solid spherical core, 30 to 50 µm in diameter.			
L7 Octyl silane chemically bonded to totally or superficially porous silica particles, 1.5 to 10 µm in diameter, or a monolithic silica rod.	Kinetex C8	Core-Shell	240
	Luna C8(2)	Spherical	270
	Onyx C8	Monolith	305
	Aeris WIDEPORE XB-C8	Core-Shell	210
L8 An essentially monomolecular layer of aminopropyl-silane chemically bonded to totally porous silica gel support, 1.5 to 10 µm in diameter, or a monolithic silica rod.	Luna NH ₂	Spherical	270
L9 Irregular or spherical, totally porous silica gel having a chemically bonded, strongly acidic cation-exchange coating, 3 to 10 µm in diameter.	Luna SCX	Spherical	270
L10 Nitrile groups chemically bonded to porous silica particles, 1.5 to 10 µm in diameter, or a monolithic silica rod.	Luna CN	Spherical	270
L11 Phenyl groups chemically bonded to porous silica particles, 1.5 to 10 µm in diameter, or a monolithic silica rod.	Kinetex Biphenyl	Core-Shell	240
	Kinetex Phenyl-Hexyl	Core-Shell	240
	Synergi Polar-RP	Spherical	338
	Luna Phenyl-Hexyl	Spherical	270
	Gemini C6-Phenyl	Spherical	226
	Prodigy PH-3	Spherical	317
L12 Strong anion-exchange packing made by chemically bonding a quaternary amine to a solid silica spherical core, 30 to 50 µm in diameter.			
L13 Trimethylsilane chemically bonded to porous silica particles, 3 to 10 µm in diameter.	Develosil® TMS-UG (C1) 130 Å	Spherical	Inquire
L14 Silica gel having a chemically bonded, strongly basic quaternary ammonium anion-exchange coating, 5 to 10 µm in diameter.	PhenoSphere™ SAX	Spherical	314
L15 Hexyl silane chemically bonded to totally porous silica particles, 3 to 10 µm in diameter.	PhenoSphere C6	Spherical	314
L16 Dimethyl silane chemically bonded to porous silica particles, 5 to 10 µm in diameter.			
L17 Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the hydrogen form, 6 to 12 µm in diameter.	Rezex™ RHM-Monosaccharide	Spherical	318
	Rezex ROA-Organic Acid	Spherical	318
L18 Amino and cyano groups chemically bonded to porous silica particles, 3 to 10 µm in diameter.			
L19 Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the calcium form, 5 to 15 µm in diameter.	Rezex RCM-Monosaccharide	Spherical	318
	Rezex RCU-Sugar Alcohols	Spherical	318
L20 Dihydroxypropane groups chemically bonded to porous silica or hybrid particles, 1.5 to 10 µm in diameter, or a monolithic silica rod.	Luna HILIC	Spherical	270
	BioSep™-SEC-S	Spherical	220
	Yarra™ SEC	Spherical	350
L21 A rigid, spherical styrene-divinylbenzene copolymer, 3 to 30 µm in diameter.	PolymerX™ RP-1	Spherical	315
	Phenogel™ 100 Å	Spherical	308
L22 A cation-exchange resin made of porous polystyrene gel with sulfonic acid groups, 5 to 15 µm in diameter.	Rezex ROA-Organic Acid	Spherical	318
L23 An anion-exchange resin made of porous polymethacrylate or polyacrylate gel with quaternary ammonium groups, 7-12 µm in size.	Shodex® IEC QA-825	Spherical	332
L24 Polyvinylalcohol chemically bonded to porous silica particles, 5 µm in diameter.			
L25 Packing having the capacity to separate compounds with a MW range from 100 to 5000 daltons (as determined by polyethylene oxide), applied to neutral, anionic, and cationic water-soluble polymers. A polymethacrylate resin base, crosslinked with poly-hydroxylated ether (surface contained some residual carboxyl functional groups) was found suitable.	PolySep™-GFC-P2000	Spherical	316
	Shodex OHpak SB-802.5HQ	Spherical	332

HPLC Column Selection by USP Listing

USP Column Classification	Recommended Phenomenex Column	Particle Shape	Page	
L26	Butyl silane chemically bonded to totally porous silica particles, 1.5 to 10 µm in diameter.	Jupiter 300 C4 Aeris WIDEPORE C4	Spherical Core-Shell	237 210
L27	Porous silica particles, 30 to 50 µm in diameter.	Sepra Silica	Irregular	388
L28	A multifunctional support, which consists of a high purity, 100 Å, spherical silica substrate that has been bonded with anionic exchanger, amine functionality in addition to a conventional reversed phase C8 functionality.			
L29	Gamma alumina, reversed phase, low carbon percentage by weight, alumina-based polybutadiene spherical particles, 5 µm diameter with a pore volume of 80 Å.			
L30	Ethyl silane chemically bonded to a totally porous silica particle, 3 to 10 µm in diameter.			
L31	A hydroxide-selective, strong anion-exchange resin-quaternary amine bonded on latex particles attached to a core of 8.5 µm macroporous particles having a pore size of 2000 Å and consisting of ethylvinylbenzene cross-linked with 55% divinyl benzene.			
L32	A chiral ligand-exchange resin packing-L-proline copper complex covalently bonded to irregularly shaped silica particles, 5 to 10 µm in diameter.			
L33	Packing having the capacity to separate dextrans by molecular size over a range of 4,000 to 500,000 daltons. It is spherical, silica-based and processed to provide pH stability.	Yarra SEC-2000 BioSep-SEC-S2000 Yarra SEC-3000 BioSep-SEC-S3000	Spherical Spherical Spherical Spherical	350 220 350 220
L34	Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the lead form, 7 to 9 µm in diameter.	Rezex RPM-Monosaccharide	Spherical	318
L35	A zirconium-stabilized spherical silica packing with a hydrophilic (diol-type) molecular monolayer bonded phase having a pore size of 150 Å.	(BioSep-SEC-S2000 or Yarra SEC-2000 may be used)	Spherical Spherical	220 350
L36	3,5-dinitrobenzoyl derivative of L-phenylglycine covalently bonded to 5 µm aminopropyl silica.			
L37	Polymethacrylate gel packing having the capacity to separate proteins by molecular size over a range of 2,000 to 40,000 daltons.	PolySep-GFC-P3000 Shodex OHpak SB-803HQ	Spherical Spherical	316 332
L38	Methacrylate-based size-exclusion packing for water-soluble samples.	PolySep-GFC-P series Shodex OHpak SB-800HQ	Spherical Spherical	316 332
L39	Hydrophilic polyhydroxymethacrylate gel of totally porous spherical resin.	PolySep-GFC-P series Shodex OHpak SB-800HQ series Shodex RSpak DM-614	Spherical Spherical Spherical	316 332 332
L40	Cellulose tris-3,5-dimethylphenylcarbamate coated porous silica particles, 3 µm to 20 µm in diameter.	Lux Cellulose-1	Spherical	293
L41	Immobilized α-acid glycoprotein on spherical silica particles, 5 µm in diameter.			
L42	Octylsilane and octadecylsilane groups chemically bonded to porous silica particles, 5 µm in diameter.			
L43	Pentafluorophenyl groups chemically bonded to silica particles by a propyl spacer, 1.5 to 10 µm in diameter.	Kinetex F5 Luna PFP(2)	Core-Shell Spherical	240 270
L44	A multifunctional support, which consists of a high purity, 60 Å, spherical silica substrate that has been bonded with a cationic exchanger, sulfonic acid functionality in addition to a conventional reversed phase C8 functionality.			
L45	Beta cyclodextrin, R, S-hydroxypropyl ether derivative, bonded to porous silica particles, 3 to 10 µm in diameter	Shiseido Chiral CD-Ph	Spherical	Inquire
L46	Polystyrene/divinylbenzene substrate agglomerated with quaternary amine functionalized latex beads, about 9 to 11 µm in diameter.			
L47	High capacity anion-exchange microporous substrate, fully functionalized with a trimethylamine group, 8 µm in diameter.			
L48	Sulfonated, cross-linked polystyrene with an outer layer of submicron, porous, anion-exchange microbeads, 5 to 15 µm in diameter.			
L49	A reversed phase packing made by coating a thin layer of polybutadiene on to spherical porous zirconia particles, 3 to 10 µm in diameter.			
L50	Multifunction resin with reversed phase retention and strong anion-exchange functionalities. The resin consists of ethylvinylbenzene, 55% cross-linked with divinylbenzene copolymer, 3 to 15 µm in diameter, and a surface area of not less than 350 m ² /g. Substrate is coated with quaternary ammonium functionalized latex particles consisting of styrene cross-linked with divinylbenzene.			
L51	Amylose tris-3,5-dimethylphenylcarbamate-coated, porous, spherical, silica particles, 3 to 10 µm in diameter.	Lux Amylose-1	Spherical	293
L52	A strong cation-exchange resin made of porous silica with sulfopropyl groups, 1 to 10 µm in diameter.			
L53	Weak cation-exchange resin consisting of ethylvinylbenzene, 55% cross-linked with divinylbenzene copolymer, 3 to 15 µm diameter. Substrate is surface grafted with carboxylic acid and/or phosphoric acid functionalized monomers. Capacity not less than 500 µEq/column.			
L54	A size exclusion medium made of covalent bonding of dextran to highly cross-linked porous agarose beads, 5 to 15 µm in diameter.			
L55	A strong cation-exchange resin made of porous silica coated with polybutadiene-maleic acid copolymer, about 5 µm in diameter.			
L56	Propyl silane chemically bonded to totally porous silica particles, 3 to 10 µm in diameter.			
L57	A chiral-recognition protein, ovomucoid, chemically bonded to silica particles, about 5 µm in diameter, with a pore size of 120 Å.	Ultron ES-OVM	Spherical	349
L58	Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the sodium form, about 6 to 30 µm in diameter.	Rezex RNM-Carbohydrate	Spherical	318
L59	Size-exclusion separations of proteins (separation by molecular weight) over the range of 5 to 7000 kDa. Spherical (1.5 to 10 µm), silica or hybrid packing with a hydrophilic coating.	Yarra SEC-2000 BioSep-SEC-S2000 Yarra SEC-3000 BioSep-SEC-S3000	Spherical Spherical Spherical Spherical	350 220 350 220
L60	Spherical, porous silica gel, 10 µm or less in diameter, surface has been covalently modified with alkyl amide groups and endcapped.			
L61	Hydroxide-selective, strong anion-exchange resin consisting of a highly cross-linked core of 13 µm microporous particles, pore size less than 10 Å, and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene with a latex coating composed of 85 nm diameter microbeads bonded with alkanol quaternary ammonium ions (6%).			
L62	C30 silane bonded phase on a fully porous spherical silica, 3 to 15 µm in diameter.	Develosil Combi-RP Develosil RP-Aqueous Develosil RP-Aqueous-AR	Spherical Spherical Spherical	Inquire Inquire Inquire

HPLC Column Selection by USP Listing

USP Column Classification	Recommended Phenomenex Column	Particle Shape	Page
L63	Glycopeptide teicoplanin linked through multiple covalent bonds to a 100Å spherical silica.		
L64	Strongly basic anion-exchange resin consisting of 8% crosslinked styrene divinylbenzene copolymer with a quaternary ammonium group in the chloride form, 45 to 180 µm in diameter.		
L65	Strongly acidic cation-exchange resin consisting of 2% sulfonated crosslinked styrene divinylbenzene copolymer with a sulfonic acid group in the hydrogen form, 63 to 250 µm in diameter.		
L66	A crown ether coated on a 5 µm particle size silica gel substrate. The active site is (S)-18-crown-6-ether.		
L67	Porous vinyl alcohol copolymer with a C18 alkyl group attached to the hydroxyl group of the polymer, 2 to 10 µm in diameter.	Asahipak ODP-50	Spherical Inquire
L68	Spherical, porous silica, 10 µm or less in diameter, the surface of which has been covalently modified with alkyl amide groups and not endcapped.		
L69	Ethylvinylbenzene/divinylbenzene substrate agglomerated with quaternary amine functionalized 130 nm latex beads, about 6.5 µm in diameter.		
L70	Cellulose tris (phenyl carbamate) coated on 5 µm silica.		
L71	A rigid, spherical polymethacrylate 4 to 6 µm in diameter.	Shodex RSpak DE-413 Shodex RSpak DE-613	Spherical Spherical 332 332
L72	(S)-phenylglycine and 3,5-dinitroaniline urea linkage covalently bonded to silica.	Chirex 3012	Spherical 223
L73	A rigid, spherical polydivinylbenzene particle 5 to 10 µm in diameter.		
L74	A strong anion-exchange resin consisting of a highly cross-linked core of 7 µm macroporous particles having a 100Å average pore size and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene and an anion-exchange layer grafted to the surface, which is functionalized with alkyl quaternary ammonium ions.		
L75	A chiral-recognition protein, bovine serum albumin (BSA), chemically bonded to silica particles, about 7 µm in diameter, with a pore size of 300Å.		
L76	Silica-based weak cation-exchange material, 5 µm in diameter. Substrate is surface polymerized polybutadiene-maleic acid to provide carboxylic acid functionalities. Capacity not less than 29 µEq/column.		
L77	Weak cation-exchange resin consisting of ethylvinylbenzene, 55% cross-linked with divinylbenzene copolymer, 6 to 9 µm diameter. Substrate is surface grafted with carboxylic acid functionalized groups. Capacity not less than 500 µEq/column (4 mm x 25 cm).		
L78	A silane ligand that consists of both reversed phase (an alkyl chain longer than C8) and anion-exchange (primary, secondary, tertiary, or quaternary amino groups) functional groups chemically bonded to porous or non-porous or ceramic micro-particles, 1.0 to 50 µm in diameter or a monolithic rod.		
L79	A chiral-recognition protein, human serum albumin (HSA), chemically bonded to silica particles, about 5 µm in diameter.		
L80	Cellulose tris(4-methylbenzoate)-coated, porous, spherical, silica particles, 5 to 20 µm in diameter.	Lux Cellulose-3	Spherical 293
L81	A hydroxide-selective, strong anion-exchange resin consisting of a highly cross-linked core of 9 µm porous particles having a pore size of 2000Å units and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene with a latex coating composed of 70 nm diameter microbeads (6% crosslinked) bonded with alkanol quaternary ammonium ions.		
L82	Polyamine chemically bonded to cross-linked polyvinyl alcohol polymer, 4 - 5 µm in diameter	Asahipak NH ₂ -50	Spherical Inquire
L83	A hydroxide-selective, strong anion-exchange resin-quaternary amine bonded on latex particles attached to a core of 10.5 µm microporous particles having a pore size of 10Å and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene.		
L84	Weak cation-exchange resin consisting of ethylvinylbenzene, 55% cross-linked with divinylbenzene copolymer, 5 µm diameter. Substrate is surface grafted with carboxylic acid functionalized groups. Capacity not less than 8400 µEq column (5 mm x 25 cm).		
L85	A silane ligand that consists of both reversed phase (an alkyl chain longer than C8) and weak cation-exchange (carboxyl groups) functional groups chemically bonded to porous or non-porous particles, 1.0 to 50 µm in diameter.		
L86	Fused core particle with a highly polar ligand possessing 5 hydroxyl groups tethered to the silica gel outer layer, 1.5 to 5 µm in diameter.		
L87	Dodecyl silane chemically bonded to porous silica particles, 1.5 to 10 µm in diameter.	Synergi Max-RP	Spherical 338
L88	Glycopeptide vancomycin linked through multiple covalent bonds to 100 Å spherical silica.		
L89	Packing having the capacity to separate compounds with a molecular weight range from 100 - 3000 dalton (as determined by polyethylene oxide), applied to neutral and anionic water-soluble polymers. A polymethacrylate resin base, cross-linked with polyhydroxylate ether (surface contains some residual cationic functional groups).		
L90	Amylose tris-[(S)-alpha-methylbenzylcarbamate] coated on porous, spherical silica particles, 3 to 10 µm in diameter.		
L91	Strong anion-exchange resin consisting of monodisperse porous polystyrene/divinylbenzene beads coupled with quaternary amine. Bead size is 3 to 10 µm.		
L92	A strong anion-exchange resin consisting of a highly cross-linked core of 5-9 µm macroporous particles having a 100Å average pore size and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene and an anion-exchange layer grafted to the surface, which is functionalized with alkanol quaternary ammonium ions.		
L93	Cellulose tris (3,5-dimethylphenylcarbamate) reversed phase chiral stationary phase coated on 3 or 5 µm silica gel particles.	Lux Cellulose-1	Spherical 293
L94	A strong anion-exchange resin consisting of highly cross-linked 15 µm microporous particles functionalized with very low cross-linked latex (0.5%) to provide alkanol quaternary ammonium ion-exchange sites.		
L95	Highly polar alkyl ligand comprising five hydroxyl groups that are chemically bonded to totally porous or superficially porous silica, or a monolithic silica rod.		
L96	Alkyl chain, reversed phase bonded totally or superficially porous silica designed to retain hydrophilic and other polar compounds when using highly aqueous mobile phases, including 100% aqueous, 1.5 µm to 10 µm in diameter.	Kinetex Polar C18 Kinetex EVO C18 Luna Omega Polar C18 Luna Omega PS C18 Synergi Hydro-RP	Spherical Spherical Spherical Spherical Spherical 240 240 284 284 338
L97	Weak cation-exchange resin consisting of a highly cross-linked core of 5.5 µm porous particles having a pore size of 2000Å and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene. Substrate is surface grafted with carboxylic acid functionalized groups. Capacity not less than 2400 µEq/column (4 mm x 25 cm).		

HPLC Column Selection by USP Listing

USP Column Classification	Recommended Phenomenex Column	Particle Shape	Page
L98 Weak cation-exchange resin consisting of a highly cross-linked core of 8 µm microporous particles having an average pore size of 10 Å and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene. Substrate is surface grafted with carboxylic acid functionalized groups. Capacity not less than 46 µEq/column (4 mm x 5 cm).			
L99 Amylose tris-(3,5- dimethylphenylcarbamate), immobilized on porous, spherical, silica particles, 3 to 5 µm in diameter	Lux i-Amylose-1	Spherical	293
L100 A 55% cross-linked, microporous, hydrophobic resin core (9 µm microporous particles having a pore size of 10 Å) that consists of a bilayer of anion and cation-exchange latex. The first layer is fully sulfonated (140 nm) and the second layer is fully aminated (76 nm).			
L101 Cholesteryl groups chemically bonded to porous or non-porous silica or ceramic micro-particles, 1.5 to 10 µm in diameter, or a monolithic rod.			
L102 (Naproxen, (S,S)Whelk-O 1) 1-(3,5- dinitrobenzamido)-1,2,3,4- tetrahydrophenanthrene covalently bonded to porous spherical silica particles, 5 to 10 µm in diameter.			
L103 A hydroxide-selective, strong anion-exchange resin consisting of a highly cross-linked core of 7.5 µm porous particles having a pore size of 2000 Å and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene electrostatically bonded with hyperbranched alkanol quaternary ammonium ions.			
L104 Triazole groups chemically bonded to porous silica particles, 1.5 to 10 µm in diameter.			
L105 A strong anion-exchange resin consisting of a highly cross-linked 9 µm supermacroporous (2000 Å) particles functionalized with very low cross-linked latex (0.2%) to provide alkyl quaternary ammonium ion sites.			
L106 Weak cation-exchange resin consisting of ethylvinylbenzene, 55% cross-linked with divinylbenzene copolymer, 5-8 µm diameter, macroporous particles having an average pore size of 100 Å units. Substrate is surface grafted with carboxylic acid and phosphonic acid functional groups. Capacity not less than 2800 µEq/column (4 mm x 25 cm).			
L107 Cellulose tris(4-methylbenzoate)-coated porous spherical particles, 3 to 5 µm in diameter, for use with reversed phase mobile phases.	Lux Cellulose-3	Spherical	293
L108 A chiral-recognition protein, cellobiohydrolase (CBH), chemically bonded to silica particles, about 5 µm in diameter.			
L109 Spherical particles of porous graphitic carbon, 3 to 30 µm in diameter.			
L110 A strong anion-exchange resin consisting of a highly cross-linked 13 µm microporous (less than 10 Å) particles coated with very low cross-linked latex (0.5%) to provide alkanol quaternary ammonium ion-exchange sites.			
L111 Polyamine chemically bonded to porous spherical silica particles, 5 µm in diameter.			
L112 A hydroxide-selective, strong anion-exchange resin consisting of a highly cross-linked core of 8.5 µm porous particles having a pore size of 2000 Å units and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene with a latex coating composed of 65 nm diameter microbeads (5% cross-linked) bonded with alkanol quaternary ammonium ions.			
L113 A hydroxide-selective, strong anion-exchange resin consisting of a highly cross-linked core of 7.5 µm porous particles having a pore size of 2000 Å and consisting of ethylvinylbenzene cross-linked with 55% divinylbenzene with a latex coating composed of 65 nm diameter microbeads (5% crosslinked) bonded with alkanol quaternary ammonium ions.			
L114 Sulfobetaine graft-polymerized to totally or superficially porous silica, 1.5 to 10 µm in diameter, or a monolithic rod. Packing having densely bonded zwitterionic groups with 1:1 charge balance.			

HPLC Column Selection by Ph. Eur. Listing

The European Pharmacopoeia (*Ph. Eur.*), of the Council of Europe is a pharmacopoeia, listing a wide range of active substances and excipients used to prepare pharmaceutical products in Europe. It includes general and specific monographs that give quality standards for all the main medicines used in Europe. All medicines sold in the 38 Member States of the European Pharmacopoeia must comply with these quality standards so that consumers have a guarantee for products obtained from pharmacies and other legal suppliers.

It is widely understood that all HPLC packings are not alike, and no single column can perform a myriad of desired separations. HPLC packings differ in hydrophobicity, surface coverage, surface area, pore size, and particle shape.

For each European Pharmacopoeia (*Ph. Eur.*) description of the HPLC stationary phase, you will find listed the most suitable Phenomenex HPLC column. Other possible columns can also be used for these analyses. Please contact Phenomenex for your specific LC column needs.

Description According to Pharm. Eur. 9 4.1.1. Reagents 2017	Number	Recommended Phenomenex Column	Page
Silica gel Π -acceptor / Π -Donor for chiral separations (1-(3,5-dinitrobenzamide)-1,2,3,4-tetrahydrophenanthrene).	1160100		
Silica gel AD for chiral separation coated with Amylose tris (3,5-dimethylphenylcarbamate); 5 μ m.	1171700	Lux [®] Amylose-1	293
Silica gel AGP for chiral chromatography. (alpha 1-acid glycoprotein).	1148700		
Silica gel BC for chiral chromatography. (Beta-Cyclodextrin).	1161300	SumichiralOA-7000	Inquire
Silica gel for chiral separation, cellulose derivative coated with tris (3,5-dimethylphenylcarbamate), 5 μ m.	1110300	Lux Cellulose-1	293
Silica gel for chiral separation, L-Penicillamine coated silica gel.	1200050	SumichiralOA-5000L	Inquire
Silica gel for chiral chromatography, urea type derivative: (R)-phenylglycin and 3, 5-dinitroaniline; 5 μ m.	1181000	Chirex 3021	223
Silica gel for chiral separation, protein derivative of	1196300		
Silica gel for chromatography.	1076900	Kinetex HILIC Luna Silica(2)	240 270
Silica gel for chromatography, alkyl bonded for use with highly aqueous mobile phases.	1160200	Luna Omega Polar C18 Synergi [™] Hydro-RP Synergi Fusion-RP Gemini C18 Gemini NX-C18 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	284 338 338 226 226 240 240 240 240
Silica gel for chromatography, alkyl bonded for use with highly aqueous mobile phases, endcapped.	1176900	Luna Omega Polar C18 Synergi Hydro-RP Synergi Fusion-RP Gemini C18 Gemini NX-C18 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	284 338 338 226 226 240 240 240 240
Silica gel for chromatography, alkylsilyl, solid core, endcapped. Spherical silica particles containing a non-porous solid silica core surrounded by a thinner outer porous silica coating with alkylsilyl groups. To minimize an interaction with basic compounds it is carefully endcapped to cover most of the remaining silanol groups.	1194300	Kinetex C8 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	240 240 240 240 240
Silica gel for chromatography, amidohexadecylsilyl.	1170400		
Silica gel for chromatography, amidohexadecylsilyl, endcapped	1201100		
Silica gel for chromatography, aminoheptadecylsilyl.	1138400		
Silica gel for chromatography, aminopropylmethylsilyl.	1102400	SphereClone NH ₂ (Amino) PhenoSphere NH ₂ (Amino)	335 Inquire
Silica gel for chromatography, aminopropylsilyl.	1077000	SphereClone NH ₂ (Amino) PhenoSphere NH ₂ (Amino)	335 Inquire
Silica gel for chromatography, Amylose derivative of.	1109800	Lux Amylose-1 Lux Amylose-2	293 293
Silica gel for chromatography, butylsilyl. Spheroidal 300 Å; pore volume: 0.6 cm ³ /g; area: 80 m ² /g.	1076200	Aeris WIDEPORE C4	210
Silica gel for chromatography, butylsilyl, endcapped.	1170500	Aeris WIDEPORE C4 Jupiter 300 C4	210 237
Silica gel for chromatography compatible with 100% aqueous mobile phase, octadecylsilyl, endcapped.	1188400	Luna Omega Polar C18 Synergi Hydro-RP Synergi Fusion-RP Kinetex EVO C18 Kinetex Polar C18	284 338 338 240 240
Silica gel for chromatography, crown-ether.	1178000	SumichiralOA-8000	Inquire
Silica gel for chromatography, cyanosilyl.	1109900	Luna CN (Cyano) HyperClone CN (Cyano) PhenoSphere CN (Cyano)	270 234 314

HPLC Column Selection by Ph. Eur. Listing

Description According to Pharm. Eur. 9 4.1.1. Reagents 2017	Number	Recommended Phenomenex Column	Page
Silica gel for chromatography, cyanopropylsilyl, endcapped, base-deactivated.	1194200	Luna CN (Cyano)	270
Silica gel for chromatography, cyanopropylsilyl, endcapped.	1195000	Luna CN (Cyano)	270
Silica gel for chromatography, di-isobutyloctadecylsilyl.	1140000	Kinetex XB-C18 ZORBAX StableBond C18	240 359
Silica gel for chromatography, diisopropylcyanopropylsilyl.	1168100	ZORBAX StableBond CN	Inquire
Silica gel for chromatography, dimethyloctadecylsilyl. irregular; area: 300 m ² /g.	1115100	Bondclone C18	222
Silica gel for chromatography, diol dihydroxypropyl, 100 Å.	1110000	Luna HILIC	270
Silica gel for chromatography, dodecylsilyl, endcapped.	1179700	Synergi Max-RP	338
Silica gel for chromatography, hexadecylamidylsilyl with hexadecylcarboxamidopropyl dimethylsilyl groups; 5 µm.	1162500		
Silica gel for chromatography, hexadecylamidylsilyl, endcapped with hexadecylcarboxamidopropyl dimethylsilyl groups; 5 µm.	1172400		
Silica gel for chromatography, hexylsilyl.	1077100	SphereClone™ C6 PhenoSphere™ C6	335 Inquire
Silica gel for chromatography, hexylsilyl, endcapped.	1174400	SphereClone C6 PhenoSphere C6	335 Inquire
Silica gel for chromatography, human albumin coated.	1138500		
Silica gel for chromatography, hydrophilic surface has been modified to provide hydrophilic characteristics.	1077200	Luna® HILIC Kinetex® HILIC	270 240
Silica gel for chromatography, nitrile cyanopropylsilyl.	1077300	Luna CN (Cyano) HyperClone™ CN (Cyano) PhenoSphere CN (Cyano)	270 234 Inquire
Silica gel for chromatography, nitrile R1 chemically bonded nitrile groups.	1077400	Luna CN (Cyano) HyperClone CN (Cyano) PhenoSphere CN (Cyano)	270 234 Inquire
Silica gel for chromatography, nitrile R2 ultrapure silica (<20 ppm metal) with cyanopropylsilyl groups.	1119500	Luna CN (Cyano) HyperClone CN (Cyano) PhenoSphere CN (Cyano)	270 234 Inquire
Silica gel for chromatography, nitrile, endcapped with cyanopropylsilyl groups.	1174500	Luna CN (Cyano)	270
Silica gel for chromatography, 4-nitrophenylcarbamidesilyl. A very finely divided silica gel, chemically modified at the surface by bonding with 4-nitrophenylcarbamide groups.	1185200		
Silica gel for chromatography, octadecanoylamino propylsilyl amino propylsilyl groups which are acylated with octadecanoyl groups.	1115200		
Silica gel for chromatography, octadecylsilyl.	1077500	Luna C18(2) Luna Omega C18 Luna Omega PS C18 Luna Omega Polar C18 Synergi Hydro-RP Synergi Fusion-RP Gemini® C18 Gemini NX-C18 HyperClone C18 Kinetex® C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18 SphereClone C18 ODS(1) or (2)	270 284 284 284 338 338 226 226 234 240 240 240 240 240 335
Silica gel for chromatography, octadecylsilyl R1 ultrapure silica (<20 ppm metals), pore size and C-load are indicated in the method.	1110100	Luna C18(2) Luna Omega C18 Luna Omega PS C18 Luna Omega Polar C18 Synergi Hydro-RP Synergi Fusion-RP Gemini C18 Gemini NX-C18 Jupiter C18 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	270 284 284 284 338 338 226 226 237 240 240 240 240
Silica gel for chromatography, octadecylsilyl R2 ultrapure silica; 150 Å pore size; 20% C-load; optimized for the analysis of PAHs.	1115300	EnviroSep-PP Prodigy ODS-2	Inquire 317
Silica gel for chromatography, octadecylsilyl, base-deactivated pretreated before the bonding by careful washing and hydrolyzing most of the superficial siloxane bridges to minimize the interaction with basic components.	1077600	Luna C18(2) Luna Omega C18 Luna Omega PS C18 Luna Omega Polar C18 Gemini C18 Gemini NX-C18 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	270 284 284 284 226 226 240 240 240 240

HPLC Column Selection by Ph. Eur. Listing

Description According to Pharm. Eur. 9 4.1.1. Reagents 2017	Number	Recommended Phenomenex Column	Page
Silica gel for chromatography, octadecylsilyl, endcapped. To minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups.	1115400	Luna C18(2) Luna Omega C18 Luna Omega PS C18 Luna Omega Polar C18 Gemini C18 Gemini NX-C18 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	270 284 284 284 226 226 240 240 240 240
Silica gel for chromatography, octadecylsilyl, endcapped R1 ultrapure silica (<20 ppm metal), 100Å pore size; 19% C-load. To minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups.	1115401	Luna C18	270
Silica gel for chromatography, octadecylsilyl, endcapped, base-deactivated; pore size 100 Å; 16% C-load, pretreated before the bonding by careful washing and hydrolyzing most of the superficial siloxane bridges. To further minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups.	1108600	Luna C18(2) Prodigy DDS-3 Gemini C18 Gemini NX-C18	270 317 226 226
Silica gel for chromatography, octadecylsilyl, endcapped, base-deactivated R1; pretreated before the bonding by careful washing and hydrolyzing most of the superficial siloxane bridges. To further minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups.	1162600	Luna C18(2) Luna Omega C18 Luna Omega PS C18 Luna Omega Polar C18 Gemini C18 Gemini NX-C18 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	270 284 284 284 226 226 240 240 240 240
Silica gel for chromatography, octadecylsilyl, ethylene-bridged (hybrid material). Synthetic, spherical ethylene-bridged particles, containing both organic and inorganic (silica) components.	1190500	Kinetex EVO C18 Gemini NX-C18	240 226
Silica gel for chromatography, octadecylsilyl, extra-dense bonded, endcapped.	1188500	Luna® C18(2) Luna Omega C18 Luna Omega PS C18 Luna Omega Polar C18 Gemini C18 Gemini NX-C18 Kinetex C18 Kinetex EVO C18 Kinetex XB-C18 Kinetex Polar C18	270 284 284 284 226 226 240 240 240 240
Silica gel for chromatography, octadecylsilyl, monolithic.	1154500	Onyx™ C18	305
Silica gel for chromatography, octadecylsilyl, solid core, endcapped with spherical silica particles containing a non-porous solid silica core surrounded by a thin outer porous silica coating with octadecylsilyl groups. To minimize any interaction with basic compounds it is carefully endcapped to cover most of the remaining silanol groups.	1193900	Kinetex C18 Kinetex XB-C18 Kinetex EVO C18 Kinetex Polar C18 Aeris PEPTIDE XB-C18 Aeris WIDEPOR XB-C18	240 240 240 240 210 210
Silica gel for chromatography, octadecylsilyl, with polar embedded groups, endcapped; the particles are based on a mixture of silica chemically modified at the surface by the bonding of octadecylsilyl groups and silica chemically modified with a reagent providing a surface with chains having embedded polar groups.	1177900	Synergi™ Fusion-RP	338
Silica gel for chromatography, octadecylsilyl, with extended pH range, endcapped (resistant to bases up to pH 11)	1196700	Gemini C18 Gemini NX-C18 Kinetex EVO C18	226 226 240
Silica gel for chromatography, octadecylsilyl, with polar incorporated groups, endcapped; the particles are based on silica, chemically modified with a reagent providing a surface with chains having polar incorporated groups and terminating octadecyl groups.	1165100	Synergi Fusion-RP	338
Silica gel for chromatography, octadecylsilyl, endcapped. A very finely divided silica gel, chemically modified at the surface by bonding of octadecylphenylsilyl groups. To minimize any interaction with basic compounds it is carefully endcapped to cover most of the remaining silanol groups.	1199300		
Silica gel for chromatography, (hybrid, material), polar-embedded, octadecylsilyl, ethylene-bridged, endcapped. Synthetic, spherical ethylene-bridged hybrid particles, containing both inorganic (silica) and organic (organosiloxanes) components, chemically modified at the surface by bonding of polar embedded octadecylsilyl groups. To minimize any interaction with basic compounds it is carefully endcapped to cover most of the remaining silanol groups.	1200800		
Silica gel for chromatography, octylsilyl.	1077700	Kinetex C8 Luna C8(2) Prodigy C8 HyperClone C8 (MOS) SphereClone C8	240 270 317 234 335
Silica gel for chromatography, octylsilyl R1. Bonding of octylsilyl and methyl groups (double bonded phase).	1077701	Kinetex C8 Luna C8(2) Prodigy C8 HyperClone C8 (MOS) SphereClone C8	240 270 317 234 335
Silica gel for chromatography, octylsilyl R2 ultrapure silica (<20 ppm metal); pore size 100Å; C-load: 19%.	1077702		
Silica gel for chromatography, octylsilyl R3 ultrapure silica, bonding of octylsilyl groups and sterically protected with branched hydrocarbons at the silanes.	1155200	ZORBAX StableBond C8	359

HPLC Column Selection by Ph. Eur. Listing

Description According to Pharm. Eur. 9 4.1.1. Reagents 2017	Number	Recommended Phenomenex Column	Page
Silica gel for chromatography, octylsilyl, base-deactivated pretreated before the bonding by careful washing and hydrolyzing most of the superficial siloxane bridges to minimize the interaction with basic components.	1131600	Kinetex C8 Luna C8(2) Prodigy C8 HyperClone C8 (BDS)	240 270 317 234
Silica gel for chromatography, octylsilyl, endcapped. To minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups.	1119600	Kinetex C8 Luna C8(2) Prodigy C8 HyperClone C8 (BDS)	240 270 317 234
Silica gel for chromatography, octylsilyl, endcapped, base-deactivated pretreated before the bonding by careful washing and hydrolyzing most of the superficial siloxane bridges to minimize the interaction with basic components. To further minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanols.	1148800	Kinetex C8 Luna C8(2) Prodigy C8 HyperClone C8 (BDS)	240 270 317 234
Silica gel for chromatography, octylsilyl, with polar incorporated groups, endcapped; chains having polar incorporated groups and terminating octyl groups.	1152600		
Silica gel for chromatography, octylsilyl, extra-dense bonded, endcapped.	1200900	Luna C8(2) Kinetex C8	270 240
Silica gel for chromatography, oxypropionitrilsilyl	1184700		
Silica gel for chromatography, palmitamidopropylsilyl, endcapped bonding with palmitamidopropyl groups and endcapped with acetamidopropyl groups.	1161900		
Silica gel for chromatography, phenylhexylsilyl.	1153900	Kinetex Phenyl-Hexyl Luna Phenyl-Hexyl Gemini C6-Phenyl	240 270 226
Silica gel for chromatography, phenylhexylsilyl, endcapped. To minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups.	1170600	Kinetex Phenyl-Hexyl Luna Phenyl-Hexyl Gemini C6-Phenyl	240 270 226
Silica gel for chromatography, phenylhexylsilyl, solid core, endcapped. Silica gel with spherical silica particles containing a non-porous solid core surrounded by a thin outer porous silica coating with phenylhexylsilyl groups. To minimize any interaction with basic compounds it is carefully endcapped to cover most of the remaining silanol groups.	1198900	Kinetex Phenyl-Hexyl	240
Silica gel for chromatography, phenylsilyl.	1110200	Synergi Polar-RP Luna Phenyl-Hexyl Gemini C6-Phenyl Prodigy Phenyl-3 (PH3) Kinetex Biphenyl Kinetex Phenyl-Hexyl	338 270 226 317 240 240
Silica gel for chromatography, phenylsilyl, R1 spherical silica; pore size: 80 Å; surface area: 180 m ² /g; C-load: 5.5 %.	1075700	ZORBAX® StableBond Phenyl	359
Silica gel for chromatography, phenylsilyl, endcapped. To minimize any interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups.	1154900	Synergi™ Polar-RP Luna® Phenyl-Hexyl Gemini® C6-Phenyl Prodigy™ Phenyl-3 (PH3) Kinetex® Biphenyl Kinetex Phenyl-Hexyl	338 270 226 317 240 240
Silica gel for chromatography, phenylsilyl, endcapped, base-deactivated.	1197900	Synergi™ Polar-RP Luna Phenyl-Hexyl Gemini C6-Phenyl Prodigy Phenyl-3 (PH3) Kinetex Biphenyl Kinetex Phenyl-Hexyl	338 270 226 317 240 240
Silica gel for chromatography, (hybrid material), phenylsilyl, ethylene-bridged, endcapped. Synthetic, spherical ethylene-bridged hybrid particles containing both organic (organosiloxanes) and inorganic (silica) components, chemically modified at the surface by bonding of phenylsilyl groups. To minimize the interaction with basic compounds it's carefully endcapped to cover most of the remaining silanol groups..	1200700	Gemini C6-Phenyl	226
Silica gel for chromatography, propoxybenzene, endcapped.	1174600	Synergi Polar-RP	338
Silica gel for chromatography, propylsilyl.	1170700	ZORBAX® StableBond C3	Inquire
Silica gel for chromatography, strong anion-exchange bonding of quaternary ammonium groups; pH limit of use: 2 to 8.	1077800	PhenoSphere™ SAX	Inquire
Silica gel for chromatography, strong cation-exchange bonding of sulfonic acid groups.	1161400	Luna® SCX	270
Silica gel for chromatography, trimethylsilyl.	1115500	Develosil® TMS-UG (C1) Capcell Pak® C1 UG PhenoSphere C1	Inquire Inquire Inquire
Silica for size-exclusion chromatography. 10 µm silica with a very hydrophilic surface. Pore size average: 30 nm; pH stability 2 to 8; exclusion range for proteins: 1 x 10 ³ to 3 x 10 ⁵ ; 10 µm.	1077900	BioSep™-SEC-S3000	220
Silica gel OC for chiral separations. Coated with cellulose tris (phenylcarbamate); 5 µm.	1146800		
Silica gel OD for chiral separations.	1110300	Lux® Cellulose-1	293
Silica gel OJ for chiral separations. Coated with cellulose tris (4-methylbenzoate).	1179800	Lux Cellulose-3	293
Organosilica polymer, amorphous, octadecylsilyl. Synthetic, spherical hybrid particles containing both inorganic (silica) and organic (organosiloxanes) components, chemically modified at the surface by trifunctionally bonded octadecylsilyl groups.	1144200	Kinetex EVO C18 Gemini C18 Gemini NX-C18	240 226 226
Organosilica polymer, amorphous, octadecylsilyl, endcapped. Synthetic, spherical hybrid particles containing both inorganic (silica) and organic (organosiloxanes) components, chemically modified at the surface by trifunctionally bonded octadecylsilyl groups. To minimize any interaction with basic compounds, it is carefully endcapped to cover most of the remaining silanol groups.	1178600	Kinetex EVO C18 Gemini C18 Gemini NX-C18	240 226 226

HPLC Column Selection by Ph. Eur. Listing

Description According to Pharm. Eur. 9 4.1.1. Reagents 2017	Number	Recommended Phenomenex Column	Page
Organosilica polymer, amorphous, polar embedded, octadecylsilyl, endcapped. Synthetic, spherical hybrid particles containing both inorganic (silica) and organic (organosiloxanes) components, chemically modified at the surface by the bonding of polar embedded octadecylsilyl groups. To minimize any interaction with basic compounds, it is carefully endcapped to cover most of the remaining silanol groups.	1150600		
Organosilica polymer, amorphous, polar embedded propyl-2-phenylsilyl, endcapped. Synthetic, spherical hybrid particles containing both inorganic (silica) and organic (organosiloxanes) components, chemically modified at the surface by the bonding of polar embedded propyl-2-phenylsilyl groups. To minimize any interaction with basic compounds, it is carefully endcapped to cover most of the remaining silanol groups.	1178100		
Organosilica polymer for mass spectrometry, amorphous, octadecylsilyl, endcapped. Synthetic, spherical hybrid particles containing both inorganic (silica) and organic (organosiloxanes) components. To minimize any interaction with basic compounds, it is carefully endcapped to cover most of the remaining silanol groups.	1164900	Kinetex EVO C18 Gemini C18 Gemini NX-C18	240 226 226
Vinyl polymer for chromatography, amino alkyl. Spherical particles (5 µm) of a vinyl alcohol copolymer, bonding of amino alkyl groups.	1191500	Asahipak® NH ₂ -P	Inquire
Vinyl polymer for chromatography, octadecyl. Spherical particles (5 µm) of a vinyl alcohol copolymer, bonding of octadecyl groups on the hydroxyl groups.	1155400	Asahipak ODP-50	Inquire
Vinyl polymer for chromatography, octadecylsilyl. Spherical particles (5 µm) of a vinyl alcohol copolymer bonded to an octadecylsilane. C-load: 17 %.	1121600	Asahipak ODP-50	Inquire
Ion-exclusion resin for chromatography. A resin with sulfonic acid groups attached to a polymer lattice consisting of polystyrene cross-linked with divinylbenzene.	1131000	Rezex™ ROA-Organic Acid Rezex RHM-Monosaccharide	318 318
Cation-exchange resin, strong. Strong cation-exchange resin in protonated form with sulfonic acid groups attached to a polymer lattice consisting of polystyrene cross-linked with divinylbenzene.	1156800	Rezex ROA-Organic Acid Rezex RHM-Monosaccharide	318 318
Cation-exchange resin R1. A resin in protonated form with sulfonic acid groups attached to a polymer lattice consisting of polystyrene cross-linked with 8 % divinylbenzene. Available as spherical beads.	1016700	Rezex™ ROA-Organic Acid Rezex RHM-Monosaccharide	318 318
Cation-exchange resin R1. A resin in protonated form with sulfonic acid groups attached to a polymer lattice consisting of polystyrene cross-linked with 4 % divinylbenzene. Available as spherical beads.	1121900		
Cation-exchange resin R2. Resin containing strongly acidic propylsulfonic acid groups.	1195400		
Cation-exchange resin (Calcium form), strong. Resin in calcium form with sulfonic acid groups attached to a polymer lattice consisting of polystyrene cross-linked with 8 % divinylbenzene	1104600	Rezex RCM-Monosaccharide Rezex RCU-USP Sugar Alcohols	318 318
Cation-exchange resin (Sodium form), strong. Resin in sodium form with sulfonic acid groups attached to a polymer lattice consisting of polystyrene cross-linked with divinylbenzene.	1176100	Rezex RNM-Carbohydrate	318

If Aeris core-shell columns do not provide at least an equivalent separation as compared to a competing column of the same phase, return the column with the comparative data within 45 days for a FULL REFUND.


Core-Shell HPLC / UHPLC Columns for Proteins and Peptides

Ultra-High Resolution and Performance

Introducing Aeris, a specialized line of reversed phase core-shell HPLC / UHPLC columns, built exclusively for the ultra-high performance separation and analysis of proteins and peptides.

These columns can provide improved resolving power, selectivity, throughput, sensitivity, column lifetime, and method flexibility compared to other fully porous and core-shell columns typically used for bioseparations.

Aeris WIDEPORE

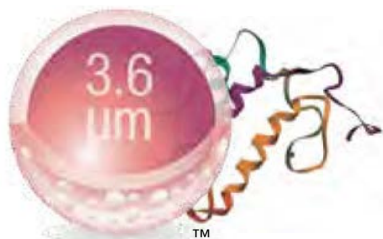

Large pore optimized for intact proteins and polypeptides

Aeris PEPTIDE



Small pore optimized for peptides and for peptide mapping

The precise architecture of Aeris core-shell particles provides dramatic leaps in performance in two important ways:

1 The thin, porous layer, or “shell”, decreases the diffusion path length, thus reducing the time it takes for biomolecules to adsorb/desorb into and out of the particle.

2 Expert manufacturing combined with tight packing specifications and high particle density reduces losses in efficiency and performance due to band broadening.


Aeris Core-Shell Particle

- High particle density helps create optimal bed structure which reduces band broadening effects of Eddy Diffusion
- Ultra-high performance on HPLC and UHPLC systems alike
- Reduced diffusion path improves efficiency



Fully Porous Particle

- Less homogenous bed structure leads to performance loss
- Ultra-high performance limited to sub-2µm particles on UHPLC systems
- Diffusion path limits efficiencies

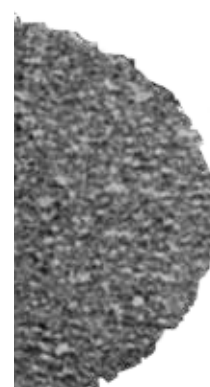

The result is:

- **3.6µm core-shell particles** that can perform like sub-2µm columns on both HPLC and UHPLC systems at a fraction of the pressure
- **5µm core-shell particles** allow scale up to preparative dimensions
- **1.7µm and 2.6µm core-shell particles** that can provide higher peak capacities compared to fully porous sub-2µm columns on UHPLC systems



To see our entire BioSeparations column and accessory portfolio, visit: www.phenomenex.com/biopharm

Selecting the Optimal Aeris Column for Your Applications

Aeris core-shell columns are designed for the separation of complex protein and peptide mixtures. Chromatographers can easily narrow down the column(s) that has a high probability of success for their separation by selecting from a variety of phase, pore size, and particle size options.

Aeris PEPTIDE

Recommended for the separation of low molecular weight peptides and for peptide mapping.

- **XB-C18 chemistry best suited for resolving peptides**
- **1.7 µm, 2.6 µm, and 3.6 µm particles for method development flexibility between HPLC and UHPLC systems**
- **5 µm particle for peptide purification**
- **Small pore optimized for peptide diffusion**


For increased resolving power, use a longer column, preferably a 250mm (or 150mm for the Aeris 1.7 µm XB-C18). Due to the lower backpressure of Aeris 3.6 µm, one can easily run 250mm columns on both HPLC and UHPLC systems, AND one can couple multiple 250mm columns together and run them inline for even better results. For maximum UHPLC resolution, the 150mm length Aeris 1.7 µm or 250mm length Aeris 2.6 µm columns are excellent choices.

Aeris WIDEPORE

Recommended for the separation of intact proteins and polypeptides.

- **XB-C18, XB-C8, and C4 phases for alternate selectivities**
- **3.6 µm particle for system flexibility**
- **Large pore optimized for fast protein adsorption/desorption**

Because of the reduced hydrophobicity compared to fully porous 300Å columns, one should start gradients with reduced organic concentrations compared to other columns to improve peak shape of polar proteins and peptides. Shallower gradients compared to other fully porous columns may be appropriate.

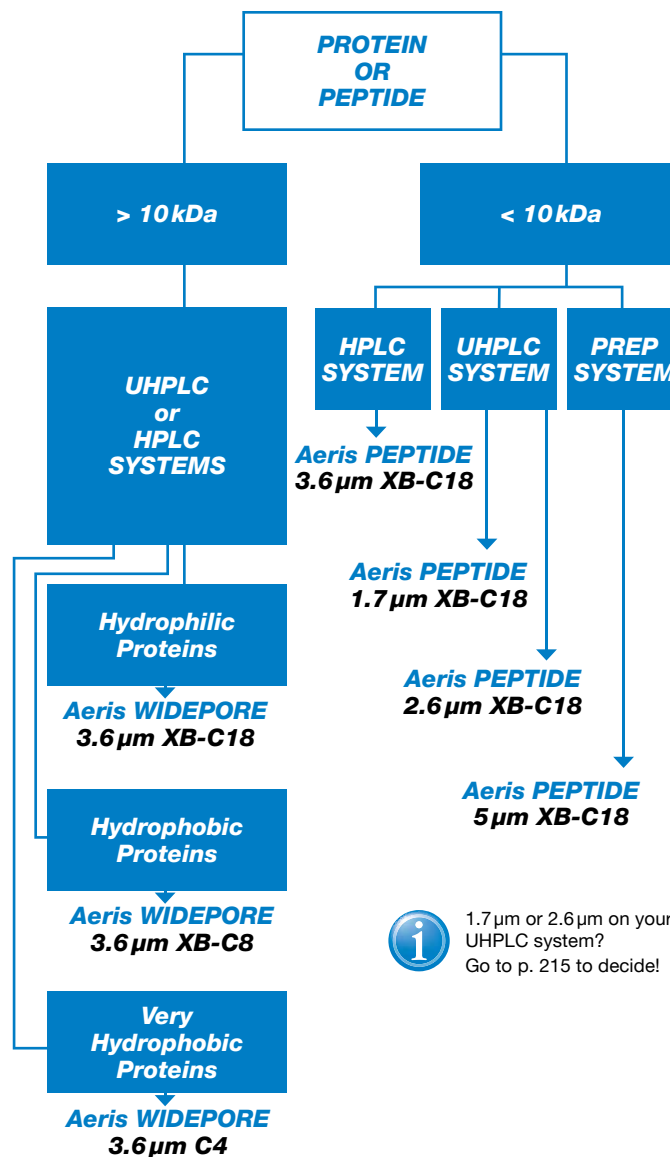

1.7 µm or 2.6 µm on your UHPLC system? Go to p. 215 to decide!

Material Characteristics

Packing Material	Total Particle Size (µm)	Porous Shell (µm)	Core Size (µm)	pH Stability	Temp Stability °C	Pressure Stability bar
Aeris WIDEPORE	3.6	0.2	3.2	1.5 - 9	90	600
Aeris PEPTIDE	1.7	0.22	1.25	1.5 - 9	90	1000
Aeris PEPTIDE	2.6	0.35	1.9	1.5 - 9	90	1000
Aeris PEPTIDE	3.6	0.5	2.6	1.5 - 9	90	600
Aeris PEPTIDE	5	0.6	3.8	1.5 - 9	90	600



Aeris WIDEPORE XB-C18 and Aeris PEPTIDE XB-C18 make a perfect pair for peptide mapping. See p. 215 for more details.


Aeris WIDEPORE Columns for Intact Protein and Polypeptide Separations

Aeris WIDEPORE columns are packed with 3.6µm core-shell particles that are specially engineered with a thin porous shell, large pores, and sterically protected XB surface chemistry to address the inherent separation challenges of proteins and peptides. This unique mix of features results in low backpressures, fast rates of diffusion, and excellent selectivity, generating exceptional chromatographic resolution on both HPLC and UHPLC systems.

Recommended for:


- Protein structural characterization
- Stability indicating assays
- Post-translational modification identification
- PEGylated proteins, antibodies, etc.
- Antibody-Drug Conjugates (ADCs)
- Biosimilars and biogenerics
- Impurity profiling
- Peptide mapping

3.6µm Core-Shell Particle

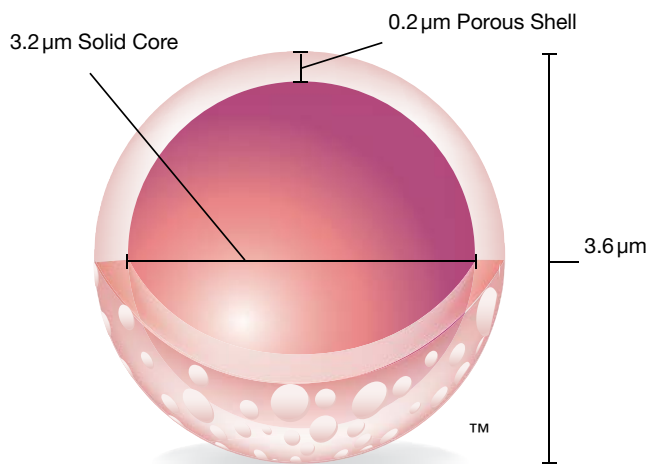


Easy Method Development with Three Selectivities

Aeris WIDEPORE 3.6µm Core-Shell Stationary Phases

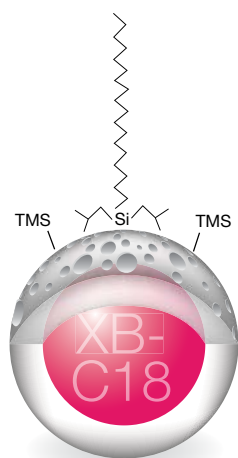


XB-C18
Maximum hydrophobicity
recommended for:

- Proteins
- Hydrophilic proteins
- PEGylated proteins
- High temperature separations
- Alternative selectivity for peptide mapping

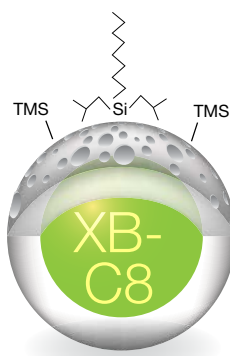

XB-C8
Moderate hydrophobicity
recommended for:

- Large proteins
- Moderately hydrophobic proteins
- Monoclonal antibodies
- Glycosylated proteins
- High temperature separations



C4
Low hydrophobicity
recommended for:


- Very large proteins
- Very hydrophobic proteins
- Membrane proteins
- Least retentive

Maximize Resolving Power with Unique Wide Pore 3.6 μm Core-Shell Particle

3.6 μm core-shell technology combined with inert surface chemistries and tight packing specifications results in Aeris WIDEPOR columns delivering exceptional resolving power at significantly lower backpressures. Chromatographers now have the ability to

generate higher quality data than typically produced by columns packed with fully porous particles for every protein analysis – on HPLC or UHPLC systems.

Performance Equivalent to Sub-2 μm Particle at Low Backpressure

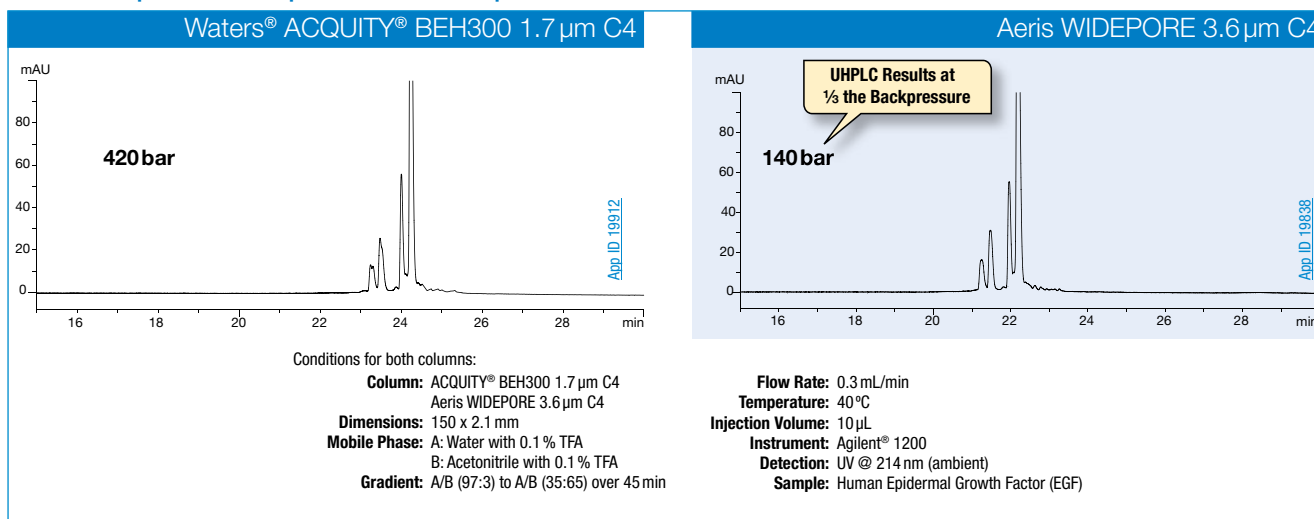


Achieve UHPLC Performance on HPLC Systems by Replacing 3 μm and 5 μm Columns

The innovative structure of 3.6 μm Aeris core-shell particles was specially designed to provide sub-2 μm performance at backpressures similar to fully porous 3 μm and 5 μm particles. Aeris columns can deliver increased resolution for existing protein and peptide separations performed on fully porous 3 μm and 5 μm columns,

using the same HPLC system!

Now you can have UHPLC performance on your HPLC system and experience better performance and method flexibility than ever before.

Upgrade Existing Methods on 3 μm and 5 μm Fully Porous Columns to Aeris Core-Shell Technology

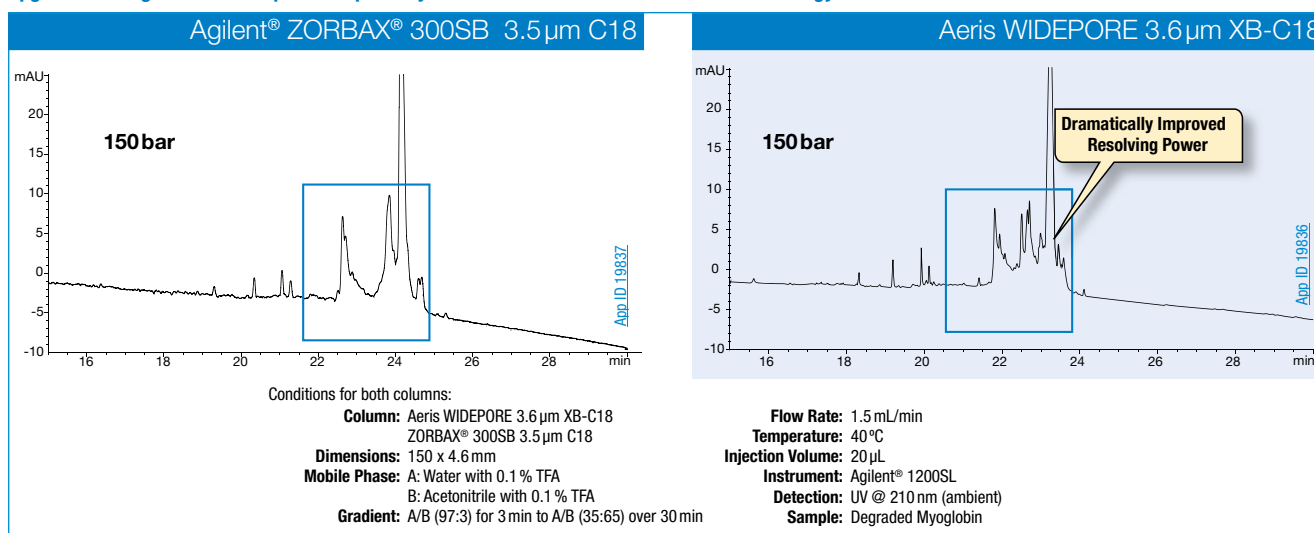


Studies were performed using new columns and, to the extent possible, identical experimental conditions were applied. Comparative separations may not be representative of all applications.

Long Column Lifetimes Under Extreme Method Conditions

Aeris columns provide temperature stability up to 90°C, and pH stability from 1.5 - 9, giving ample flexibility for method development and excellent column lifetime.

Over 1,000 Injections at 90°C

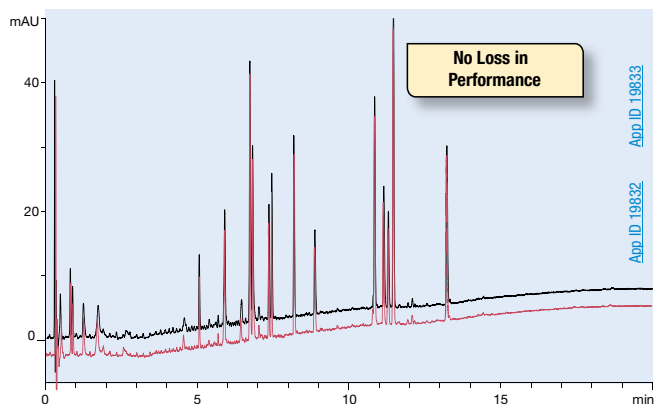

Column: Aeris WIDEPORE 3.6µm XB-C18
Dimensions: 50 x 2.1 mm
Part No.: [00B-4482-AN](#)
Guard Cartridge: [AJ0-8948](#)
Guard Holder: [AJ0-9000](#), SecurityGuard ULTRA Holder for UHPLC Columns 2.1 to 4.6 mm ID
Mobile Phase: A: Water with 0.1% TFA
 B: Acetonitrile with 0.1% TFA
Gradient: A/B (97:3) for 3 min, then to A/B (35:65) over 20 min
Flow Rate: 0.3 mL/min
Temperature: 90°C
Injection Volume: 10 µL
Detection: UV @ 214 nm (ambient)


Filter: [AF0-8108-52](#)
 Phenex-PES 28 mm Syringe Filters 0.45 µm, Non-Sterile Luer/Slip
Vial: [ARO-9925-13](#)
 Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: Apomyoglobin Digest

App ID: 19833

Low Column Bleed for Amplified Mass Spec (MS) Sensitivity

Aeris columns show no significant phase bleed under LC/MS conditions, making them very suitable for protein and peptide analysis. Chemists can be assured accurate, dependable, and consistent results, time and time again.

Virtually No LC/MS Bleed

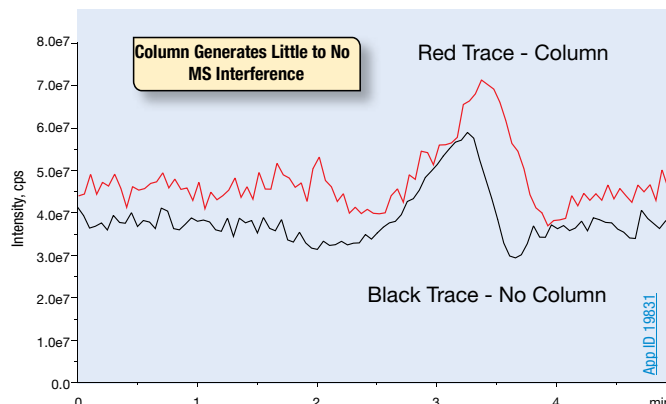

Column: Aeris WIDEPORE 3.6µm XB-C18
Dimensions: 50 x 2.1 mm
Part No.: [00B-4482-AN](#)
Guard Cartridge: [AJ0-8948](#)
Guard Holder: [AJ0-9000](#), SecurityGuard ULTRA Holder for UHPLC Columns 2.1 to 4.6 mm ID
Mobile Phase: A: Water with 0.1% Formic Acid
 B: Acetonitrile with 0.1% Formic Acid
Gradient: A/B (95:5) for 2.5 min, to A/B (5:95) hold for 0.5 min, then re-equilibrate
Flow Rate: 0.5 mL/min
Temperature: 25°C
Detection: MS (SCIEX API 4000™)



Filter: [AF0-8108-52](#)
 Phenex-PES 28 mm Syringe Filters 0.45 µm, Non-Sterile Luer/Slip
Vial: [ARO-9925-13](#)
 Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: Blank

App ID: 19831

Minimize Adsorption and Maximize Recoveries for Accurate Results

Aeris phase chemistries and bonding technology create a highly inert surface, leading to greatly reduced irreversible adsorption, higher recoveries, and sharper, narrower peaks, providing high quality and accurate results for each consecutive analysis.

Maximize Recoveries of Hydrophobic Proteins

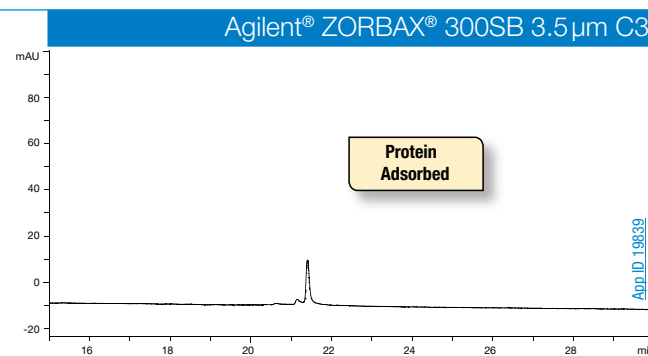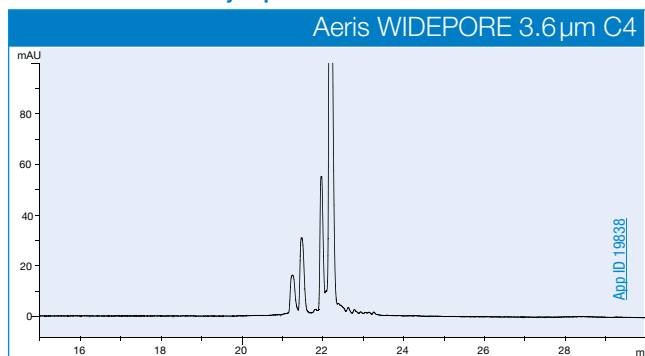

Conditions for both columns:
Column: Aeris WIDEPORE 3.6µm C4
 ZORBAX® 300SB 3.5µm C3
Dimensions: 150 x 2.1 mm
Mobile Phase: A: Water with 0.1% TFA
 B: Acetonitrile with 0.1% TFA
Gradient: A/B (97:3) to A/B (35:65) over 45 min

Flow Rate: 0.3 mL/min
Temperature: 40°C
Injection Volume: 20 µL
Instrument: Agilent® 1200
Detection: UV @ 214 nm (ambient)
Sample: Human Epidermal Growth Factor

Studies were performed using new columns and, to the extent possible, identical experimental conditions were applied. Comparative separations may not be representative of all applications

Aeris PEPTIDE Columns for Peptide and Peptide Mapping Separations





Based on core-shell particle technology, Aeris PEPTIDE particles are designed with small pores, inert XB-C18 surface chemistry, and three different particle sizes (3.6 μm, 2.6 μm, and 1.7 μm) to meet the resolution demands of chromatographers performing complex peptide and peptide map separations on HPLC and/or UHPLC systems.

Aeris PEPTIDE columns are built for the following:

- Synthetic peptide impurity analysis
- Peptide mapping
- Identifying protein modifications
Glycosylation, Substitution, and Truncation
- Analyzing post-translational modifications
Deamidation, Oxidation, and Deletions

Select the Most Suitable Aeris PEPTIDE Column to Achieve Your Separation Goals

The family of Aeris PEPTIDE XB-C18 columns is designed to provide versatility for the development of peptide separation methods. Depending on your resolution, throughput goals, and pressure capabilities of your system, you can choose from three particle sizes with unique performance attributes, as well as several column lengths to select the most suitable column for seamless method development and excellent results.

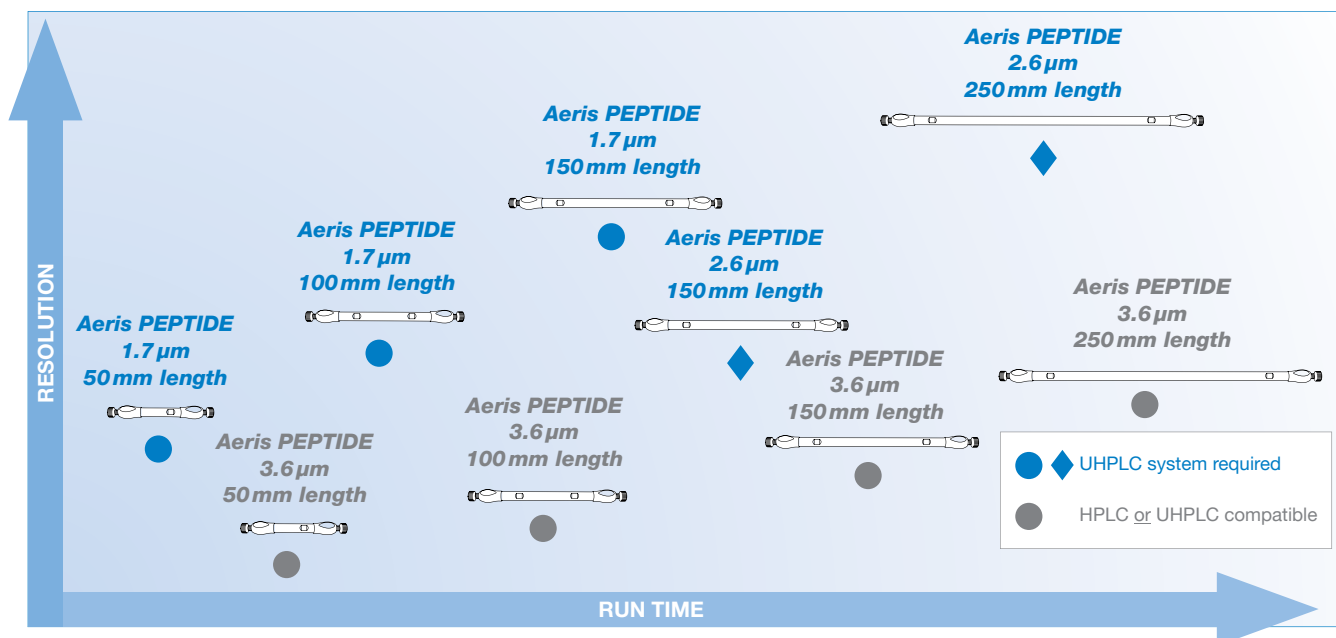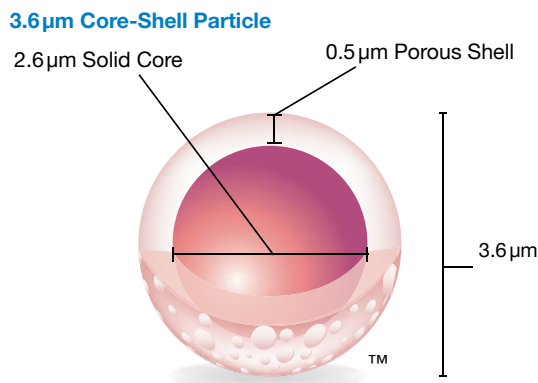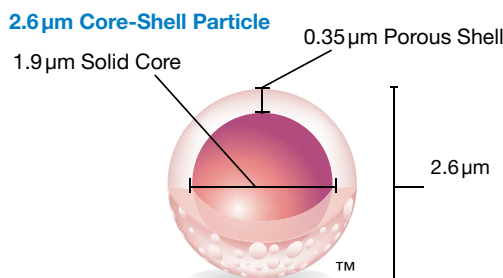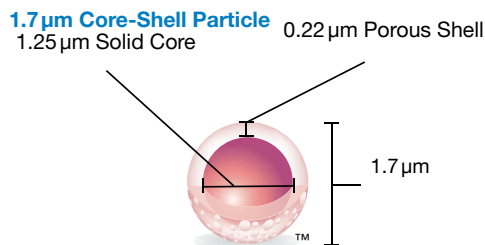


Ultra-High Resolving Power on UHPLC Systems with Aeris PEPTIDE 2.6 μm Columns of 250 mm Length

The Aeris PEPTIDE 2.6 μm core-shell particle was designed with one purpose in mind: to enhance the separation and maximize the peak count of complex peptide maps on UHPLC systems. Because the 2.6 μm core-shell particle reduces backpressure on UHPLC

systems while maintaining similar efficiencies to sub-2 μm fully porous particles, longer columns can be used to further maximize the separation power while still being well within the backpressure constraints of the instrumentation.


Increase UHPLC Performance with Aeris PEPTIDE 2.6 mm Columns

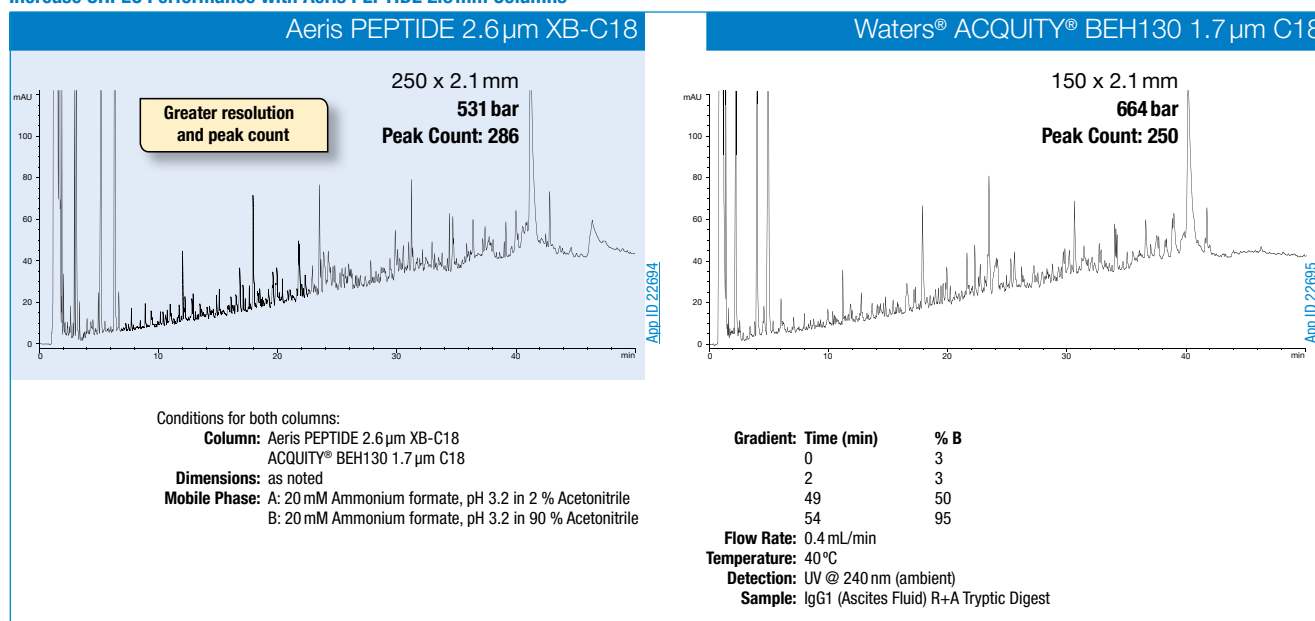

Maximize Separation Power on HPLC Systems with Longer Aeris PEPTIDE 3.6 μm Columns

For applications like peptide separations and peptide mapping where resolution is the primary goal, the lower backpressure of Aeris PEPTIDE 3.6 μm core-shell columns allow one to use longer


columns for higher resolving power resulting in increased separation of closely eluting peptides. Use longer (or coupled) 3.6 μm columns on UHPLC and HPLC systems to resolve critical peaks.

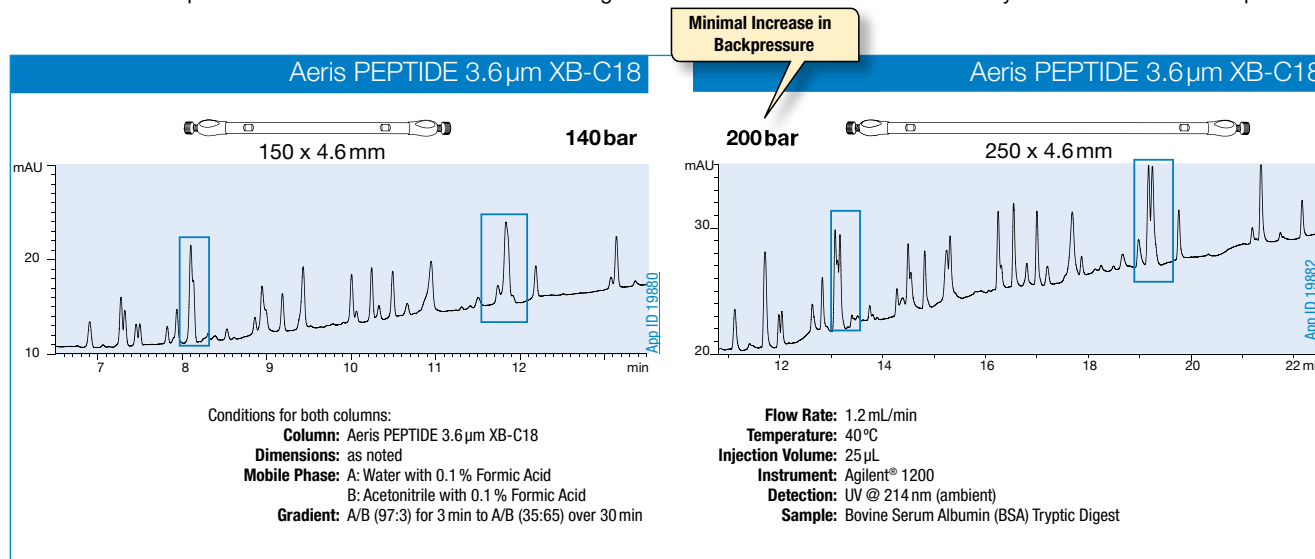

Studies were performed using new columns and, to the extent possible, identical experimental conditions were applied. Comparative separations may not be representative of all applications.


Seamless Scalability of Peptide Separations from HPLC/UHPLC to PREP

The addition of Aeris PEPTIDE 5 µm makes it possible for small-scale peptide purification in 10mm ID semi-prep and 21.2mm ID Axia™ packed prep formats. Aeris PEPTIDE is fully scalable in retention and selectivity with its 4 unique particle sizes (1.7 µm, 2.6 µm, 3.6 µm, and 5 µm) for easy transfer from HPLC and UHPLC methods to preparative applications.

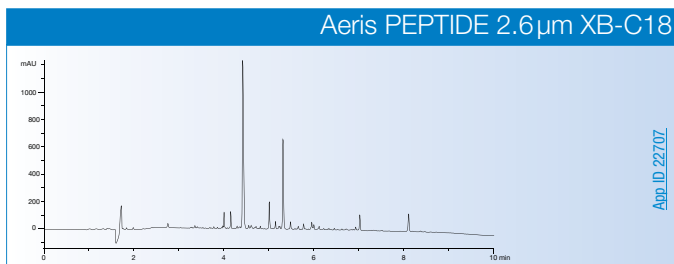


Analytical method

Column: Aeris PEPTIDE 2.6 µm XB-C18
Dimensions: 150 x 4.6 mm
Part No.: [00F-4505-E0](#)
Injection Volume: 10 µL
Flow Rate: 1 mL/min
Sample: Crude peptide mix

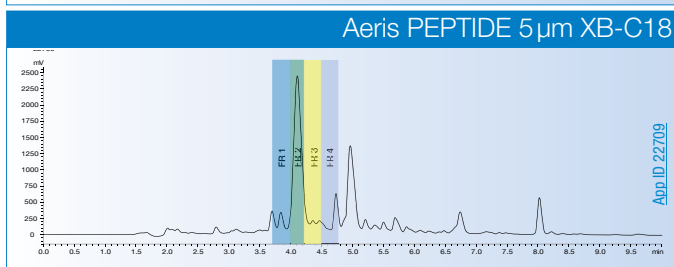

Preparative scale-up and fraction collection

Column: Aeris PEPTIDE 5 µm XB-C18 Axia Packed
Dimensions: 150 x 21.2 mm
Part No.: [00F-4632-PO-AX](#)
Injection Volume: 1 mL
Flow Rate: 20 mL/min
Sample: Crude peptide mix

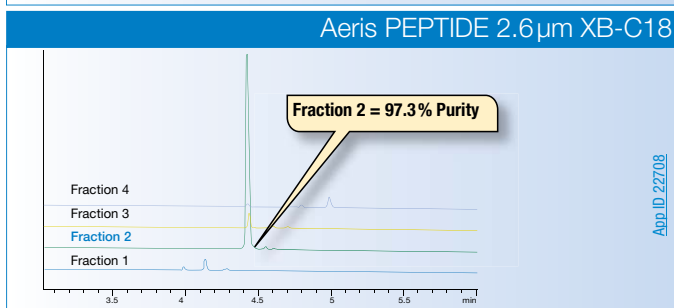

Analytical fraction analysis

Column: Aeris PEPTIDE 2.6 µm XB-C18
Dimensions: 150 x 4.6 mm
Part No.: [00F-4505-E0](#)
Injection Volume: 10 µL
Flow Rate: 1 mL/min
Sample: Purified Fractions





Conditions for all separations (except as noted):

Mobile Phase: A: 0.1% TFA in Water
 B: 0.1% TFA in Acetonitrile
Gradient: Linear 85:15 (A/B) to 5:95 (A/B) over 10 minutes
Temperature: Ambient
Detection: UV @ 210 nm

Increased Efficiency of Axia Packing Technology

Expect sharper peaks and higher loadability due to the high efficiencies achieved with Aeris PEPTIDE 5 µm XB-C18 Axia packed prep compared to traditionally packed Waters® XBridge® 5 µm C18 Prep OBD™.

Maximize Recoveries of Hydrophobic Proteins

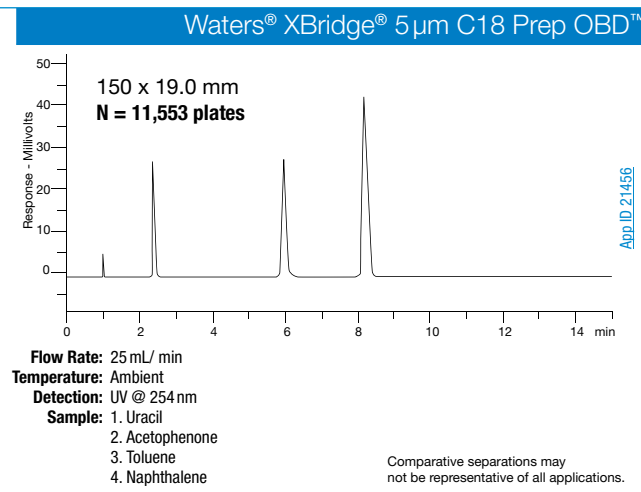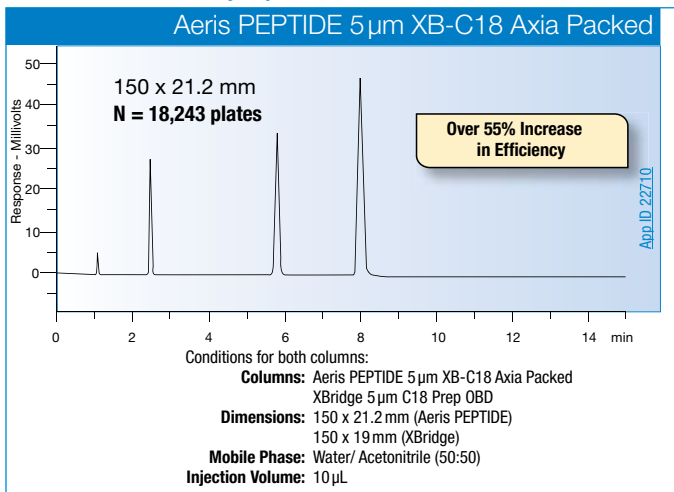

Aeris™ Core-Shell LC Columns for Proteins & Peptides

guarantee

If Aeris core-shell columns do not provide at least an equivalent separation as compared to a competing column of the same phase, return the column with the comparative data within 45 days for a FULL REFUND.

Ordering Information

Aeris PEPTIDE 1.7 µm Minibore Columns (mm)				SecurityGuard™ ULTRA Cartridges*
Phase	50 x 2.1	100 x 2.1	150 x 2.1	3/pk
XB-C18	00B-4506-AN	00D-4506-AN	00F-4506-AN	AJ0-8948

for 2.1 mm ID

Aeris PEPTIDE 2.6 µm Minibore Columns (mm)				SecurityGuard ULTRA Cartridges*	
Phase	50 x 2.1	100 x 2.1	150 x 2.1	250 x 2.1	3/pk
XB-C18	00B-4505-AN	00D-4505-AN	00F-4505-AN	00G-4505-AN	AJ0-8948

for 2.1 mm ID

Aeris PEPTIDE 2.6 µm MidBore™ and Analytical Columns (mm)			SecurityGuard ULTRA Cartridges*		
Phase	150 x 3.0	150 x 4.6	250 x 4.6	3/pk	3/pk
XB-C18	00F-4505-Y0	00F-4505-E0	00G-4505-E0	AJ0-8947	AJ0-8946

for 3.0 mm ID

for 4.6 mm ID

Aeris PEPTIDE 3.6 µm Minibore Columns (mm)				SecurityGuard ULTRA Cartridges*	
Phase	50 x 2.1	100 x 2.1	150 x 2.1	250 x 2.1	3/pk
XB-C18	00B-4507-AN	00D-4507-AN	00F-4507-AN	00G-4507-AN	AJ0-8948

for 2.1 mm ID

Aeris PEPTIDE 3.6 µm Analytical Columns (mm)				SecurityGuard ULTRA Cartridges*	
Phase	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	3/pk
XB-C18	00B-4507-E0	00D-4507-E0	00F-4507-E0	00G-4507-E0	AJ0-8946

for 4.6 mm ID

Aeris PEPTIDE 5 µm Analytical Scout and Semi-Prep Columns (mm)				SecurityGuard ULTRA Cartridges*	SecurityGuard SemiPrep Cartridges**	
Phase	150 x 4.6	250 x 4.6	150 x 10.0	250 x 10.0	3/pk	10 x 10
XB-C18	00F-4632-E0	00G-4632-E0	00F-4632-N0	00G-4632-N0	AJ0-8946	AJ0-9317

for 4.6 mm ID

for 10 mm ID

Aeris PEPTIDE 5 µm Axia™ Packed Preparative Columns (mm)		SecurityGuard PREP Cartridges†	
Phase	150 x 21.2	250 x 21.2	15 x 21.2
XB-C18	00F-4632-P0-AX	00G-4632-P0-AX	AJ0-9318

for 21.2 mm ID

Aeris WIDEPORE 3.6 µm Minibore Columns (mm)				SecurityGuard™ ULTRA Cartridges*	
Phases	50 x 2.1	100 x 2.1	150 x 2.1	250 x 2.1	3/pk
XB-C18	00B-4482-AN	00D-4482-AN	00F-4482-AN	00G-4482-AN	AJ0-8783
XB-C8	00B-4481-AN	00D-4481-AN	00F-4481-AN	00G-4481-AN	AJ0-8785
C4	00B-4486-AN	00D-4486-AN	00F-4486-AN	00G-4486-AN	AJ0-8899

for 2.1 mm ID

Aeris WIDEPORE 3.6 µm Analytical Columns (mm)			SecurityGuard ULTRA Cartridges*	
Phases	100 x 4.6	150 x 4.6	250 x 4.6	3/pk
XB-C18	00D-4482-E0	00F-4482-E0	00G-4482-E0	AJ0-8769
XB-C8	00D-4481-E0	00F-4481-E0	00G-4481-E0	AJ0-8771
C4	00D-4486-E0	00F-4486-E0	00G-4486-E0	AJ0-8901

for 4.6 mm ID



SecurityGuard ULTRA
Holder with cartridge



Cartridge Holder

*SecurityGuard ULTRA Cartridges require holder, Part No.: [AJ0-9000](#)

**SemiPREP SecurityGuard Cartridges require holder, Part No.: [AJ0-9281](#)

†PREP SecurityGuard Cartridges require holder, Part No.: [AJ0-8223](#)



For more about SecurityGuard ULTRA, see p. 331
For Core-Shell Performance Enhancement Kit, see p. 411



For HPLC Column Performance Check Standards, see pp. 414-415

A C18 Column with Polar Endcapping

Use Synergi Hydro-RP, an Improved Alternative to Aqua 125 Å

See p. 338

Material Characteristics

Packing Material	Particle Shape/Size (µm)	Pore Size (Å)	Pore Volume (mL/g)	Surface Area (m ² /g)	Carbon Load %	Calculated Bonded Phase Coverage (µmole/m ²)	End Capping
AQUA C18	Spher. 3, 5	125	1.05	320	15	N/A	Proprietary
AQUA C18	Spher. 5	200	1.15	215	11	N/A	Proprietary

125 Å Aqua C18 Column

Aqua's polar endcapping produces a surface chemistry that is well suited for the analysis of small peptides. This chemistry...

- makes it an excellent column for smaller, basic peptides
- allows for faster column equilibration in gradient analyses
- ensures a surface that can be "wetted" with aqueous trifluoroacetic acid (TFA)

200 Å Aqua C18 Column

- Increased pore size for enhanced diffusion of large pharmaceuticals and biomolecules
- Reduced surface area for faster analyses and greater sample throughput

Ordering Information

3 µm Minibore, Analytical, LC-MS and CombiChem Columns (mm)						SecurityGuard™ Cartridges (mm)	
Phases	50 x 2.0	75 x 2.0	150 x 2.0	100 x 4.6	150 x 4.6	4 x 2.0*	4 x 3.0*
C18 125 Å	00B-4311-B0	00C-4311-B0	00F-4311-B0	00D-4311-E0	00F-4311-E0	AJ0-7510 /10pk	AJ0-7511 /10pk
						for ID: 2.0–3.0 mm	3.2–8.0 mm

5 µm Minibore, MidBore™ and LC-MS Columns (mm)						SecurityGuard™ Cartridges (mm)
Phases	50 x 2.0	150 x 2.0	250 x 2.0	150 x 3.0	250 x 3.0	4 x 2.0*
C18 125 Å	00B-4299-B0	00F-4299-B0	00G-4299-B0	00F-4299-Y0	00G-4299-Y0	AJ0-7510 /10pk
C18 200 Å	—	00F-4331-B0	—	—	—	AJ0-7510 /10pk
						for ID: 2.0–3.0 mm

5 µm Analytical, CombiChem, SemiPrep and Preparative Columns (mm)					SecurityGuard™ Cartridges (mm)	
Phases	50 x 4.6	150 x 4.6	250 x 4.6	250 x 10	4 x 3.0*	10 x 10*
C18 125 Å	00B-4299-E0	00F-4299-E0	00G-4299-E0	00G-4299-N0	AJ0-7511 /10pk	AJ0-7512 /3pk
C18 200 Å	—	00F-4331-E0	00G-4331-E0	—	AJ0-7511	AJ0-7512
					for ID: 3.2–8.0 mm	9–16 mm



For SecurityGuard Cartridge Holders and Cartridges, see p. 326

*SecurityGuard Analytical Cartridges require holder, Part No.: [KJ0-4282](#)
 †SemiPrep SecurityGuard Cartridges require holder, Part No.: [AJ0-7220](#)

Asahipak®

By Showa Denko K.K.

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/asahipak

Aqueous Size Exclusion (SEC)/Gel Filtration (GFC) for Protein and Peptide Analysis

Gel Filtration Chromatography is used to analyze and/or characterize proteins, peptides, and other biomolecules; including antibodies, immunoglobulins, protein complexes, protein aggregates, and desalting. BioSep GFC columns offer many important benefits for your separation needs.


Low MW Proteins and Peptides on BioSep-SEC-s2000

BioSep-SEC-s2000 columns are used for peptide therapeutics, small proteins, PEGylated peptides, and small PEGylated proteins, as well as biogeneric aggregate applications.

PEGylated β -Lactoglobulin A (N-Terminal PEG 20 kDa)

Column: BioSep-SEC-s2000
Dimensions: 300 x 7.8 mm
Part No.: [00H-2145-K0](#)
Guard Cartridge: [AJ0-4487](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 100 mM Sodium Phosphate pH 6.8
Flow Rate: 1 mL/min
Temperature: Ambient
Detection: UV @ 220 nm

Filter: [AF0-8108-52](#), Phenex-PES 28 mm Syringe Filters 0.45 μ m, Non-Sterile, Luer/Slip
Vial: [ARO-9925-13](#), Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: 1. 2 PEG Modified Complex
 2. PEGylated β -Lactoglobulin
 3. β -Lactoglobulin
 4. PEG Reagent

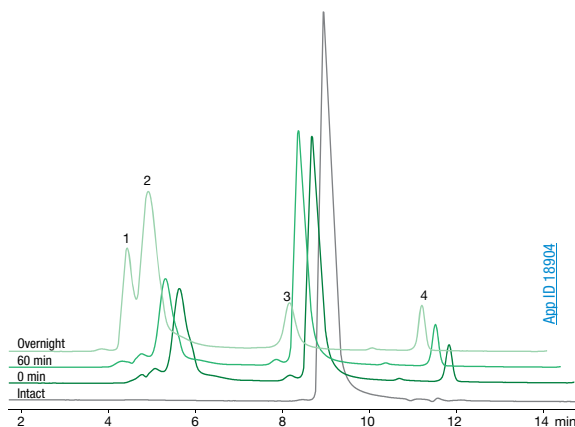


Medium MW Proteins on BioSep-SEC-s3000

BioSep-SEC-s3000 columns are great for medium to large MW proteins, serum proteins, immunoglobulins, and aggregate applications.

Murine IgG1 Aggregates

Column: BioSep-SEC-s3000
Dimensions: 300 x 7.8 mm
Part No.: [00H-2146-K0](#)
Guard Cartridge: [AJ0-4488](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 50 mM Sodium Phosphate pH 6.8, 300 mM Sodium Chloride
Flow Rate: 1 mL/min
Temperature: Ambient
Detection: UV @ 220 nm

Filter: [AF0-8108-52](#), Phenex-PES 28 mm Syringe Filters 0.45 μ m, Non-Sterile, Luer/Slip
Vial: [ARO-9925-13](#), Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: 1. HMW aggregates
 2. IgG1 dimer 1
 3. IgG1 dimer 2
 4. IgG Monomer
 5. Low MW impurity
 6. Void Volume Peak

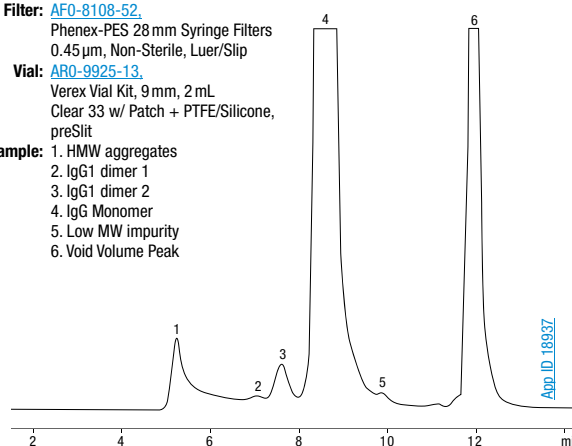


Large MW Proteins on BioSep-SEC-s4000

BioSep-SEC-s4000 is capable of resolving large MW proteins and PEGylated IgG applications.

High MW Protein Mixture

Column: BioSep-SEC-s4000
Dimensions: 300 x 7.8 mm
Part No.: [00H-2147-K0](#)
Guard Cartridge: [AJ0-4489](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 100 mM Sodium Phosphate pH 7.0, 300 mM Sodium Chloride
Flow Rate: 1 mL/min
Temperature: Ambient
Detection: UV @ 214 nm

Filter: [AF0-8108-52](#), Phenex-PES 28 mm Syringe Filters 0.45 μ m, Non-Sterile, Luer/Slip
Vial: [ARO-9925-13](#), Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: 1. HMW impurity
 2. IgM 900 kDa
 3. Thyroglobulin 669 kDa
 4. IgA 380 kDa
 5. β -Amylase 200 kDa
 6. BSA 66 kDa
 7. Ribonuclease A 13.7 kDa
 8. Uridine 244 Da

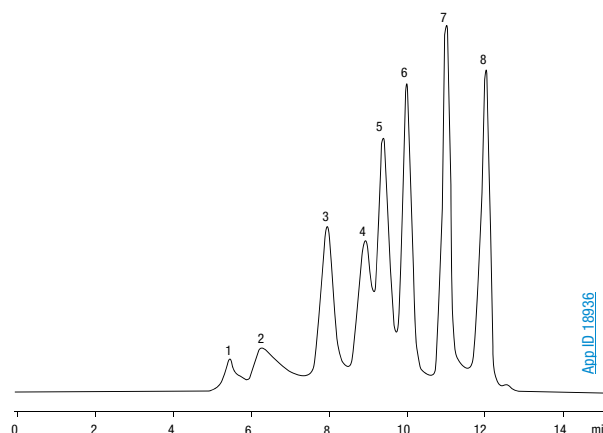

- Global support and availability in over 100 countries
- 3 batches available for validation
- For increased resolution and efficiencies, try Yarra SEC/GFC columns

If BioSep analytical columns do not provide you with at least an equivalent separation as any other GFC column of similar porosity, type and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Technical Data and Specifications

	BioSep- 0	BioSep- 0	BioSep- 0
Resin Type	Silica	Silica	Silica
Particle Size (µm)	5	5	5
Pore Size (Å)	145	290	500
Exclusion Range in Daltons for Proteins:			
Native	1,000 - 300,000	5,000 - 700,000	15,000 - 1,500,000
0.5% SDS	200 - 75,000	5,000 - 100,000	15,000 - 500,000
6 M GdnHCl	500 - 100,000	1,000 - 150,000	5,000 - 700,000
pH Range	2.5 - 7.5	2.5 - 7.5	2.5 - 7.5
Maximum Backpressure (psi)	1,500	1,500	1,500
Typical Backpressure (psi)	800	800	700
Efficiency (minimum number theoretical plates 300 x 7.8 mm)	30,000	30,000	25,000
Maximum Flow Rate	This is a function of pressure. Columns can withstand up to 1,500 psi, but avoid sudden pressure changes.		
Column Hardware	Standard: 316 stainless steel column with stainless steel frits. Titanium frits available.		
Maximum Temp.	50 °C		
Maximum Salt Conc.	1 M		
Denaturants	0.5% SDS, 6 M Guanidine HCl, or 8 M urea		
Regeneration	After exposure to denaturants, wash with water overnight.		
Max. Organic Modifier	Up to 100% CH ₃ CN, 10% DMSO or 500 mM β-mercaptoethanol.		
Cleaning Procedure	General protein removal: wash with 30 mL of 0.1 M NaH ₂ PO ₄ , pH 3.0. Hydrophobic protein removal: use acetonitrile gradient. Strongly adsorbed proteins: wash with 30 mL of 6 M Guanidine thiocyanate or 10% DMSO.		
Storage	Overnight storage: run mobile phase at 0.2 mL/minute. Prolonged storage: use 0.05% Na ₂ S ₂ O ₃ in H ₂ O or 20% methanol in H ₂ O.		
Column Protection	Use of a SecurityGuard is recommended to prolong column lifetime.		

Cross Reference Chart

Phenomenex BioSep Phases	TSKgel®	Shodex®	Sepax	Bio-Rad®	Waters® BioSuite™	ZORBAX®
SEC-s2000	G2000SW G2000SW _{XL}	PROTEIN KW-802.5	SRT®-100* SRT®-150	Bio-Sil® SEC 125	BioSuite™ 125	GF-250
SEC-s3000	G3000SW G3000SW _{XL}	PROTEIN KW-803	SRT®-300	Bio-Sil® SEC 250	BioSuite™ 250	GF-450
SEC-s4000	G4000SW G4000SW _{XL}	PROTEIN KW-804	SRT®-500**	Bio-Sil® SEC 400	BioSuite™ 450**	

** Only up to 1,500,000 MW

* Only above 1,000 MW

Ordering Information

Columns (mm)	Narrow Bore			Analytical			SecurityGuard™ Cartridges (mm)
	300 x 4.6	300 x 7.8	600 x 7.8				4 x 3.0*
BioSep-SEC-s2000	00H-2145-E0	00H-2145-K0	00K-2145-K0				AJ0-4487
BioSep-SEC-s3000	00H-2146-E0	00H-2146-K0	00K-2146-K0				AJ0-4488
BioSep-SEC-s4000	00H-2147-E0	00H-2147-K0	00K-2147-K0				AJ0-4489

*SecurityGuard Analytical cartridges require holder, Part No.: [KJ0-4282](#)

for ID: 4.6-7.8 mm



Guard Columns (mm)	Narrow Bore	Express	Analytical
Phases	30 x 4.6	35 x 7.8	75 x 7.8
BioSep-SEC-s2000	03A-2145-E0	03Q-2145-K0	03C-2145-K0
BioSep-SEC-s3000	03A-2146-E0	03Q-2146-K0	03C-2146-K0
BioSep-SEC-s4000	—	03Q-2147-K0	03C-2147-K0

Aqueous SEC 1 Column Check Standard

(for BioSep-SEC-S and other protein SEC columns)

Part No.: [AL0-3042](#)

Unit quantity: Dry; reconstituted to 2 mL

Contains: Bovine thyroglobulin; Human gamma globulin (contains IgA and IgG); Ovalbumin; Myoglobin; Uridine (reconstitute with 1 mL of 100 mM Sodium phosphate pH 6.8)

Diluent: 100 mM Sodium phosphate pH 6.8

Storage: Add 0.1% Na₂S₂O₃ to the solution and refrigerate

Test Conditions

Mobile phase: 100 mM Sodium phosphate, pH 6.8

Flow rate: 1.0 mL/min for a 300 x 7.8 mm column

Injection volume: 10 µL

Detection: UV @ 280 nm



For ultra-high resolution aqueous SEC, see Yarra on p. 350.



For Column Heater, see p. 408.



Other column dimensions available upon request.

Guaranteed Replacement to μ Bondapak®

- Highly reproducible
- Long column life
- Mimics performance of Waters® μ Bondapak®

Phenomenex Bondclone columns have been developed to provide chromatographic behavior that mimics that of Waters μ Bondapak columns. For comparative applications, please contact your local Phenomenex representative.

Bondclone Silica Physical Properties

Nominal Particle Size	BET Surface Area	Pore Volume*	Pore Size**
10 μ m	296.0 m ² /g	1.1 cc/g	148.7 Å

*Single point total pore volume.
 **Average pore diameter (4V/A by BET).
 Data provided by an independent laboratory.

If Bondclone analytical columns do not provide you with at least equivalent separations to a μ Bondapak column of the same phase, particle size and dimension, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information and Cross-Reference Chart

Waters				Phenomenex	SecurityGuard™ Cartridges (mm)
Description (mm)	Part No.	Part No.	Description (mm)		4 x 3.0
μ Bondapak C18 300 x 3.9	WAT027324	00H-2117-CO	Bondclone C18 300 x 3.9	AJQ-4287	/ 10pk
μ Bondapak C18 150 x 3.9	WAT086684	00F-2117-CO	Bondclone C18 150 x 3.9	AJQ-4287	
—	—	00G-2117-E0	Bondclone C18 250 x 4.6	AJQ-4287	
μ Bondapak C18 Radial-Pak Cartridge 100 x 8	WAT085721	00D-2117-LO	Bondclone C18 100 x 8 (S.S. Column)	AJQ-4287	
μ Bondapak Phenyl 300 x 3.9	WAT027198	00H-3129-CO	Bondclone Phenyl [†] 300 x 3.9	AJQ-4351	
—	—	00H-3127-CO	Bondclone CN 300 x 3.9	AJQ-4305	
μ Bondapak NH ₂ 300 x 3.9	WAT084040	00H-3128-CO	Bondclone NH ₂ 300 x 3.9	AJQ-4302	
μ Porasil Silica 300 x 3.9	WAT02 7477	00H-2119-CO	Bondclone Silica 300 x 3.9	AJQ-4348	

[†]Bondclone phenyl phase uses a different silica than other phases in the Bondclone series.

for ID: 3.2-8.0 mm

SecurityGuard™ Analytical Cartridges require universal holder Part No.: [KJQ-4282](#)

Guard Column

Size (mm)	C18
Conventional Guard Column 30 x 3.9	03A-2117-CO

Capcell Pak®

By Shiseido Co., Ltd.


- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/capcellpak

Chiral CD-Ph

By Shiseido Co., Ltd.

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/chiralcd

- High enantioselectivity
- Fast run times
- Rugged, long-lived columns
- Easy scale-up to preparative
- Allow direct/indirect resolution of enantiomeric amines, amino acids, hydroxy acids, alcohols, carboxylic acids, ketones, ethers, and esters

 Hundreds of applications demonstrate the performance of Chirex phases for a multitude of pharmaceutical and agrochemical compounds. For a complete list, please contact your Phenomenex technical consultant.

Which Chirex Stationary Phase?

Stationary phase selection depends on presence/absence of chemical groupings in the chiral molecule.

Chirex Column Selection Guide

Presence of Chemical Groupings in Chiral Molecule							Recommended Columns:	
Class	Aromatic	-N-	-COOH	-OH	Other	Comment	First Choice	Second Choice
Group 1	Y	Y	Y			Aromatic α -amino acids, α -hydroxy acids	3126	3001
Group 2	Y	Y		Y			3022 or 3020	3014
Group 3	Y	Y			Y		3014 or 3020	3022
Group 4	Y		Y				3010	3001
Group 5	Y			Y			3001 or 3014	3020 or 3022
Group 6	Y				Y		3001	3019 or 3020
Group 7		Y	Y			Aliphatic α -amino acids, α -hydroxy acids and their derivatives	3126	
Group 8				Y			3126	3010
Group 9					Y		3014	3019 or 3020
Group 10					Y	Asymmetric other than carbon. Chiral center at N,S,P,B, etc	3014	3010

Ordering Information


5 μ m Starter Columns (mm)				
Phase	Chirex Phase Description	Bond Type	Linkage Type	50 x 4.6
3010	(S)-VAL and DNAn	Covalent	Urea	00B-3010-E0
3011	(S)-LEU and DNAn	Covalent	Urea	00B-3011-E0
3014	(S)-VAL and (R)-NEA	Covalent	Urea	00B-3014-E0
3020	(S)-LEU and (R)-NEA	Covalent	Urea	00B-3020-E0
3126	(D)-Penicillamine	Ion-Metal	Lig Exchange	00B-3126-E0
3012	(R)-PGLY and DNAn	Covalent	Urea	00B-3012-E0


5 μ m Analytical and Guard Columns (mm)					Analytical			Guards
Phase	Chirex Phase Description	Bond Type	Linkage Type	150 x 2.0	150 x 4.6	250 x 4.6	30 x 4.6	
3001	(R)-PGLY and DNB	Covalent	Amide	—	00F-3001-E0	00G-3001-E0	—	
3011	(S)-LEU and DNAn	Covalent	Urea	—	—	00G-3011-E0	—	
3012	(R)-PGLY and DNAn	Covalent	Urea	—	—	00G-3012-E0	—	
3014	(S)-VAL and (R)-NEA	Covalent	Urea	—	—	00G-3014-E0	—	
3019	(S)-LEU and (S)-NEA	Covalent	Urea	—	—	00G-3019-E0	—	
3020	(S)-LEU and (R)-NEA	Covalent	Urea	—	00F-3020-E0	00G-3020-E0	—	
3022	(S)-ICA and (R)-NEA	Covalent	Urea	—	00F-3022-E0	00G-3022-E0	—	
3126	(D)-Penicillamine	Ion-Metal	Lig Ex	00F-3126-B0	00F-3126-E0	00G-3126-E0	03A-3126-E0	

Chiral separations are extremely important to the pharmaceutical and biotechnology industries, as well as most other areas of natural products chemistry. Optically active therapeutic drugs require selective and sensitive techniques. Government regulations also continue to spur and require the development of rapid, accurate and reproducible methods for the analysis and purification of enantiomeric compounds.

The challenge is to provide selective yet versatile HPLC columns for both trace analysis and the purification of bulk drug.

Phenomenex meets these challenges with Chirex brand HPLC columns. Chirex is available in 10 different stationary phases. These chemically rugged, versatile columns are used for the direct and indirect resolution of enantiomeric amines, alcohols, carboxylic acids, hydroxy acids, amino acids, ketones, lactones, ethers, esters, and other biologically active compounds.

 Preparative Columns and Bulk Media are available in 15 and 30 μ m particle sizes. Call for information on pricing and availability. Detailed notes on Care and Use, as well as performance testing, are provided with each column.

 For Chiral Column Performance Check Standards, see p. 415.

Chiral HPLC of Amino Acids

- Pirkle-concept and Ligand Exchange type columns
- High enantioselectivity
- Excellent efficiency

Chirex HPLC columns are an excellent choice for underivatized and derivatized amino acids.

Separations of Amino Acid Derivatives

Compound	Chirex Phase	Separation Factor (α)	App ID No.
t-BOC-Derivatives (Butyloxycarbonyl)			
t-BOC-Leucine	3012	1.09	14064
t-BOC-Phenylalanine	3012	1.09	13784
t-BOC-Valine	3012	1.10	14063
N-FMOC Derivatives (9-Fluorenylmethoxycarbonyl)			
N-FMOC-Leucine	3011	1.20	13800
N-FMOC-Phenylalanine	3011	1.10	13796
N-FMOC-Valine	3011	1.12	13798
Z-Derivatives (Benzyloxycarbonyl)			
Z-Alanine	3011	1.16	13729
Z-Asparagine	3010	1.12	13760
Z-Leucine	3011	1.17	13731
Z-Norvaline	3011	1.13	13755
Z-Phenylalanine	3012	1.08	13762
Z-Serine	3011	1.09	13758
Z-Valine	3011	1.13	13753
N-Acetyl Derivatives			
N-Acetylalanine	3126	1.17	14052
N-Acetylleucine	3126	1.39	14058
N-Acetylmethionine	3126	1.27	13728
N-Acetylvaline	3126	1.50	14055
N-Formyl Derivatives			
N-Formylvaline	3126	1.37	13721
N-Formylmethionine	3126	1.25	13722
N-Benzoyl Derivatives			
N-Benzoylglutamic acid	3012	1.14	13782
N-Benzoylleucine	3012	1.11	14460
N-Benzoylphenylalanine	3012	1.17	13730
N-Benzoylphenylglycine	3012	1.13	14461
N-Benzoylvaline	3012	1.19	13778
N-Dansyl Derivatives (5-5-Dimethyl-aminonaphthalene-1-sulfonyl derivative)			
N-Dansylnorvaline	3011	1.24	13766
N-Dansylphenylalanine	3011	1.27	13771
N-Dansylthreonine	3012	1.18	13734
N-Dansyltryptophan	3010	1.15	13774
N-Dansylvaline	3011	1.28	13763
PTH Derivatives (Phenylthiohydantoin)			
PTH-Valine	3014	1.12	13921

Separations of Underivatized "Free" Amino Acids


Compound	Chirex Phase	Separation Factor (α)	App ID No
Alanine	3126	1.66	14004
Alanylglycine	3126	2.26	14080
Alanyl-glycyl-glycine	3126	1.62	14082
Alloisoleucine	3126	1.67	14038
Allothreonine	3126	1.19	14046
Arginine	3126	2.15	14027
Asparagine	3126	1.10	14049
Aspartic acid	3126	1.42	14019
Baclofen	3126	1.23	13785
p-Boronophenylalanine	3126	1.36	13790
2-amino-n-Butyric acid	3126	1.80	14034
Cystine	3126	2.47	14085
2,6-Diaminopimelic acid	3126	2.77	14066
3-(3,4-Dihydroxyphenyl)-alanine (DOPA)	3126	1.22	13750
Glutamic acid	3126	1.11	14047
Glutamine	3126	1.71	14022
Glycylalanine	3126	1.78	14079
Glycylvaline	3126	1.69	14081
Histidine	3126	1.32	13745
Isoleucine	3126	1.70	14035
Leucine	3126	1.56	14009
Leucylglycyl-glycine	3126	1.36	14083
Lysine	3126	1.83	14018
Methionine	3126	1.42	14024
α -Methyl Leucine	3126	1.59	14457
α -Methyl Tryptophan	3126	1.18	14456
Naphthylglycine	3126	1.42	13789
Norvaline	3126	1.95	14029
Ornithine	3126	1.38	14041
Phenylalanine	3126	1.44	13740
Phenylglycine	3126	1.78	13748
Pipecolic acid	3126	1.77	14031
Proline	3126	2.50	14011
Serine	3126	1.17	14016
Threonine	3126	1.20	14043
dl-Threo-3-phenylserine	3126	1.15	13787
Tryptophan	3126	1.11	13737
Tyrosine	3126	1.34	13743
Valine	3126	1.91	14006

i Alpha (α) = Separation Factor = k_2/k_1

i Separation potential of some other amino acid derivatives: (Recommended columns: Chirex 3010, 3011, 3012, 3014)
 CBZ-Derivatives (carbobenzoxy; benzyloxycarbonyl); IC-Derivatives (phenylisocyanate);
 Dabsyl Derivatives (4-4-dimethylaminoazobenzene-4'-sulfonyl)

Z-Alanine


Column: Chirex 3011
Dimensions: 250 x 4.0 mm
Part No.: 00G-3011-00
Mobile Phase: 0.01 M Ammonium Acetate in Methanol
Flow Rate: 1.0 mL/min
Detector: UV @ 254 nm



App ID: 13729

Baclofen

Column: Chirex 3126
Dimensions: 150 x 4.6 mm
Part No.: 00F-3126-EQ
Mobile Phase: 2 mM Copper (II) sulfate in water / Isopropanol (85:15)
Flow Rate: 1.0 mL/min
Detector: UV @ 254 nm



App ID: 13785

Columbus™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/columbus
- For new methods, we recommend Gemini NX HPLC columns, see p. 226

Cosmosil™

By Nacalai Tesque

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/cosmosil

Curosil™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/curosil
- For new methods, we recommend Luna PFP columns, see p. 270

Develosil®

By Nomura Chemical Co.

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/develosil

EnviroSep™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/envirosep
- For alternative EnviroSep-PP and -CM applications, we recommend Kinetex® Biphenyl Core-shell columns, see p. 240
- For alternative EnviroSep-ABC GPC sample cleanup columns, see Phenogel p. 308



Gemini[®] pH Flexible LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

pH Flexibility Expands Robustness and Reproducibility

Gemini columns are rugged reversed phase HPLC columns that offer extended lifetime at extreme pH conditions and excellent stability for reproducible, high efficiency separations.

- Take full advantage of high and low pH conditions (pH 1-12) to manipulate selectivity
- Expect longer column lifetime with patented TWIN-NX[™] technology
- For analytical and preparative separations of basic and acidic compounds

Phase	Description	USP Classification
NX-C18	The most rugged Gemini column, offering 5 times the durability of previous generation hybrid columns	L1
C6-Phenyl	A low bleed phenyl phase. For UV and MS detection, which offers an aromatic selectivity complementary to C18 phases	L11
C18	Selectivity, high structural integrity and increased loadability for preparative and purification applications in pre-packed columns and bulk media	L1

guarantee

If Gemini analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.


Gemini[®]
pH Flexible LC



TWIN[™] (Two-In-One) Technology

Gemini C18 and C6-Phenyl


During the final stage of silica manufacturing a unique silica-organic layer is grafted to create a completely new composite particle. Since the internal base silica is unaltered by this manufacturing process, the particle retains its mechanical strength and rigidity along with excellent efficiency, while the silica-organic shell protects the particle from chemical attack.

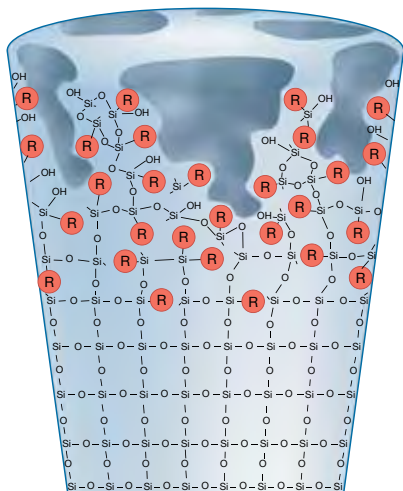

Second-Generation TWIN-NX Technology

Gemini NX-C18

TWIN-NX technology uses an improved patented organo-silica grafting process which incorporates highly stabilizing ethane cross-linking. These organic groups are evenly incorporated into the grafted layers on the silica surface while maintaining a pure silica core. This not only provides resistance to high pH attack, but also maintains the high efficiency and mechanical strength of a silica particle.

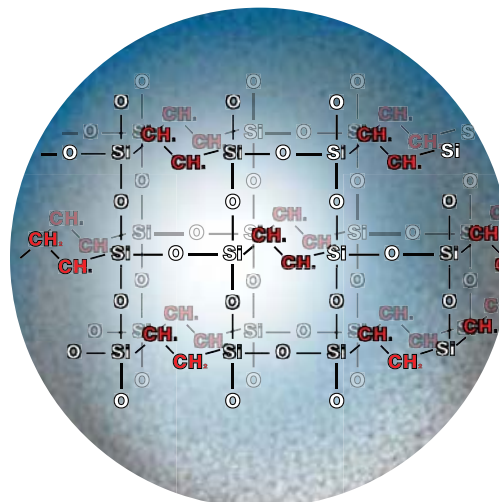

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

Gemini NX-C18

- pH stable 1-12 for durability
- Consistent performance in both volatile and non-volatile buffers
- High sample loading capacity for metabolite identification and preparative purification

Gemini NX-C18

USP: L1

LC/MS Certified

pH Stability: 1.0 – 12.0

Particle Size: 3 µm, 5 µm, and 10 µm

Phase: C18

Application: Small molecules, basic compounds

Strength: Extremely durable pH stable particle

Pore Size (Å): 110


Surface Area (m²/g): 375

Carbon Load %: 14


End Capping: TMS

Gemini NX-C18 Tested for Extreme Durability in Changing Mobile Phase pH

Column Efficiencies Maintained in High Testing for 20 Cycles

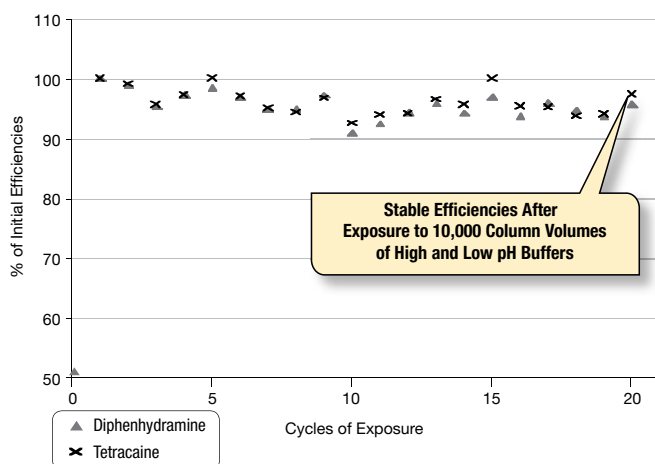

Retention Times of Four Probes Maintained in Neutral pH Testing for 20 Cycles

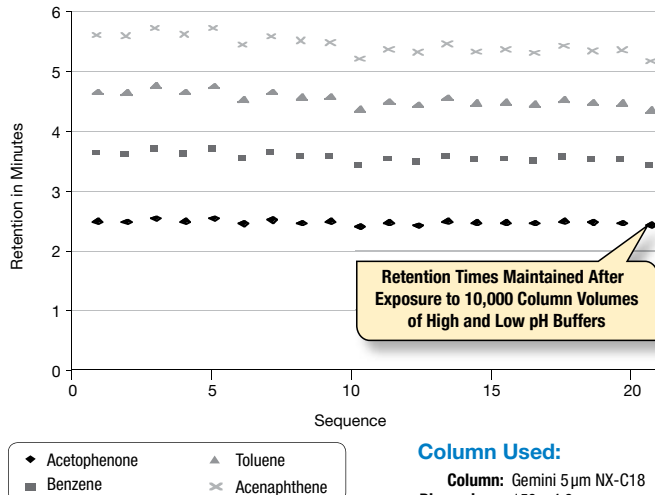

Column Used:

Column: Gemini 5 µm NX-C18
 Dimensions: 150 x 4.6 mm
 Part No.: 00F-4454-E0

Column Testing Cycle

Step 1

24x High pH Flush Procedures

Mobile Phase: A: 10 mM Ammonium Bicarbonate pH 10.5
 B: Acetonitrile

Gradient: 5% to 95% B in 6 min Hold at 95% B for 2 min

Re-equilibrate: 5% B for 2 min

Flow Rate: 1.5 mL/min

Step 2

High pH Testing

Isocratic: 10 mM Ammonium Bicarbonate pH 10.5 / Acetonitrile (50:50)

Flow Rate: 1.5 mL/min

Detection: UV @ 230 nm

Samples: 1. Tetracaine
 2. Diphenhydramine

Step 3

1x Neutral Flush Procedure

Mobile Phase: A: Water
 B: Acetonitrile

Gradient: 5% B for 2 min
 5% to 100% B in 3 min Hold at 100% B for 5 min

Flow Rate: 1.5 mL/min

Step 4

Neutral pH Testing

Isocratic: Water / Acetonitrile (35:65)

Flow Rate: 1.0 mL/min

Detection: UV @ 254 nm

Samples: 1. Acetophenone
 2. Benzene
 3. Toluene
 4. Acenaphthene

Step 5

24x Low pH Flush Procedure

Mobile Phase: A: 0.5% Formic Acid in Water
 B: 0.5% Formic Acid in Acetonitrile, pH 2.0

Gradient: 5% to 95% B in 6 min
 Hold at 95% B for 2 min

Re-equilibrate: 5% B for 2 min

Flow Rate: 1.5 mL/min

Step 6

Neutral pH Flush Repeats
 Repeats for 20 Cycles





Gemini[®] pH Flexible LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

Gemini NX-C18 (cont'd)

Polar Bases at High pH (pH 10.5)

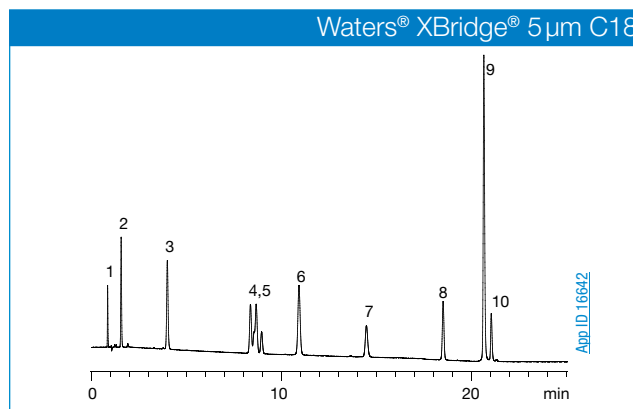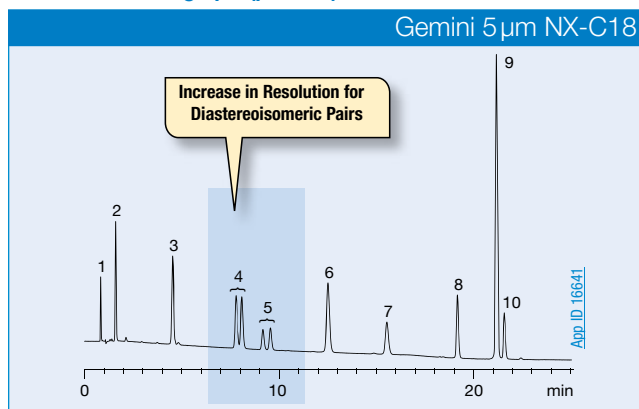

Y-axis normalized for all chromatograms.

Polar Bases (Beta Blockers) at High pH

Conditions for all columns:

Dimensions: 150 x 4.6 mm

Mobile Phase: A: 10 mM Ammonium Bicarbonate pH 10.5
B: Acetonitrile

Gradient: A/B (85:15) to (70:30) in 15 min to (50:50) in 5 min, Hold for 5 min

Flow Rate: 1.5 mL/min



Temperature: Ambient

Detection: UV @ 230 nm

- Sample:**
1. Bisoprolol Contaminant
 2. Sotalol
 3. Atenolol
 4. Labetalol (Diastereoisomeric Pair)
 5. Nadolol (Diastereoisomeric Pair)
 6. Pindolol
 7. Metoprolol
 8. Bisoprolol
 9. Propranolol
 10. Alprenolol



Polar Bases at Low pH (pH 2.7)

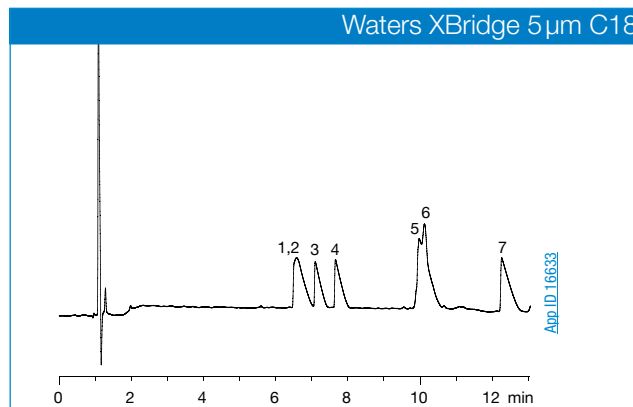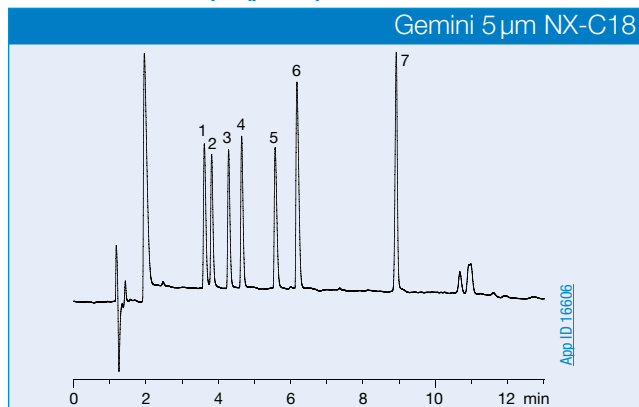

Y-axis normalized for all chromatograms.

Polar Bases (Antihistamines) in Formic Acid

Conditions for all columns:

Dimensions: 150 x 4.6 mm

Mobile Phase: A: 0.1% Formic Acid in Water
B: 0.1% Formic Acid in Acetonitrile

Gradient: A/B (90:10) to (50:50) in 10 min

Flow Rate: 1.5 mL/min

Temperature: Ambient

Detection: UV @ 210 nm

- Sample:**
1. Pyrilamine
 2. Triplennamine
 3. Chlorpheniramine
 4. Brompheniramine
 5. Chloropyramine
 6. Diphenhydramine
 7. Loratadine

Comparative chromatograms may not be representative of all applications.

Gemini[®] pH Flexible LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

Gemini C18

- Increased loading and retention of basic compounds
- Silica efficiency and mechanical strength
- pH stable 1-12 for durability

Gemini C18

USP: L1

LC/MS
Certified

pH Stability: 1.0 – 12.0

Particle Size: 3 µm, 5 µm, and 10 µm

Phase: C18

Application: Small molecules, basic compounds

Strength: Wide pH stability, high efficiency

Pore Size (Å): 110


Surface Area (m²/g): 375

Carbon Load %: 14

End Capping: TMS

Chromatographic Comparisons

Gemini 5 µm C18 110 Å

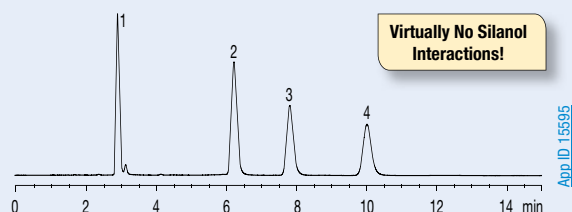

Tricyclic Antidepressants at Neutral pH

Conditions for all columns:

Dimensions: 150 x 4.6 mm

Mobile Phase: 20 mM Phosphate buffer pH 7.0/Acetonitrile/
Methanol (30:35:35)

Flow Rate: 1.5 mL/min

Detection: UV @ 254 nm


Sample: 1. Nortriptyline

2. Imipramine


3. Amitriptyline

4. Clomipramine


Agilent Technologies[®] ZORBAX[®] 5 µm Extend-C18 80 Å



Advanced Chromatography Technologies ACE[®] 5 µm C18 100 Å

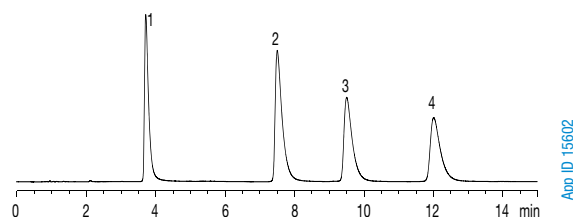

Batch-to-Batch Reproducibility

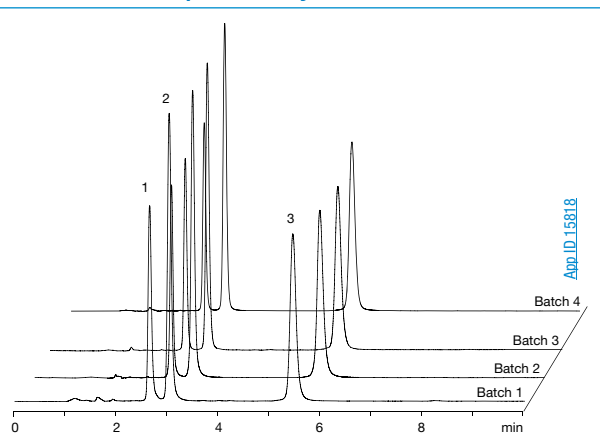

Conditions for all separations:

Column: Gemini 5 µm C18

Dimension: 150 x 4.6 mm

Part No.: 00F-4435-E0

Mobile Phase: 10 mM Ammonium Bicarbonate,
pH 10.5/Acetonitrile (50:50)

Flow Rate: 1.0 mL/min

Temperature: Ambient

Detection: UV @ 230 nm

Sample: 1. Pindolol


2. Metoprolol

3. Propranolol

Extended Column Lifetime

The TWIN™ Technology engineering of Gemini provides stability and increased column lifetime. Whether used under isocratic or gradient conditions, Gemini columns out-perform and outlasts pH stable columns. This is illustrated below.

Lifetime and Efficiency Comparison**

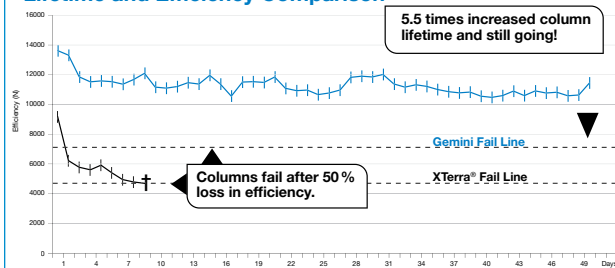

Conditions for all columns:

Columns: Gemini 5 µm C18

Waters[®] XTerra[®] 5 µm MS C18

Dimensions: 150 x 4.6 mm

Mobile Phase: Acetonitrile/50 mM Methylpyrrolidine
Buffer, pH 11.5 (50:50)

Flow Rate: 1 mL/min

Temperature: Ambient

Detection: UV @ 254 nm

Sample: Diphenhydramine

**Efficiency and lifetime comparison based on average of two columns each run in parallel.

The comparative data presented here may not be representative for all applications.

Gemini[®] pH Flexible LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

Gemini C6-Phenyl

- pH stable 1-12 for durability
- Great aromatic selectivity
- Extremely low UV and MS bleed

Gemini C6-Phenyl

USP: L11

LC/MS
Certified

pH Stability: 1.0 – 12.0

Particle Size: 3 µm and 5 µm

Phase: Phenyl with C6 linker

Application: Aromatic, polar, or basic compounds

Strength: High aromatic selectivity with exceptional peak shape even in neutral conditions. Extremely low bleed phenyl column.

Pore Size (Å): 110

Surface Area (m²/g): 375

Carbon Load %: 12

End Capping: TMS

Enhanced Performance for Aromatic Compounds

Sulfa Drug Application

Resolution	Pursuit 5 µm DiPhenyl	Gemini 5 µm C6-Phenyl
RS _{1,2}	1.0	4.0
RS _{2,3}	9.8	16.0

Conditions for all columns:

Dimensions: 150 x 4.6 mm

Mobile Phase: 0.1 % Formic Acid in Water/
Methanol (70:30)

Flow Rate: 1.0 mL/min

Temperature: Ambient


Detection: UV @ 254 nm

Sample: 1. Sulfathiazole

2. Sulfamerazine


3. Sulfamethoxazole

Phenomenex Gemini 5 µm C6-Phenyl

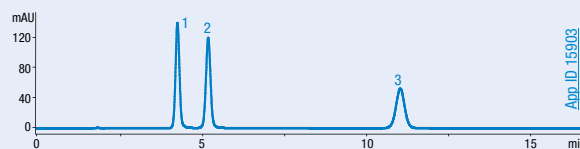

App ID: 15903

Agilent Technologies[®] Pursuit[®] 5 µm DiPhenyl




App ID: 15908



GEMINI | HPLC / UHPLC

Reproducible Phenyl Phase

Aliphatic Acid Application

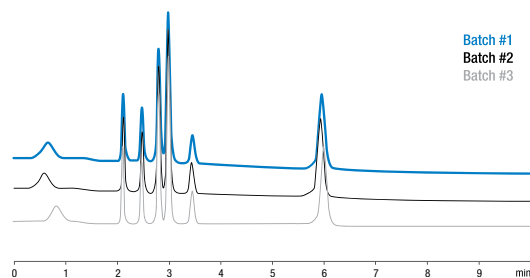

Batch #1
Batch #2
Batch #3

Conditions for all columns:

Column: Gemini 5 µm C6-Phenyl

Dimensions: 150 x 4.6 mm

Part No.: 00F-4444-E0

Mobile Phase: 20 mM Phosphate buffer,
pH 2.5/Methanol (97:3)


Flow Rate: 1.0 mL/min

Temperature: Ambient

Detection: UV @ 220 nm

Sample: 1. Tartaric Acid 4. Acetic Acid
2. Malic Acid 5. Citric Acid
3. Lactic Acid 6. Propionic Acid

Low Bleed Phenyl Phase

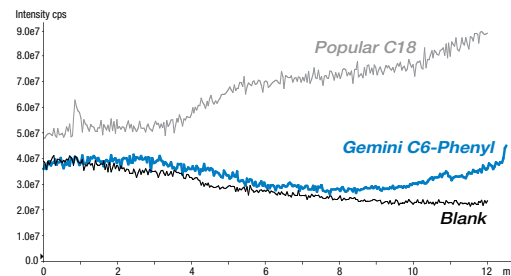

Conditions for all columns:

Dimensions: 150 x 3.0 mm

Mobile Phase: A: 0.1 % Formic acid in Water

B: 0.1 % Formic acid in Acetonitrile

Gradient: 5 % B to 95 % B in 10 min, then hold
95 % B for 2 min

Flow Rate: 0.6 mL/min

Temperature: Ambient

MS Detection: ESI + ion mode,

M/Z 100-700

Comparative chromatograms may not be representative for all applications.

Gemini[®] pH Flexible LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

Applications


Mycotoxin Screening

Column: Gemini 5 μ m C18
Dimensions: 150 x 4.6 mm
Part No.: [00F-4435-EO](#)
Mobile Phase: A: Water/Methanol (90:10) containing 5 mM Ammonium acetate and 1 % Acetic acid
 B: Water/Methanol (3:97) containing 5 mM Ammonium acetate and 1 % Acetic acid

Gradient	Time (min)	% B
	0	0
	14	100
	18.01	0
	20.5	0

Flow Rate: 1 mL/min
Temperature: 25 °C
Detection: Tandem Mass Spectrometer (MS/MS) (25 °C)
Detector: SCIEX API 4000[™] System

- Sample:**
- | | |
|-----------------|-------------------------|
| 1. Lincomycin | 8. Ergocryptine |
| 2. Ergometrine | 9. Ochratoxin A |
| 3. Aflatoxin G2 | 10. Nigirin |
| 4. Aflatoxin G1 | 11. Chloramphenicol |
| 5. Aflatoxin B2 | 12. β -Zearalenol |
| 6. Ergocryptine | 13. Rapamycin |
| 7. Aflatoxin B1 | |
- See full list of analytes at www.phenomenex.com

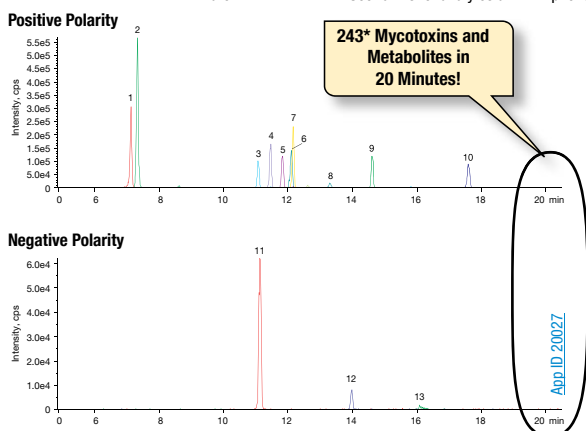


Hormones in Drinking Water: EPA Method 539

Column: Gemini 3 μ m NX-C18
Dimensions: 100 x 2.0 mm
Part No.: [00D-4453-B0](#)
Mobile Phase: A: 0.2% NH₄OH in Water
 B: 0.2% NH₄OH in Methanol

Gradient	Time (min)	% B	Time (min)	% B
	0.0	35	8.50	85
	0.1	35	13.0	85
	0.60	65	13.01	35
	7.50	65	15.0	35

Flow Rate: 0.2 mL/min
Temperature: 22 °C
Detection: Tandem Mass Spectrometer (MS/MS) (22 °C)
Detector: SCIEX API 4000[™] System

- Sample:**
- | | |
|------------------------|----------------------------------|
| 1. Estriol | 8. Ethynylestradiol-d4 |
| 2. Estriol-d2 (IS) | 9. 17 α -Ethinylestradiol |
| 3. Bisphenol A-d16 | 10. 13C2-Ethinylestradiol (IS) |
| 4. Equilin | 11. Androstenedione |
| 5. Estrone | 12. Testosterone-d3 |
| 6. Beta-estradiol | 13. Testosterone |
| 7. 13C6-estradiol (IS) | |

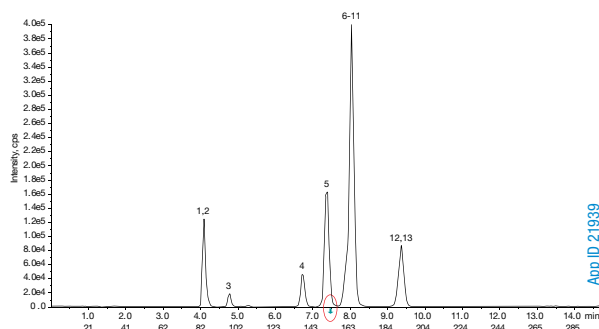


Vitamin B3

Column: Gemini 3 μ m C18
Dimensions: 100 x 4.6 mm
Part No.: [00D-4439-EO](#)
Mobile Phase: A: 0.1 % Formic acid in Water
 B: Methanol

Gradient	Time (min)	% B
	0	10
	2.5	90
	2.6	10
	4	10

Flow Rate: 0.6 mL/min
Temperature: 22 °C
Detection: Electrospray Mass Spec (ESMS) (22 °C)
Detector: SCIEX API 4000[™] System
Sample: 1. Nicotinamide
 2. Nicotinic acid

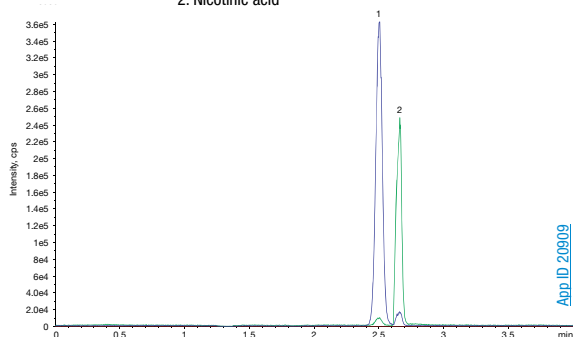


TMP and Thiamine

Column: Gemini 3 μ m NX-C18
Dimensions: 100 x 3.0 mm
Part No.: [00D-4453-Y0](#)
Mobile Phase: A: 25 mM Na₂HPO₄ with 10% methanol (pH 7.0)
 B: 25 mM Na₂HPO₄ with 70% methanol (pH 7.0)

Gradient	Time (min)	% B	Time (min)	% B
	0	97	4	0
	0.25	75	5	0
	0.75	75	5.1	97
	3	65	8	97

Flow Rate: 0.75 mL/min
Detection: Fluorescence (Excitation: 375 nm, Emission: 435 nm) (Ambient)
Temperature: 22 °C
Sample: 1. TMP
 2. Thiamine

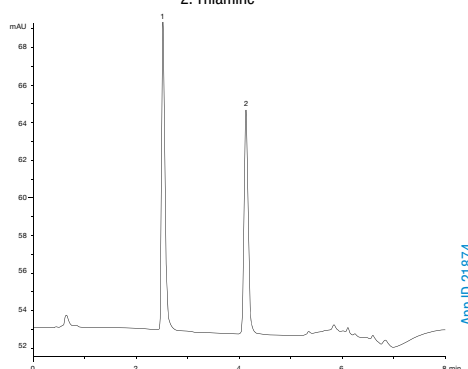

Gemini[®] pH Flexible LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

guarantee

If Gemini analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information

3µm Microbore, Minibore and MidBore™ Columns (mm)										SecurityGuard™ Cartridges (mm)
Phases	50 x 1.0	20 x 2.0	30 x 2.0	50 x 2.0	100 x 2.0	150 x 2.0	50 x 3.0	100 x 3.0	150 x 3.0	4 x 2.0* /10pk
C18	00B-4439-A0	00M-4439-B0	00A-4439-B0	00B-4439-B0	00D-4439-B0	00F-4439-B0	00B-4439-Y0	00D-4439-Y0	00F-4439-Y0	AJO-7596
C6-Phenyl	00B-4443-A0	—	00A-4443-B0	00B-4443-B0	00D-4443-B0	00F-4443-B0	00B-4443-Y0	00D-4443-Y0	00F-4443-Y0	AJO-7914
NX-C18	00B-4453-A0	00M-4453-B0	00A-4453-B0	00B-4453-B0	00D-4453-B0	00F-4453-B0	00B-4453-Y0	00D-4453-Y0	00F-4453-Y0	AJO-8367

for ID: 2.0-3.0mm

3µm Analytical Columns (mm)						SecurityGuard™ Cartridges (mm)
Phases	30 x 4.6	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0* /10pk
C18	00A-4439-E0	00B-4439-E0	00D-4439-E0	00F-4439-E0	00G-4439-E0	AJO-7597
C6-Phenyl	00A-4443-E0	00B-4443-E0	00D-4443-E0	00F-4443-E0	00G-4443-E0	AJO-7915
NX-C18	—	00B-4453-E0	00D-4453-E0	00F-4453-E0	00G-4453-E0	AJO-8368

for ID: 3.2-8.0mm



5µm Minibore and MidBore Columns (mm)								SecurityGuard™ Cartridges (mm)	
Phases	30 x 2.0	50 x 2.0	150 x 2.0	250 x 2.0	50 x 3.0	100 x 3.0	150 x 3.0	250 x 3.0	4 x 2.0* /10pk
C18	00A-4435-B0	00B-4435-B0	00F-4435-B0	00G-4435-B0	00B-4435-Y0	00D-4435-Y0	00F-4435-Y0	00G-4435-Y0	AJO-7596
C6-Phenyl	—	00B-4444-B0	00F-4444-B0	—	00B-4444-Y0	—	00F-4444-Y0	00G-4444-Y0	AJO-7914
NX-C18	00A-4454-B0	00B-4454-B0	00F-4454-B0	—	00B-4454-Y0	00D-4454-Y0	00F-4454-Y0	00G-4454-Y0	AJO-8367

for ID: 2.0-3.0mm

5µm Analytical Columns (mm)						SecurityGuard™ Cartridges (mm)
Phases	30 x 4.6	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0* /10pk
C18	00A-4435-E0	00B-4435-E0	00D-4435-E0	00F-4435-E0	00G-4435-E0	AJO-7597
C6-Phenyl	—	00B-4444-E0	00D-4444-E0	00F-4444-E0	00G-4444-E0	AJO-7915
NX-C18	—	00B-4454-E0	00D-4454-E0	00F-4454-E0	00G-4454-E0	AJO-8368

for ID: 3.2-8.0mm



For Gemini Capillary HPLC Columns and Guards, contact your Phenomenex technical consultant or local distributor.



5µm Semi-Prep Columns (mm)			SecurityGuard™ Cartridges (mm)
Phases	150 x 10	250 x 10	10 x 10 ³ /3pk
C18	00F-4435-N0	00G-4435-N0	AJO-7598
C6-Phenyl	—	00G-4444-N0	AJO-9156
NX-C18	00F-4454-N0	00G-4454-N0	AJO-8369

for ID: 9-16mm



GEMINI | HPLC / UHPLC

Axia™ Packed Preparative Columns (mm)							SecurityGuard™ Cartridges (mm)	
Phases	50 x 21.2	100 x 21.2	150 x 21.2	250 x 21.2	50 x 30	75 x 30	15 x 21.2**	15 x 30.0'
5µm							/ea	/ea
C18	00B-4435-P0-AX	00D-4435-P0-AX	00F-4435-P0-AX	00G-4435-P0-AX	00B-4435-U0-AX	—	AJO-7846	AJO-8308
C6-Phenyl	—	00D-4444-P0-AX	00F-4444-P0-AX	00G-4444-P0-AX	—	—	AJO-9157	AJO-9158
5µm							/ea	/ea
NX-C18	00B-4454-P0-AX	00D-4454-P0-AX	00F-4454-P0-AX	00G-4454-P0-AX	00B-4454-U0-AX	00C-4454-U0-AX	AJO-8370	AJO-8371
10µm							/ea	/ea
C18	—	00D-4436-P0-AX	00F-4436-P0-AX	00G-4436-P0-AX	—	—	AJO-7846	AJO-8308
10µm							/ea	/ea
NX-C18	00B-4455-P0-AX	00D-4455-P0-AX	00F-4455-P0-AX	00G-4455-P0-AX	—	—	AJO-8370	AJO-8371

for ID: 18-29mm 30-49mm

Axia™ Packed Preparative Columns (mm) continued						SecurityGuard™ Cartridges (mm)	
Phases	100 x 30	150 x 30	250 x 30	100 x 50	150 x 50	250 x 50	15 x 30.0*
5µm							/ea
C18	00D-4435-U0-AX	00F-4435-U0-AX	00G-4435-U0-AX	—	—	—	AJO-8308
5µm							/ea
NX-C18	00D-4454-U0-AX	00F-4454-U0-AX	00G-4454-U0-AX	—	—	—	AJO-8371
10µm							/ea
C18	00D-4436-U0-AX	00F-4436-U0-AX	00G-4436-U0-AX	—	00F-4436-V0-AX	00G-4436-V0-AX	AJO-8308
10µm							/ea
NX-C18	00D-4455-U0-AX	00F-4455-U0-AX	00G-4455-U0-AX	00D-4455-V0-AX	00F-4455-V0-AX	00G-4455-V0-AX	AJO-8371

for ID: 30-49mm



For PREP Columns & Bulk Media, see p. 371
 For SecurityGuard Holders and Cartridges, see p. 326
 For MercuryMS LC/MS Columns, Cartridges, and Cartridge Holders, Inquire.

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJO-4282](#)
 †SemiPrep SecurityGuard™ Cartridges require holder, Part No.: [AJO-9281](#)
 **PREP SecurityGuard™ Cartridges require holder, Part No.: [AJO-8223](#)
 ††PREP SecurityGuard™ Cartridges require holder, Part No.: [AJO-8277](#)

Hamilton®

By Hamilton Co.

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/hamilton

Hypercarb®

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/hypercarb

Hypersil® and Hypersil® BDS

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/hypersil and www.phenomenex.com/hypersilbds
- Use HyperClone™ columns as a guaranteed alternative to Hypersil, see p. 234

IB-Sil™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/ibsil

Inertsil®

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/inertsil
- See InertClone for a cost effective guaranteed replacement to Inertsil

If HyperClone™ analytical columns do not provide at least an equivalent separation compared to Hypersil® columns of the same phase, particle size and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Guaranteed Replacement to Hypersil®

- Highly reproducible
- Long column life
- Mimics performance of Thermo Hypersil-Keystone Hypersil
- Economically priced

Phenomenex HyperClone columns have been developed to provide chromatographic behavior that mimics that of Thermo Hypersil columns. For comparative applications, please contact your local Phenomenex representative.


Comparisons of physical and chemical characteristics of HyperClone and Hypersil are listed below. As you can see, HyperClone and Hypersil compare very well for important specifications such as particle size, pore size, and carbon load.

HyperClone


VS.

Hypersil


Material Characteristics

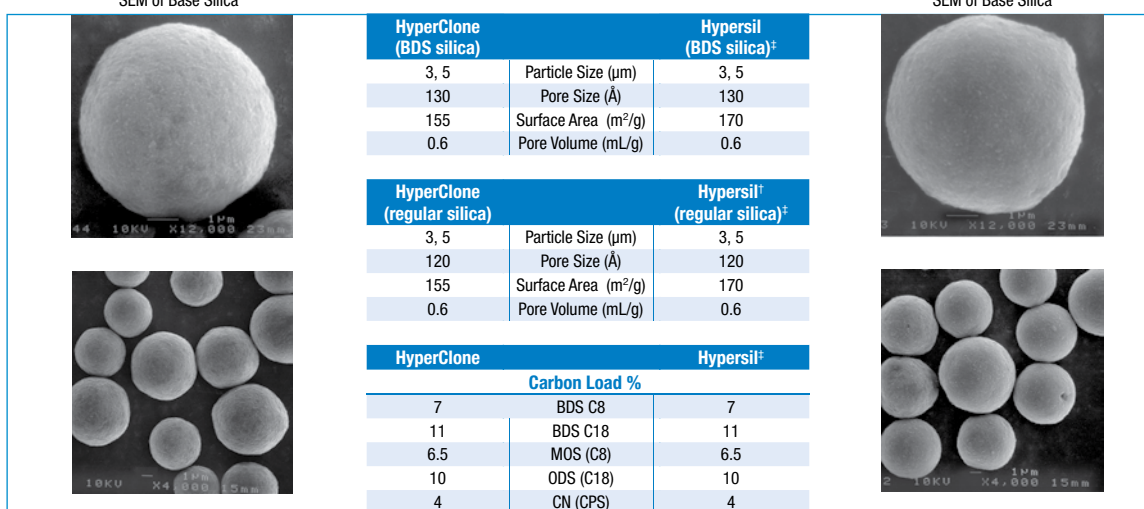

Particle Size Distribution†

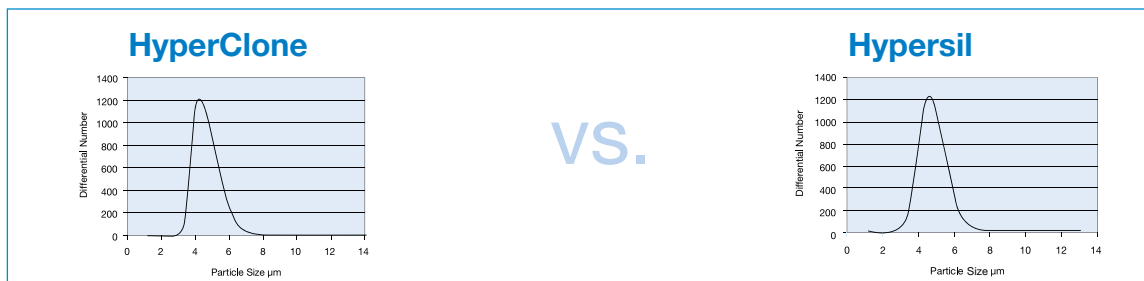

HyperClone Reproducibility

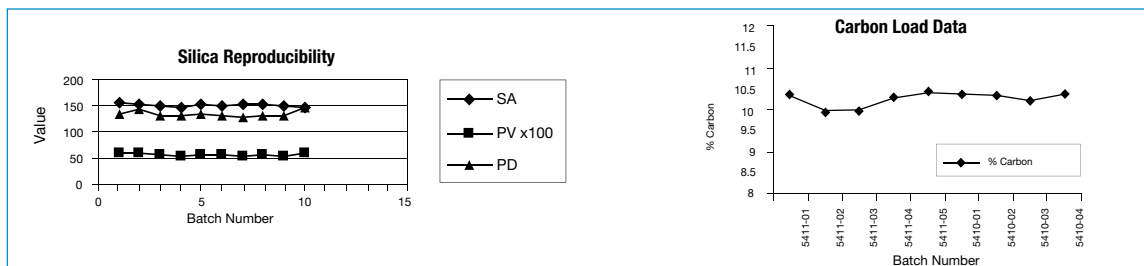



† All Hypersil information obtained from (then) Thermo Electron Corporation 2006-2007 catalog and 2012-2013 Thermo Scientific Chromatography Columns catalog.

HyperClone™ Guaranteed Replacement to Hypersil

guarantee

If HyperClone™ analytical columns do not provide at least an equivalent separation compared to Hypersil® columns of the same phase, particle size and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

VS.

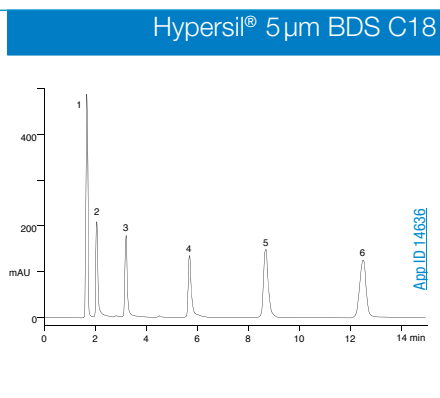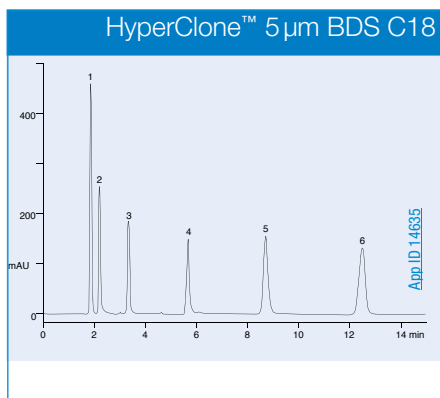

Non-Polar Basic Compounds

Conditions for Both Columns

- Dimensions:** 150 x 4.6 mm
- Mobile Phase:** Methanol/50 mM KH_2PO_4 , pH 3.5 (60:40)
- Flow Rate:** 1.0 mL/min
- Detection:** UV @ 254 nm
- Sample:**
 1. Uracil
 2. Pyridine
 3. Methylaniline
 4. Dimethylaniline
 5. Dichloronitroaniline
 6. Toluene

Ordering Information

3 µm Minibore and Analytical Columns (mm)	SecurityGuard™ Cartridges (mm)							
	50 x 2.0	150 x 2.0	150 x 3.2	100 x 4.6	125 x 4.0	150 x 4.6	4 x 2.0*	4 x 3.0*
ODS (C18)	—	00F-4356-B0	—	00D-4356-E0	00E-4356-D0	00F-4356-E0	AJ0-4286 /10pk	AJ0-4287 /10pk
BDS C8	00B-4417-B0	—	—	—	—	00F-4417-E0	AJ0-4289 /10pk	AJ0-4290 /10pk
BDS C18	00B-4419-B0	00F-4419-B0	00F-4419-R0	00D-4419-E0	—	00F-4419-E0	AJ0-4286 for ID: 2.0-3.0 mm	AJ0-4287 3.2-8.0 mm

5 µm Minibore and Analytical Columns (mm)	SecurityGuard™ Cartridges (mm)									
	150 x 2.0	150 x 3.2	250 x 3.2	125 x 4.0	250 x 4.0	100 x 4.6	150 x 4.6	250 x 4.6	4 x 2.0*	4 x 3.0*
Silica	—	—	—	—	—	—	00F-4358-E0	00G-4358-E0	AJ0-4347 /10pk	AJ0-4348 /10pk
MOS (C8)	—	—	—	00E-4359-D0	—	00D-4359-E0	00F-4359-E0	00G-4359-E0	AJ0-4289 /10pk	AJ0-4290 /10pk
ODS (C18)	—	00F-4361-R0	00G-4361-R0	00E-4361-D0	00G-4361-D0	00D-4361-E0	00F-4361-E0	00G-4361-E0	AJ0-4286 /10pk	AJ0-4287 /10pk
CN (CPS)	—	—	—	—	—	—	00F-4422-E0	00G-4422-E0	AJ0-4304 /10pk	AJ0-4305 /10pk
BDS C8	—	—	—	—	—	—	00F-4418-E0	00G-4418-E0	AJ0-4289 /10pk	AJ0-4290 /10pk
BDS C18	00F-4420-B0	00F-4420-R0	—	00E-4420-D0	00G-4420-D0	00D-4420-E0	00F-4420-E0	00G-4420-E0	AJ0-4286 for ID: 2.0-3.0 mm	AJ0-4287 3.2-8.0 mm

5 µm SemiPrep Columns (mm)	SecurityGuard™ Cartridges (mm)
Phases	250 x 10
	10 x 10 †
	/3pk
ODS (C18)	00G-4361-N0
	AJ0-7221
	for ID: 9-16 mm

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)
 †SemiPrep SecurityGuard™ Cartridges require holder, Part No.: [AJ0-9281](#)



Other dimensions available upon request.



For SecurityGuard Cartridge Holders and Cartridges, see p. 326.


Comparative separations may not be representative of all applications.

If InertClone analytical columns do not provide the equivalent separation as compared to an Inertsil column of the same particle size, phase and dimensions, return the columns with comparative data within 45 days for a FULL REFUND.


Guaranteed Replacement to Inertsil®

InertClone VS. Inertsil Material Characteristics

InertClone		Inertsil
Particle Size (µm) and Shape		
3, Spherical		3, Spherical
5, Spherical		5, Spherical
Pore Size (Å)		
150	Ph (Phenyl), C8, ODS-2	150
100	ODS-3	100
Surface Area (m²/g)		
310	Ph (Phenyl), C8, ODS-2	320
450	ODS-3	450
Carbon Load %		
12.6	C8	10.5
18.5	ODS-2	18.5
15.5	ODS-3	15.0
10.0	Ph (Phenyl)	10.0

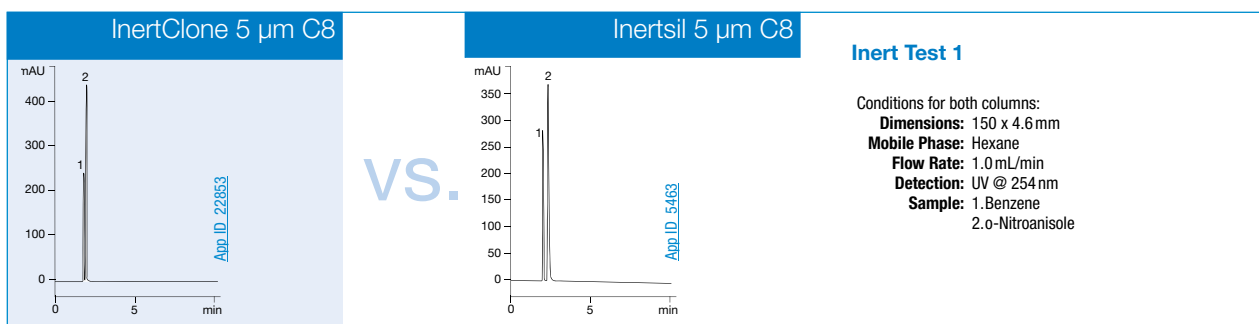

Note: Inertsil columns were manufactured by GL Sciences, Inc., Japan

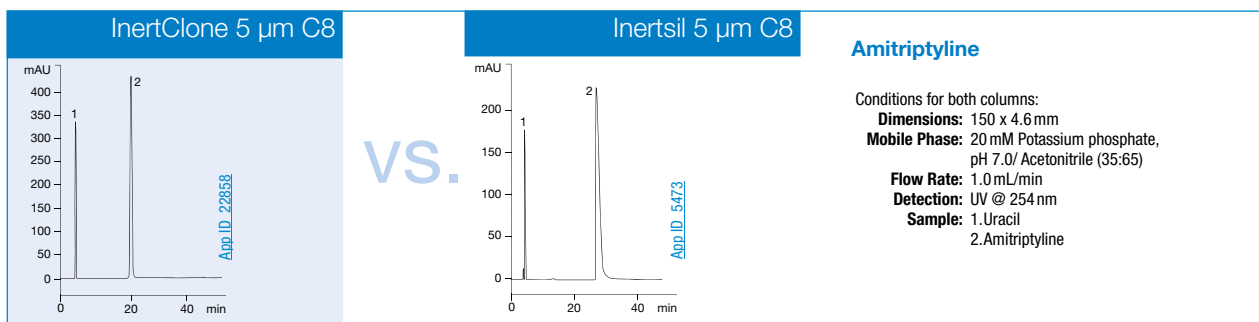

Comparative separations may not be representative of all applications.

Ordering Information

3 µm Analytical Columns (mm)			SecurityGuard™ Cartridges (mm)	
Phase	100 x 4.6	150 x 4.6	4 x 3.0*	
ODS-3	100Å 00D-4340-E0	00F-4340-E0	/10 pk AJ0-4287	

for ID: 3.2-8.0 mm

*SecurityGuard™ Analytical Cartridges require universal holder Part No.: [KJO-4282](#)

5 µm MidBore™ and Analytical Columns (mm)						SecurityGuard™ Cartridges (mm)	
Phases	150 x 3.0	250 x 3.0	100 x 4.6	150 x 4.6	250 x 4.6	4 x 2.0*	4 x 3.0*
ODS-2	150Å 00F-4342-Y0	00G-4342-Y0	00D-4342-E0	00F-4342-E0	00G-4342-E0	AJ0-4286	AJ0-4287
C8	150Å	—	—	00F-4391-E0	00G-4391-E0	AJ0-4289	AJ0-4290
Ph (Phenyl)	150Å	—	—	00F-4352-E0	00G-4352-E0	AJ0-4350	AJ0-4351
ODS-3	100Å	—	—	00F-4341-E0	00G-4341-E0	AJ0-4286	AJ0-4287

for ID: 2.0-3.0 mm

3.2-8.0 mm

RP-HPLC for Protein/Peptide Analysis and Purification

The Jupiter HPLC column portfolio, including Jupiter 300 and Jupiter Proteo, offers optimized reversed phase solutions for protein and peptide characterization and purification. With these columns, one can identify, purify, and analyze almost any protein.

Jupiter 300 – 300 Å columns designed to analyze and purify intact proteins

- For separation of intact proteins > 10,000 MW
- Available with C18, C5, and C4 bonded phases
- 1.5 – 10 pH stability for method ruggedness and easy protein removal
- Direct scale up to preparative and bulk materials

Jupiter Proteo – 90 Å columns engineered for increased peak capacity and resolution of peptide maps as well as peptide separations

- For separation of intact proteins and peptides < 10,000 MW
- Available with novel C12 bonded phase for excellent selectivity
- Identify post-translational modifications
- Capillary columns available for increased sensitivity

Material Characteristics

Packing Material	Particle Shape/Size (µm)	Pore Size (Å)	Surface Area (m ² /g)	Carbon Load %	Calculated Bonded Phase Coverage (µmole/m ²)	End Capping
C4	Spher. 5, 10, 15	300	170	5.0	6.30	Yes
C5	Spher. 5, 10	300	170	5.5	5.30	Yes
C18	Spher. 3, 5, 10, 15	300	170	13.3	5.50	Yes
Proteo	Spher. 4, 10	90	475	15.0	—	Yes

Engineered for Robustness, Reproducibility, and Quality

It is tough to compete with Jupiter standards. Each column has consistent specifications and thus consistent performance.

- pH 1.5-10 stability gives robust, method development opportunities
- Over 25 individual quality control tests performed on every batch of Jupiter material
- Every column reproducibility aspect is specified, tested, and reported in Materials Validation Document (MVD)

pH 1.5 – 10 Stability

A wide pH range means opportunity for method development, in addition to longer column life. Jupiter columns are stable for over 2500 hours at pH extremes. Jupiter 300 and Jupiter Proteo provide excellent separations using various MS compatible buffers and provide good resolution down to 0.01 % TFA.

Quality Proven

A Materials Validation Document (MVD) accompanies every Jupiter column. Each certificate documents the rigorous testing procedures performed on each batch of Jupiter material to ensure column-to-column and batch-to-batch reproducibility.

Silica physical tests and specifications

Pore size, particle size and distribution, metal content, surface area, carbon load and surface coverage specifications and results are all reported.

SEM analysis


Scanning Electron Microscopy (SEM) photos show surface smoothness and particle consistency as well as a visual representation of particle size distribution.

Diagnostic chromatography tests

Monitoring chromatographic specifications for silanol activity, hydrogen bonding capacity, hydrophobicity and peptide standards.

pH stability


Every batch goes through 1.5 and 10.0 pH testing before release, the results of which are reported on each MVD.

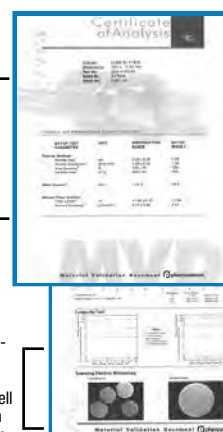

Reproducibility Assured

Batch-to-batch and column-to-column is critical to HPLC column performance. Through great advances in silica, bonding, and material characterization technology, Jupiter columns set a benchmark in reproducibility.

Column: Jupiter 5 µm C18 300 Å
Dimensions: 250 x 4.6 mm
Part No.: [00G-4053-E0](#)
Mobile Phase: A: 0.1 % TFA in Water
 B: 0.1 % TFA in Acetonitrile
Gradient: A/B (75:25) to A/B (45:55) in 15 min
Flow Rate: 1.0 mL/min
Detection: UV @ 220 nm
Sample: 1. Yeast Cytochrome c
 2. Equine Cytochrome c
 3. Bovine Cytochrome c

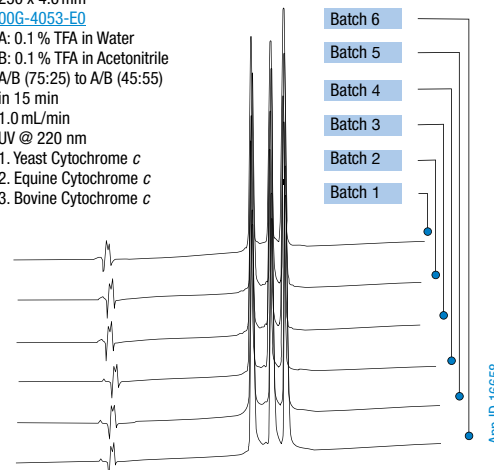

Jupiter

Selecting the Appropriate Jupiter Phase

Jupiter 300 C4 This low hydrophobicity phase is less likely to cause irreversible adsorption of “sticky” proteins and allows for the use of shallow gradients along with lower concentrations of organic solvent.

- For proteins >10,000 Da
- For highly hydrophobic proteins

Jupiter 300 C5 This bonded phase imparts greater pH stability compared to the traditional C4 phase. One can expect longer column lifetimes and more stable, reproducible retention times because of the bonded phase’s increased stability to hydrolysis.

- For proteins >10,000 Da
- For highly hydrophobic proteins
- More retentive than C4, offering slightly different selectivity

Jupiter 300 C18 Excellent for polar as well as non-polar proteins. It’s the most retentive of Jupiter 300 phases, allowing one to separate proteins with slight differences in hydrophobicity.

- For proteins >10,000 Da
- For hydrophilic proteins
- Most retentive phase


Jupiter Proteo C12 This novel phase is well suited for peptide mapping and the purification of synthetic peptides. The unique chemistry and 90 Å pore size offer improved selectivity and resolving power for peptide fragments compared to traditional 300 Å, C18 columns.

- For peptides < 10,000 Da
- For peptide mapping
- For purification of small peptides

Easy Scale-Up with Prep Columns and Bulk Material

Jupiter uses identical bonding and base silica technology in both analytical and preparative materials. Accordingly, Jupiter 300 material used in analytical separation is available in a 10 µm and 15 µm (Jupiter Proteo is available in 10 µm) version so you can easily scale up with minimal changes to the separation.


- Large loading capacity for higher sample recovery
- Easy material cleaning and regeneration
- Resistance to silica sheering and fine formation at high packing pressures and flow rates

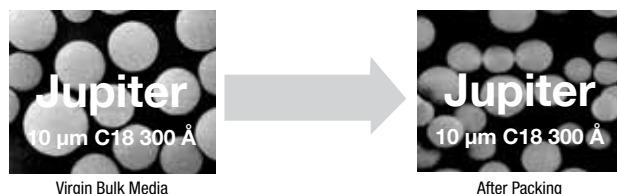

Large Proteins on Jupiter 300 C4

Column: Jupiter 300 5 µm C4 300 Å
Dimensions: 150 x 4.6 mm
Part No.: [00F-4167-EQ](#)
Guard Cartridge: [AJ0-4330](#)
Guard Holder: [KJ0-4282](#), SecurityGuard Guard Cartridge Kit
Mobile Phase: A: 0.1 % TFA in Water
 B: 0.08 % TFA in Acetonitrile
Flow Rate: 1 mL/min
Gradient: A/B (95:5) to A/B (20:80) in 20 minutes
Temperature: 22 °C
Detection: UV @ 280 nm
Inj. Volume: 25 µL


Filter: [AF0-8108-52](#), Phenex-PES 28 mm Syringe Filters 0.45 µm, Non-Sterile, Luer/Slip
Vial: [ARO-9925-13](#), Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: 1. Bovine Serum Albumin
 2. Glutamic Dehydrogenase
 3. β-Galactosidase
 4. Ovalbumin



Separation on Jupiter 300 C18

Column: Jupiter 300 5 µm C18 300 Å
Dimensions: 150 x 2.0 mm
Part No.: [00F-4053-B0](#)
Guard Cartridge: [AJ0-4320](#)
Guard Holder: [KJ0-4282](#), SecurityGuard Guard Cartridge Kit
Mobile Phase: A: 0.1 %TFA/ 95 % Water / 5 % Acetonitrile
 B: 0.085 % TFA/ 95 % Acetonitrile/ 5 % Water
Flow Rate: 0.2 mL/min
Gradient: A/B (88:12) to A/B (15:85) in 21 minutes
Detection: UV @ 220 nm

Filter: [AF0-8108-52](#), Phenex-PES 28 mm Syringe Filters 0.45 µm, Non-Sterile, Luer/Slip
Vial: [ARO-9925-13](#), Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: 1. Aprotinin
 2. Ribonuclease
 3. Lysozyme
 4. Lactalbumin
 5. Leptin



Jupiter[®] LC Columns for Proteins & Peptides

guarantee

If Jupiter analytical columns do not provide you with at least an equivalent separation as compared to a column of similar phase, particle size and dimension, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information

4 µm & 5 µm Capillary Columns (mm)				
Phases	50 x 0.30	150 x 0.30	50 x 0.50	150 x 0.50
5 µm C4 300 Å	00B-4167-AC	00F-4167-AC	00B-4167-AF	00F-4167-AF
5 µm C18 300 Å	00B-4053-AC	00F-4053-AC	00B-4053-AF	00F-4053-AF
4 µm Proteo 90 Å	00B-4396-AC	00F-4396-AC	—	00F-4396-AF

3 µm, 4 µm & 5 µm Microbore and Minibore Columns (mm)						SecurityGuard [™] Cartridges (mm)	
Phases	50 x 1.0	150 x 1.0	250 x 1.0	50 x 2.0	150 x 2.0	250 x 2.0	4 x 2.0*
5 µm C4 300 Å	00B-4167-A0	00F-4167-A0	00G-4167-A0	00B-4167-B0	00F-4167-B0	00G-4167-B0	AJ0-4329
5 µm C5 300 Å	—	—	—	00B-4052-B0	00F-4052-B0	00G-4052-B0	AJ0-4326
5 µm C18 300 Å	00B-4053-A0	00F-4053-A0	00G-4053-A0	00B-4053-B0	00F-4053-B0	00G-4053-B0	AJ0-4320
4 µm Proteo 90 Å	00B-4396-A0	00F-4396-A0	00G-4396-A0	00B-4396-B0	00F-4396-B0	00G-4396-B0	AJ0-6073
							/10pk
3 µm C18 300 Å	—	—	—	00B-4263-B0	00F-4263-B0	—	AJ0-4320

for ID: 2.0-3.0 mm

3 µm, 4 µm & 5 µm Analytical, Semi-Prep, and Preparative Columns (mm)						SecurityGuard [™] Cartridges (mm)		
Phases	50 x 4.6	150 x 4.6	250 x 4.6	250 x 10	250 x 21.2	4 x 3.0*	10 x 10 [‡]	15 x 21.2**
5 µm C4 300 Å	00B-4167-E0	00F-4167-E0	00G-4167-E0	00G-4167-N0	00G-4167-P0	AJ0-4330	AJ0-7225	AJ0-7231
5 µm C5 300 Å	00B-4052-E0	00F-4052-E0	00G-4052-E0	00G-4052-N0	00G-4052-P0	AJ0-4327	AJ0-7371	—
5 µm C18 300 Å	00B-4053-E0	00F-4053-E0	00G-4053-E0	00G-4053-N0	00G-4053-P0	AJ0-4321	AJ0-7224	AJ0-7230
4 µm Proteo 90 Å	00B-4396-E0	00F-4396-E0	00G-4396-E0	00G-4396-N0	—	AJ0-6074	AJ0-7275	—
						/10pk	—	—
3 µm C18 300 Å	—	00F-4263-E0	00G-4263-E0	—	—	AJ0-4321	—	—

for ID: 3.2-8.0 mm 9-16 mm 18-29 mm

10 µm Analytical, Semi-Prep, and Preparative Columns (mm)				SecurityGuard [™] Cartridges (mm)		
Phases	250 x 4.6	250 x 10	250 x 21.2	4 x 3.0*	10 x 10 [‡]	15 x 21.2**
C4 300 Å	00G-4168-E0	00G-4168-N0	00G-4168-P0	AJ0-4330	AJ0-7225	AJ0-7231
C5 300 Å	00G-4054-E0	—	—	AJ0-4327	—	—
C18 300 Å	00G-4055-E0	00G-4055-N0	—	AJ0-4321	AJ0-7224	AJ0-7230
Proteo 90 Å	00G-4397-E0	00G-4397-N0	—	AJ0-6074	AJ0-7275	—

for ID: 3.2-8.0 mm 9-16 mm 18-29 mm

15 µm Analytical, Semi-Prep, and Preparative Columns (mm)						SecurityGuard [™] Cartridges (mm)			
Phases	250 x 4.6	250 x 10	250 x 21.2	250 x 30	250 x 50	4 x 3.0*	10 x 10 [‡]	15 x 21.2**	15 x 30.0*
C4 300 Å	00G-4169-E0	00G-4169-N0	00G-4169-P0	—	00G-4169-V0	AJ0-4330	AJ0-7225	AJ0-7231	—
C18 300 Å	00G-4057-E0	00G-4057-N0	00G-4057-P0	00G-4057-U0	00G-4057-V0	AJ0-4321	AJ0-7224	AJ0-7230	AJ0-8313

for ID: 3.2-8.0 mm 9-16 mm 18-29 mm 30-49 mm



For Jupiter Proteo Axia[™] Packed Preparative columns, see p. 381

Ordering Information

Bulk Material			
10 µm Bulk Packings			
Phases	100 g	1 kg	10 kg
C4 300 Å	04G-4168	04K-4168	04M-4168
C5 300 Å	—	04K-4054	—
C18 300 Å	04G-4055	04K-4055	04M-4055
Proteo 90 Å	04G-4397	04K-4397	—

15 µm Bulk Packings				
Phases	100 g	1 kg	5 kg	10 kg
C4 300 Å	04G-4169	04K-4169	04L-4169	04M-4169
C18 300 Å	04G-4057	04K-4057	—	04M-4057



Effectively desalt acidic, basic, and neutral peptides with Strata[™]-X. See p. 58 for more information.



For SecurityGuard Cartridge Holders and Cartridges, see p. 326



For Column Heater (25-90 °C), see p. 408





guarantee

If Kinetex core-shell columns do not provide at least an equivalent separation as compared to a competing column of the same phase, return the column with the comparative data within 45 days for a FULL REFUND.

Performance Gains on Any LC System

- Achieve sub-2 μ m performance within HPLC backpressure limitations
- Substitute 3 μ m and 5 μ m columns for 2-3x higher efficiency
- Obtain higher throughput without sacrificing resolution
- Easy method transfer across LC system platforms
- Reduce solvent consumption with faster analysis
- Reach lower levels of detection and quantitation



Complete scalable solution from UHPLC to HPLC to PREP LC

	UHPLC	HPLC	PREP	
	✓			Incredible UHPLC efficiency and performance gains
	✓			20% higher efficiency than fully porous 1.7 μ m columns
	✓	✓		Achieve sub-2 μ m performance on HPLC and UHPLC systems
		✓		Instantly improve your pharmacopoeia (Ph. Eur. & USP) monographs that require 3.5 μ m particle size
		✓	✓	3 μ m or better efficiencies at 5 μ m pressures for HPLC and PREP LC methods

KINETEX | HPLC / UHPLC



For more information on Kinetex PREP LC applications, see pp. 379



Kinetex has earned the Gold Seal of Quality!
Learn more at:
www.phenomenex.com/Gold


Innovation in Particle Technology

Using sol-gel processing techniques that incorporate nano-structuring technology, a durable, homogenous porous shell is grown on a solid silica core. This highly optimized process combined with industry leading packing technology produces highly reproducible columns that generate extremely high plate counts.

SEM of Kinetex Core-Shell Particles



Cross Section of Kinetex Core-Shell Particle

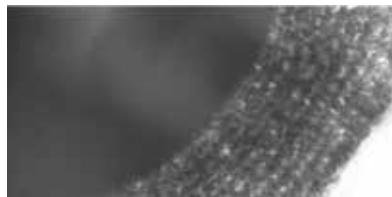

Optimized for Ultra-High Performance

High Efficiency, High Density Particle

Kinetex particles are built with a solid high density core that promotes the particles to settle into an optimal bed structure. This reduces the band broadening effects of Eddy Diffusion since the interstitial space between the particles is virtually homogeneous and results in ultra-high column efficiency and excellent reproducibility.

High Efficiency over Extended Range of Flow Rates

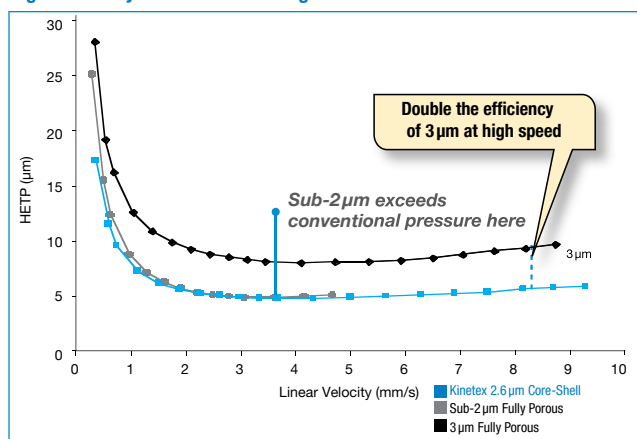


Illustration of Eddy Diffusion Effects

Kinetex Core-Shell

Fully Porous









Illustration - not actual test data.

Kinetex particles are nearly monodispersed. This extremely narrow particle size distribution results in increased column efficiency and excellent reproducibility.

Uniform Particle Size Distribution

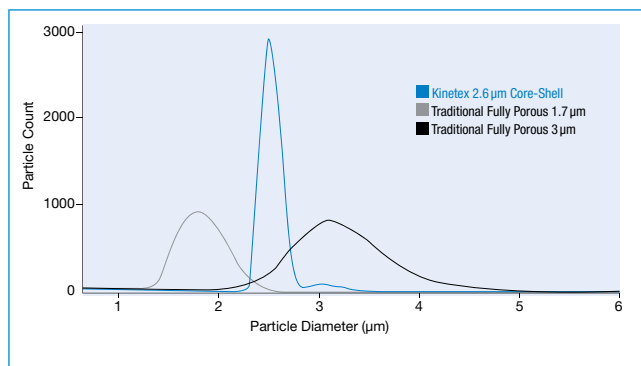


Batch-to-Batch Reproducibility Overlay

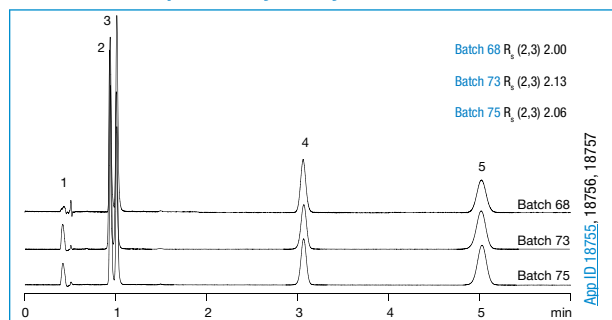

Conditions same for all batches:
Column: Kinetex 2.6 µm C18
Dimensions: 50 x 4.6 mm
Part No.: 008-4462-E0
Mobile Phase: Water / Acetonitrile (65:35)
Flow Rate: 1.0 mL/min
Detection: UV @ 254 nm
Sample: 1. Uracil
 2. Hydroxycortisone
 3. Cortisone
 4. Cortisone acetate
 5. 17-Hydroxyprogesterone


Achieve Sub-2 μ m Performance within HPLC Backpressure Limitations

With the efficiency of a sub-2 μ m column and typical operating backpressure less than 400 bar[†], you can achieve the promise of ultra-high performance on **any LC system**.

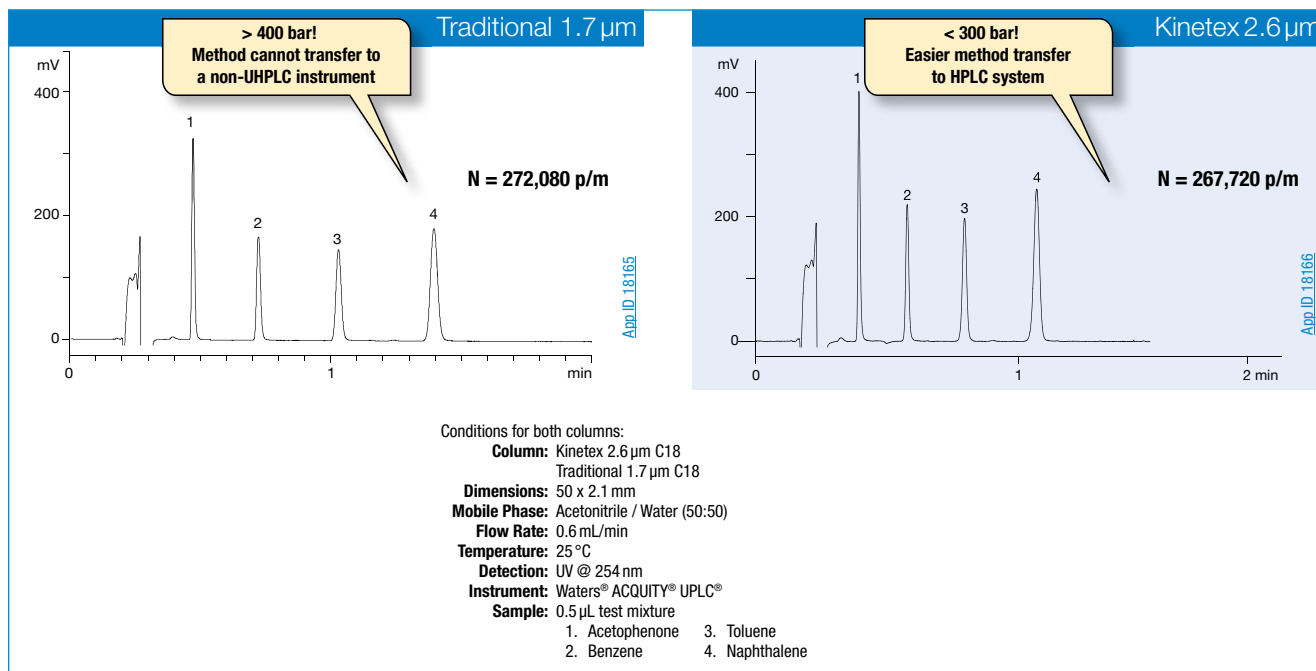

Unparalleled Levels of Ultra-High Performance

For users of higher pressure capable instruments who want increased levels of efficiency, we offer the Kinetex 1.7 μ m column—the first sub-2 μ m core-shell particle to be available on the market.

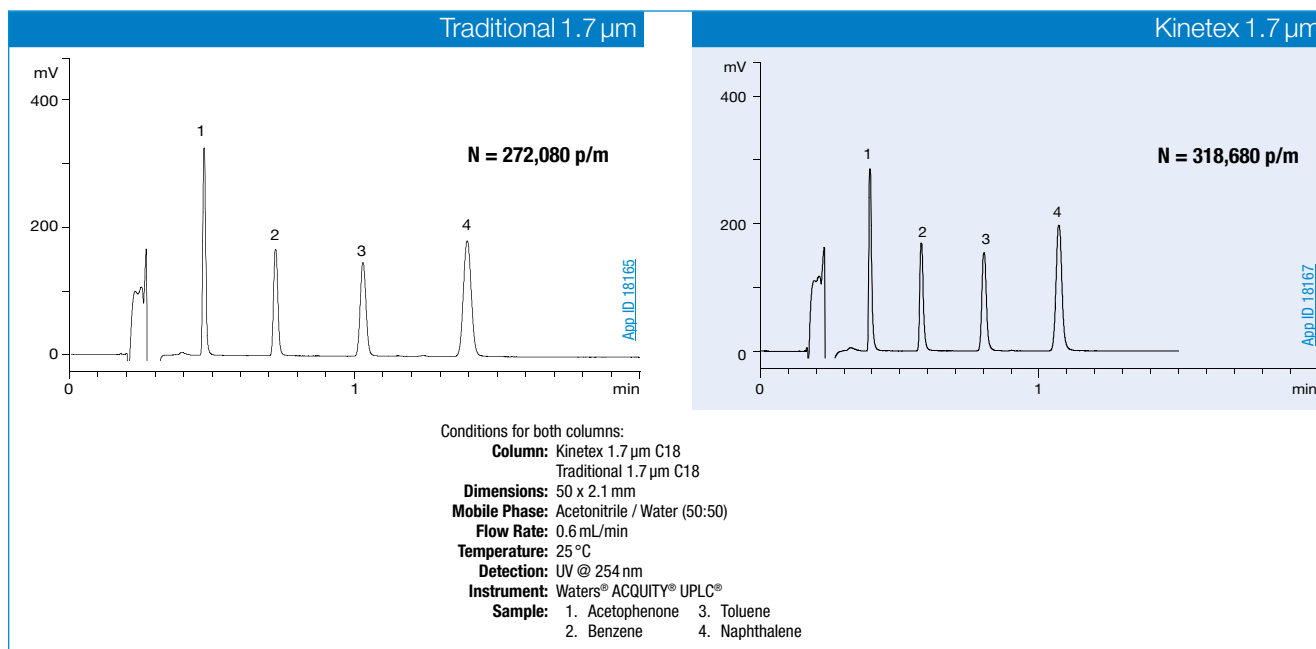


[†] Kinetex 2.6 μ m columns, 2.1 mm ID, are pressure rated to 1000 bar use on both HPLC and UHPLC instrumentation.

Comparative separations may not be representative of all applications.


Higher Resolution with No Pressure Increase

Replace traditional 3 and 5 μm columns with Kinetex 5 μm core-shell columns for immediate improvements in resolution, productivity, and sensitivity.

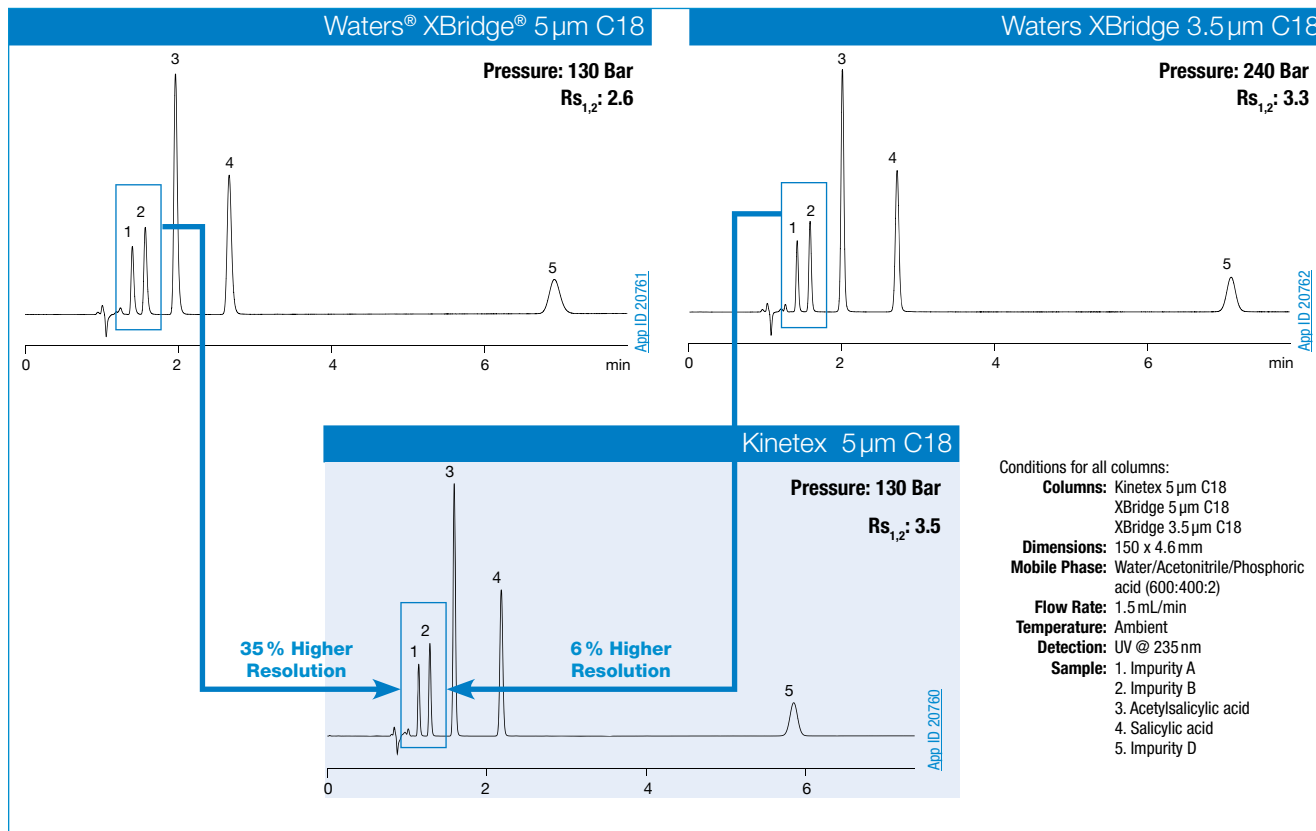

Enhanced Sensitivity at 5 μm Pressure

Kinetex 5 μm core-shell columns easily provide enhanced sensitivity on any HPLC system without an increase in backpressure.

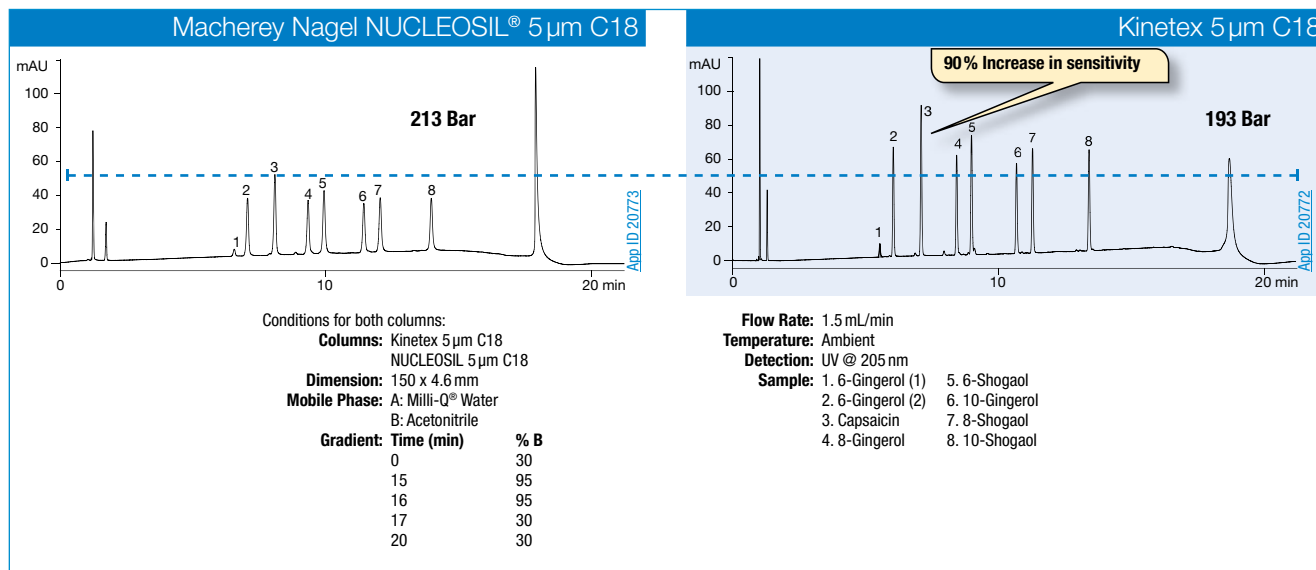




Comparative separations may not be representative of all applications.

Get the Most Performance Out of Your UHPLC System

Kinetex 1.3 μm , 1.7 μm , and 2.6 μm core-shell particles were engineered to provide incredible efficiency gains and improved performance compared to traditional fully porous sub-2 μm particles on UHPLC systems.

- Increase resolution, throughput, and sensitivity
- Save time and money
- 1.3 μm , 1.7 μm and 2.6 μm particles are directly scalable
- Available in C18, XB-C18, EVO C18, Polar C18, C8, Biphenyl, HILIC, Phenyl-Hexyl, and F5 phases (1.3 μm available in C18)

1.3 μm and 1.7 μm Kinetex core-shell columns are the FIRST and ONLY scalable sub-2 μm core-shell particles on the market, and produce up to 50% and 20% higher efficiencies respectively than sub-2 μm fully porous particles, taking UHPLC to the next level.

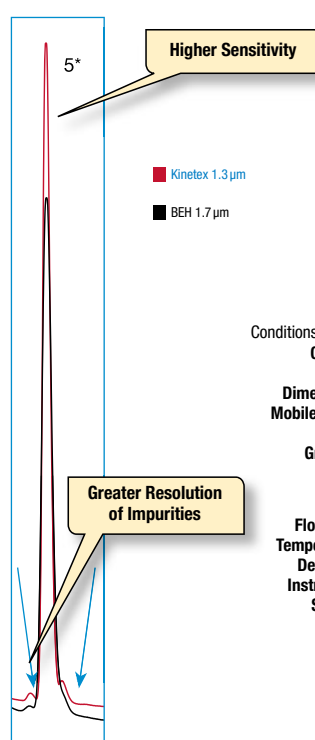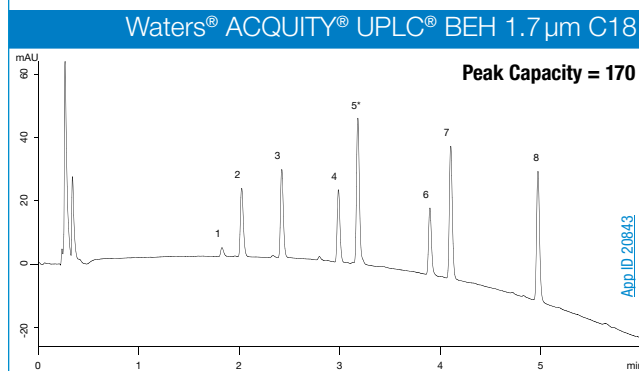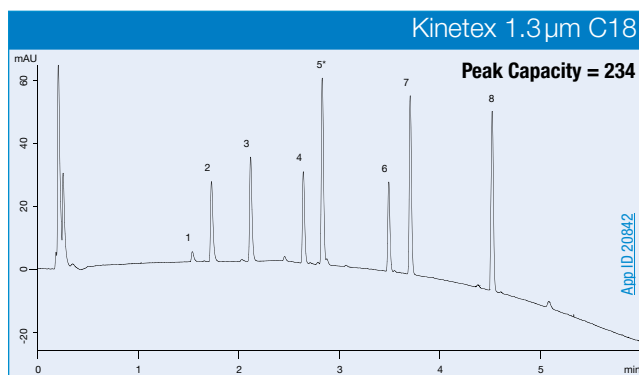

Conditions for both columns:

- Column:** Kinetex 1.3 μm C18
ACQUITY UPLC BEH 1.7 μm C18
- Dimensions:** 50 x 2.1 mm
- Mobile Phase:** A: 0.1% TFA in Water
B: 0.1% TFA in Acetonitrile
- Gradient:**

Time (min)	% B
0	30
5	95
- Flow Rate:** 0.5 mL/min
- Temperature:** Ambient
- Detection:** UV @ 214 nm
- Instrument:** Waters ACQUITY UPLC
- Sample:**
 1. 6-Gingerol (1)
 2. 6-Gingerol (2)
 3. Capsaicin
 4. 8-Gingerol
 5. 6-Shogaol
 6. 10-Gingerol
 7. 8-Shogaol
 8. 10-Shogaol



Comparative separations may not be representative of all applications.



for Kinetex 1.3 μ m UHPLC columns

Our New Standard for UHPLC

Bring your UHPLC analyses to the next level with the resolving power of Kinetex 1.3 μ m Core-Shell Technology. It's time you were able to see MORE!

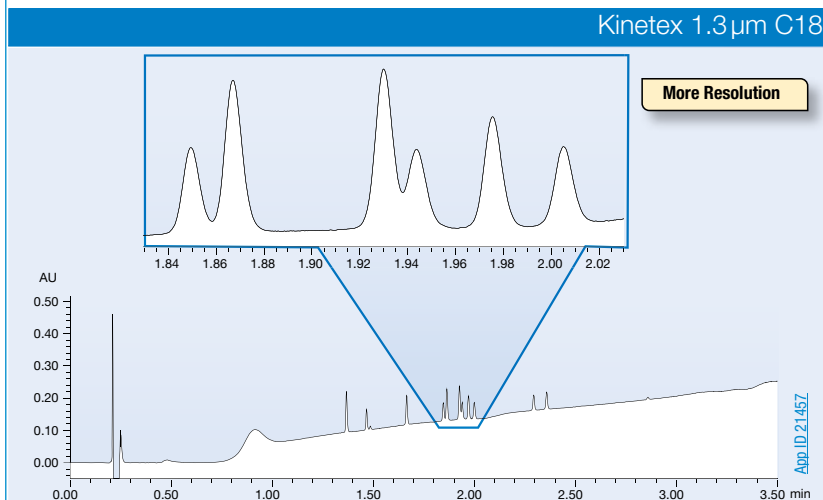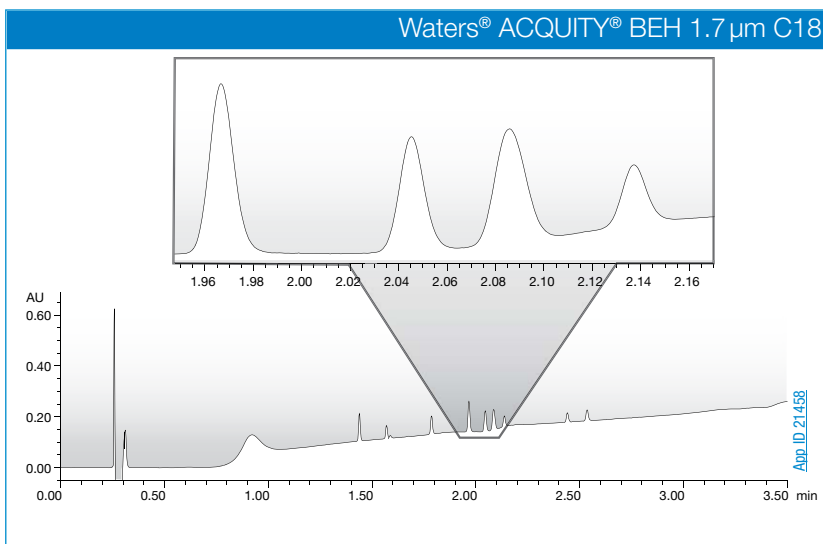

Conditions for all columns same except where noted:

Columns: Waters ACQUITY UPLC[®] BEH 1.7 μ m C18
Kinetex 1.3 μ m C18

Dimensions: 50 x 2.1 mm

Mobile Phase: A: 0.1% Formic Acid in Water
B: 0.1% Formic Acid in Acetonitrile

Gradient:	Time (min)	% B
	0	5
	3.0	95
	3.5	95
	3.6	5

Flow Rate: 0.5 mL/min

Temperature: Ambient

Detection: UV @ 254 nm

Instrument: Waters ACQUITY UPLC

Sample:


1. Estriol
2. Hydrocortisone
3. Corticosterone
4. Cortisone acetate
5. 17-beta-estradiol
6. 17-alpha-estradiol
7. 21-OH-progesterone
8. 17-alpha-ethynylestradiol
9. Estrone
10. Deoxycorticosterone acetate
11. Progesterone

Comparative separations may not be representative of all applications.


Kinetex[®] Core-Shell LC Columns

Analytical Scalability and Portability HPLC to UHPLC


UHPLC methods developed with fully porous sub-2 μm columns often generate backpressure higher than HPLC system limitations. With Kinetex 5 μm , 2.6 μm , 1.7 μm , and 1.3 μm core-shell technology, you are no longer restricted from developing high performance LC methods and transferring them anywhere. These four scalable Kinetex particle sizes offer you the ability to develop and transfer your method effortlessly from system to system.

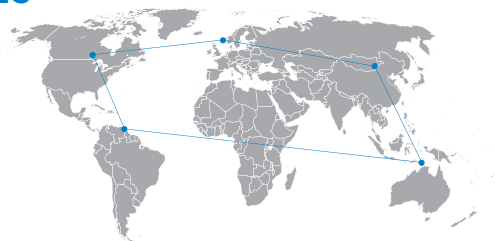


4 Kinetex particles give you full scalability HPLC \leftrightarrow UHPLC

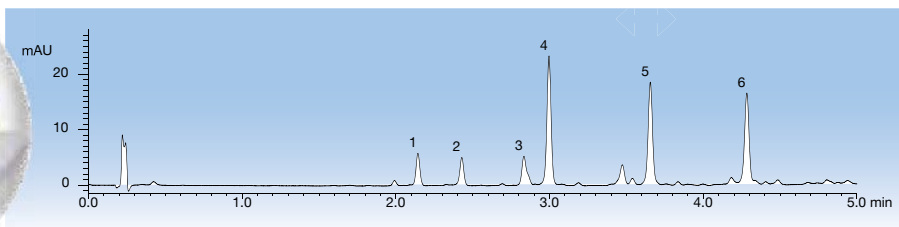

Kinetex 5 μm : 3 μm or better efficiencies at 5 μm pressures for HPLC and PREP LC methods

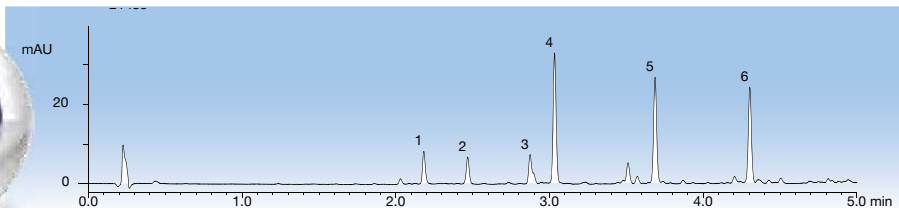


Kinetex 2.6 μm : Achieve sub-2 μm performance on HPLC and UHPLC systems

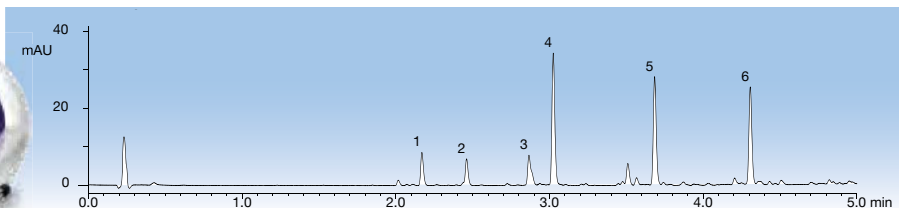

Kinetex 1.7 μm : 20% higher efficiency than fully porous 1.7 μm columns



for Kinetex 1.3 μm UHPLC columns

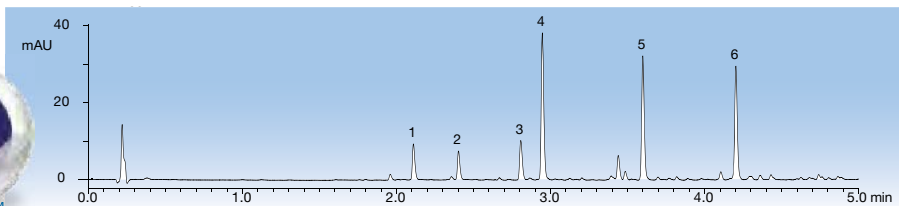

Kinetex 1.3 μm : Incredible UHPLC efficiency and performance gains


*Gingerols analyzed on 50x2.1 mm columns

Improve Performance, Save Solvent

When chromatographic column performance improves you can not only decrease your analysis time but also decrease your overall solvent consumption without compromising your separations. Use Kinetex core-shell technology to dramatically decrease the solvent consumption in your laboratory and increase sample throughput.

Column: Traditional 5 μ m C18
Dimensions: 250 x 4.6 mm
Flow Rate: 1.0 mL/min


Example Method Consumption

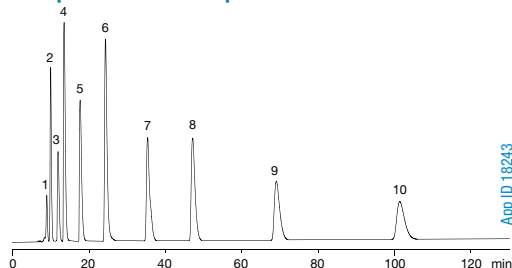

110 mL
solvent per run!

Column: Kinetex 2.6 μ m C18
Dimensions: 50 x 2.1 mm
Part No.: 00B-4462-AN
Flow Rate: 0.6 mL/min

Less Solvent Consumption with Kinetex Column

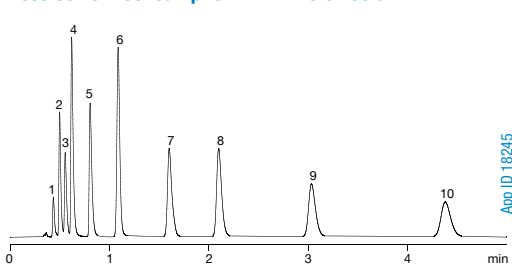

< 4 mL
solvent per run!

Conditions for both columns:

Mobile Phase: A: 20 mM Potassium phosphate pH 7
 B: Methanol / Acetonitrile (50:50)
 A/B (48:52)

Temperature: 40 °C

Detection: UV @ 254 nm


Sample:

- | | |
|---------------------|------------------|
| 1. Tianeptine | 6. Amoxapine |
| 2. Desmethyldoxepin | 7. Doxepin |
| 3. Protriptyline | 8. Nortriptyline |
| 4. Desipramine | 9. Amitriptyline |
| 5. Imipramine | 10. Clomipramine |

Reach Lower Levels of Detection and Quantitation

The combination of the small particle size, narrow particle size distribution, and the significantly shorter diffusion path results in much higher column efficiencies and increased chromatographic resolution. The increased efficiencies provide an immediate benefit on sensitivity since higher chromatographic efficiencies translate into significantly narrower and taller peaks, making it easier to detect low level impurities.


Agilent Technologies[®] ZORBAX[®] 3.5 μ m SB-C18

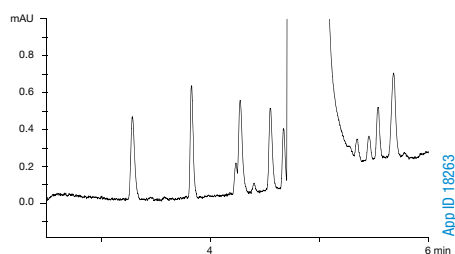

Conditions for both columns:

Dimensions: 150 x 4.6 mm
Mobile Phase: A: Water
 B: Acetonitrile
Gradient: (95:5) A/B for 1.16 min, then to (5:95) A/B
Flow Rate: 1.5 mL/min
Temperature: 45 °C
Detection: UV @ 254 nm
Instrument: Agilent 1200

Kinetex 2.6 μ m C18

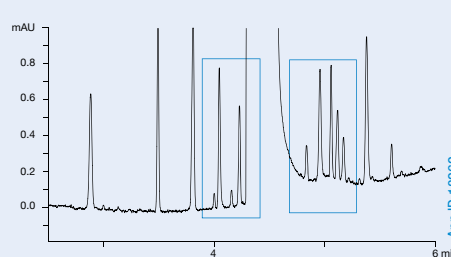






Sample:






- | | |
|---------------------|-------------------------------------|
| 1. Pyridine | 9. Nortriptyline |
| 2. Acetaminophen | 10. 4-Chlorobenzoic acid |
| 3. Pindolol | 11. 5-Methyl-2-hydroxy benzaldehyde |
| 4. Quinine | 12. 4-Chlorocinnamic acid |
| 5. Acebutolol | 13. Diazepam |
| 6. Chlorpheniramine | 14. Diflunisal |
| 7. Triprolidine | 15. Niflumic acid |
| 8. Prednisolone | 16. Hexanophenone |

Comparative separations may not be representative of all applications.

Complementary and Orthogonal Selectivities

To provide alternative and orthogonal selectivity phases, Kinetex columns are available in 10 selectivities: Polar C18, EVO C18, XB-C18, C18, C8, Biphenyl, Phenyl-Hexyl, F5, PAH, and HILIC (Hydrophilic Interaction Liquid Chromatography), for resolution of a wide range of compounds from polar to hydrophobic, aromatic, and isomers.

Kinetex Polar C18	Kinetex EVO C18	Kinetex XB-C18	Kinetex C18	Kinetex C8
				
Combined C18 and polar modified surface that provide polar and non-polar retention alongside 100% aqueous stability	Novel pH 1-12 stable C18 that delivers robust methods and improved peak shape for bases	This unique C18 phase yields increased hydrogen bonding with hydrophobic selectivity, resulting in improved peak shape for basic compounds and increased retention of acidic compounds	Balanced C18 phase that provides the highest degree of hydrophobic selectivity relative to the other Kinetex phases	Moderate hydrophobic and steric selectivity is offered, bringing ultra-high performance to USP L7 and other octyl silane methods
pH Range: 1.5 – 8.5* USP Classification: L1 Effective Carbon Load: 9%	pH Range: 1 – 12 USP Classification: L1 Effective Carbon Load: 11%	pH Range: 1.5 – 8.5* USP Classification: L1 Effective Carbon Load: 10%	pH Range: 1.5 – 8.5* USP Classification: L1 Effective Carbon Load: 12%	pH Range: 1.5 – 8.5* USP Classification: L7 Effective Carbon Load: 8%

Kinetex Biphenyl	Kinetex Phenyl-Hexyl	Kinetex F5	Kinetex HILIC	Kinetex PAH
				
100% aqueous stable reversed phase chemistry with hydrophobic, aromatic, and enhanced polar selectivity	Aromatic and moderate hydrophobic selectivity result in the great retention and separation of aromatic hydrocarbons	Highly reproducible pentafluorophenylpropyl phase, exceptional for halogenated, conjugated, isomeric, or highly polar compounds	Used under HILIC running conditions, this phase provides the highest polar selectivity for retention and separation of hydrophilic compounds	Polymerically bonded C18 phase specifically developed for the separation of EU and EPA priority PAHs
pH Range: 1.5 – 8.5* USP Classification: L11 Effective Carbon Load: 11%	pH Range: 1.5 – 8.5* USP Classification: L11 Effective Carbon Load: 11%	pH Range: 1.5 – 8.5 USP Classification: L43 Effective Carbon Load: 9%	pH Range: 2.0 – 7.5 USP Classification: L3 Carbon Load: –	pH Range: 1.5 – 8.5* USP Classification: – Carbon Load: 12%

*Columns are pH stable from 1.5-10 under isocratic conditions. Columns are pH stable 1.5-8.5 under gradient conditions.

Selecting The Right Chemistry

Use the charts below to determine the best Kinetex core-shell chemistry for your work.

Recommended Selectivities If You're Working With:

Acids	Bases	Neutrals	Aromatics	Acids, Bases, and Neutrals	Highly Polar Compounds	High pH	Isomers
C18	EVO C18	C18	Biphenyl	Polar C18	Polar C18	EVO C18	F5
F5	XB-C18	C8	Phenyl-Hexyl	Biphenyl	F5		
Phenyl-Hexyl	Biphenyl Polar C18	Biphenyl	F5	EVO C18 F5	Biphenyl HILIC		

Column Characteristics

Kinetex Phases	Shipping Solvent†	Particle Sizes (µm)	Pore Size (Å)	Surface Area (m ² /g)	Carbon Load (%)	pH Stability	Reversed Phase	Normal Phase	HILIC	100% Aqueous Stable
Polar C18	Acetonitrile/Water (50:50)	2.6	100	200	9	1.5-8.5*	●			●
C18	Acetonitrile/Water (50:50)	1.3, 1.7, 2.6, 5	100	200	12	1.5-8.5*	●			
EVO C18	Acetonitrile/Water (45:55)	1.7, 2.6, 5	100	200	11	1-12	●			●
XB-C18	Acetonitrile/Water (50:50)	1.7, 2.6, 3.5, 5	100	200	10	1.5-8.5*	●			
C8	Acetonitrile/Water (45:55)	1.7, 2.6, 5	100	200	8	1.5-8.5*	●			
Biphenyl	Acetonitrile/Water (45:55)	1.7, 2.6, 5	100	200	11	1.5-8.5*	●			●
Phenyl-Hexyl	Acetonitrile/Water (45:55)	1.7, 2.6, 5	100	200	11	1.5-8.5*	●			
F5	Acetonitrile/Water (40:60)	1.7, 2.6, 5	100	200	9	1.5-8.5*	●		●	●
HILIC	Acetonitrile/ 100 mM Ammonium Formate (93:7)	1.7, 2.6, 5	100	200	0	2.0-7.5		●	●	
PAH	Acetonitrile/Water (65:35)	3.5	—	—	12	1.5-8.5*	●			

† Shipping conditions may vary slightly in terms of organic to aqueous ratio, depending on column dimensions.
* pH stability under gradient conditions. pH stability is 1.5-10 under isocratic conditions.

Draw it. Find it.
Application search by
compound structure!





www.phenomenex.com/application/structuresearch

Kinetex[®] Core-Shell LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

Kinetex EVO C18

- Develop robust methods from pH 1-12
- Get improved peak shape for bases
- Easily reduce run times and increase sensitivity

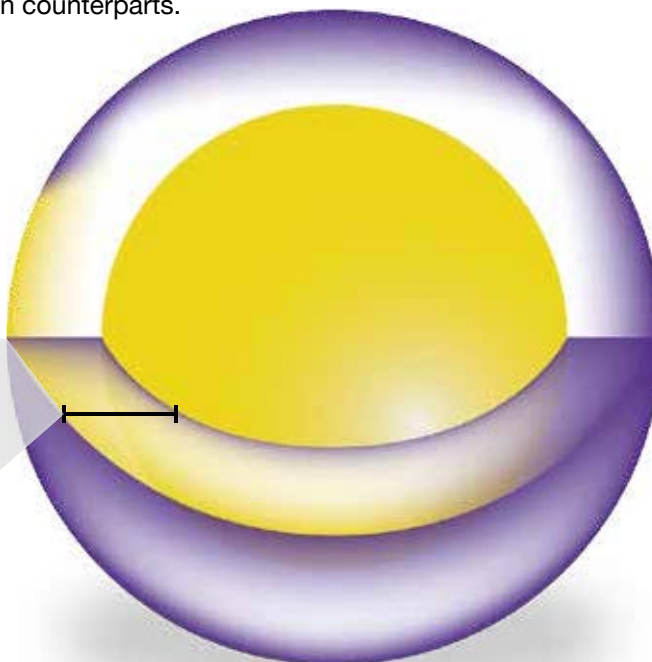
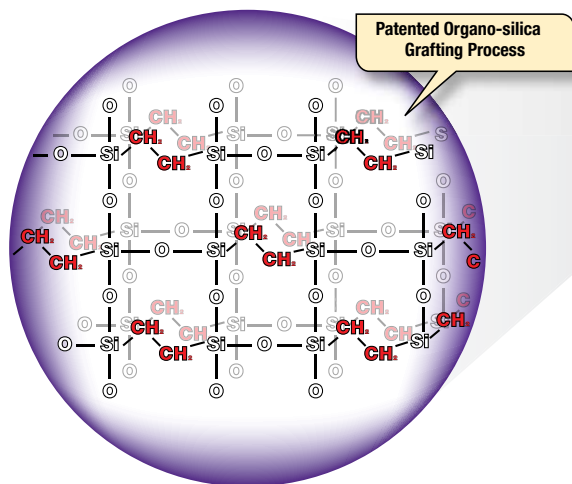


Kinetex EVO C18 uses a patented organo-silica grafting process which incorporates uniform stabilizing ethane cross-linking to provide resistance to high pH attack while maintaining mechanical strength of the core-shell particle.

Marvelous Peak Shapes for Bases

The unique organo-silica layer of ethane cross-linking found within each Kinetex EVO C18 particle creates a highly inert surface which provides the additional benefit of better peak shape for bases.

KINETEX | HPLC/UHPLC

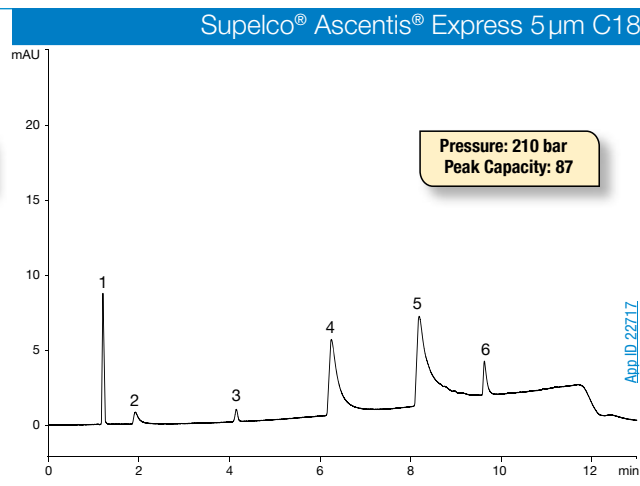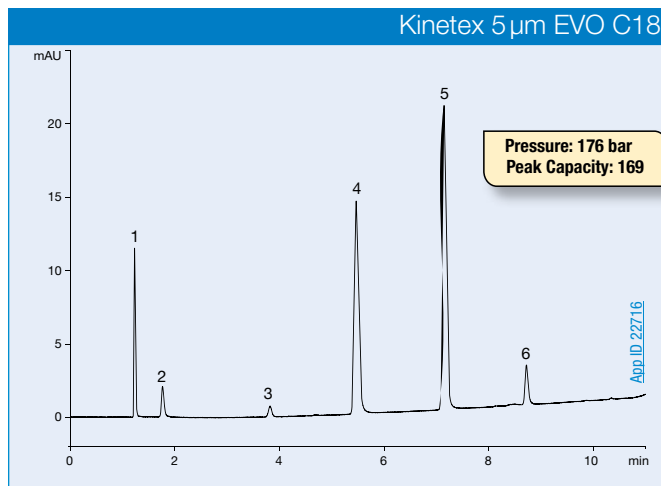

Conditions for both columns:
Column: Kinetex 5 μm EVO C18
 Ascentis Express 5 μm C18
Dimensions: 150 x 4.6 mm
Mobile Phase: A: 20 mM Sodium phosphate dehydrate pH 7.0
 B: Methanol
Gradient: 40% to 90% B over 10 minutes
Flow Rate: 1 mL/min

Temperature: Ambient
Detection: UV @ 254 nm
Sample: 1. Maleate
 2. Pseudoephedrine
 3. Scopolamine
 4. Doxylamine
 5. Chlorpheniramine
 6. Diphenhydramine


Comparative separations may not be representative of all applications.

Kinetex[®] Core-Shell LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

Drop in a Kinetex EVO 5µm Column to Start Smiling


With the combination of rugged pH stability from 1-12 and the core-shell performance advantage, you can easily replace old hybrid silica columns and gain immediate method improvements without increasing backpressure.

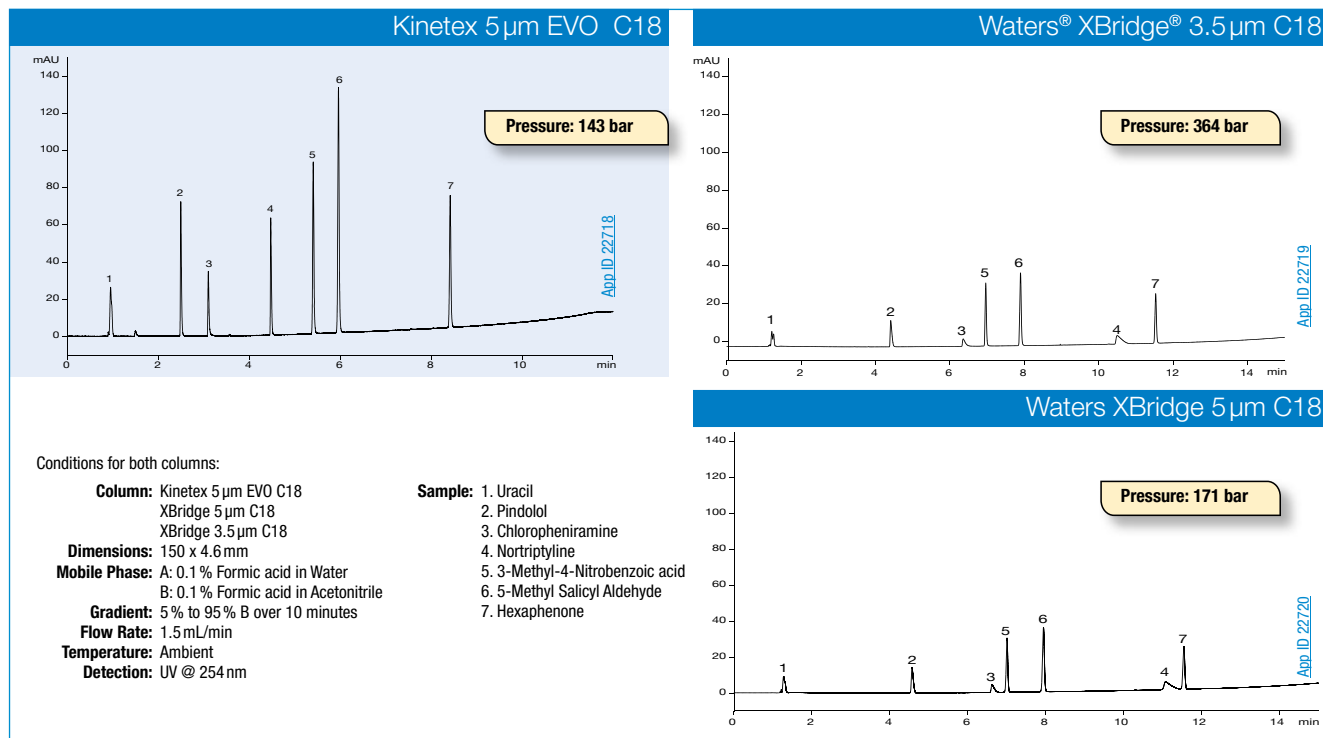

Comparative separations may not be representative of all applications.

Increased Sensitivity for LC-MS Applications

Alongside LC-UV analyses, the high performance and low pressure of the Kinetex EVO 5µm make it a tremendous tool for LC-MS and LC-MS/MS. Increased polar basic retention provided by the Kinetex EVO allows for greater use of organic within the mobile phase, subsequently leading to improved ionization and increased sensitivity.

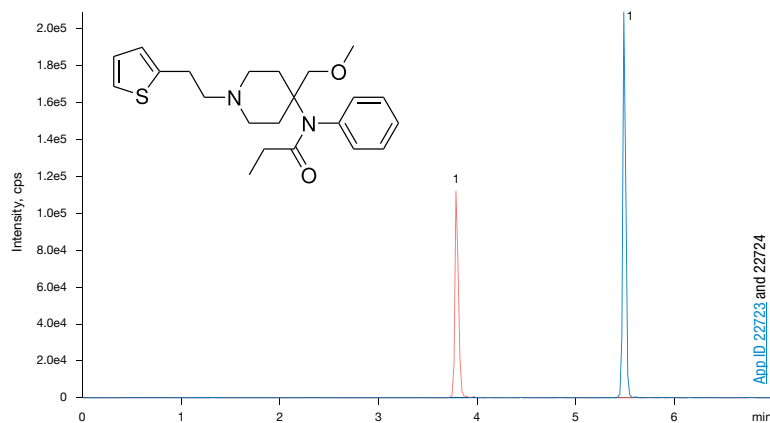

Column: Kinetex 5µm EVO C18

Dimensions: 50 x 2.1 mm

Part No.: [00B-4633-AN](#)

Mobile Phase: A: 0.1% Formic acid in Water
B: 0.1% Formic acid in Methanol

Mobile Phase: A: 10 mM Ammonium Bicarbonate (pH 8.2)
B: Methanol

Gradient: Time (min)	% B
0	10
0.5	10
2	25
4.5	80
4.51	85
5.5	85
5.51	10
7	10

Flow Rate: 0.5 mL/min

Temperature: Ambient

Detection: MS/MS (SCIEX API 4000™)

Sample: 1. Sufentanil


Kinetex[®] Core-Shell LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

A Simple Upgrade for Potential Greater Performance!

For scientists who are interested in high performance and fast run times, 2.6 μ m Kinetex EVO C18 columns are an amazing UHPLC solution. Start by matching a Kinetex 2.6 μ m column to the sub-2 μ m column you're currently using. With lower backpressure

and similar or better performance, you'll then have three options: keep the lower pressure for less system strain, increase the flow for higher productivity, or utilize a longer column length to increase potential resolving power.

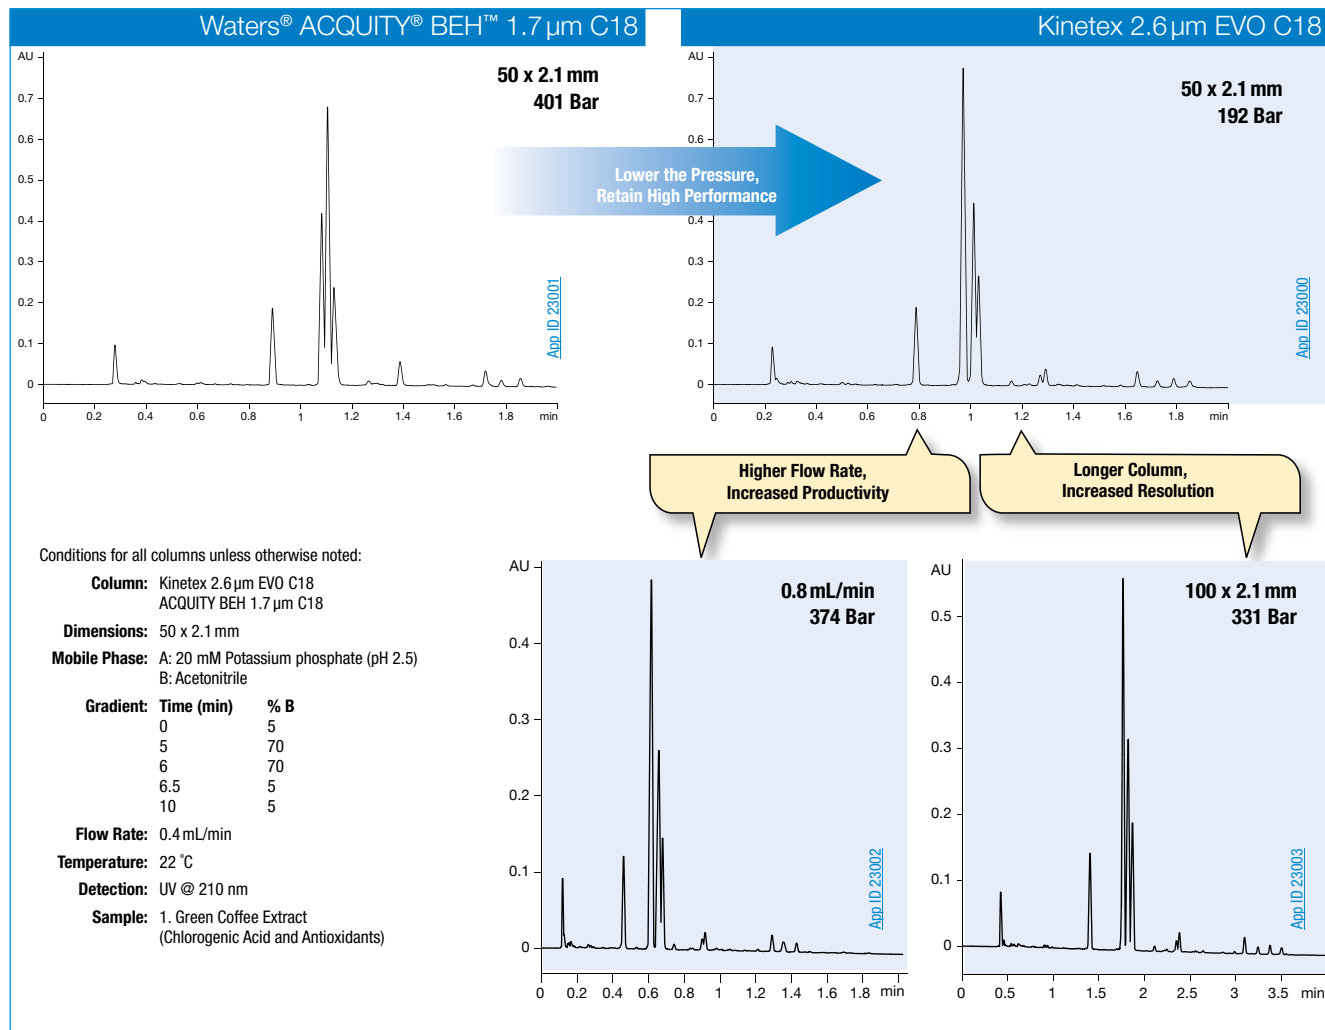

Comparative separations may not be representative of all applications.


Kinetex[®] Core-Shell LC Columns

U.S. Patent Nos. 7, 563, 367 and 8, 658, 038 and foreign counterparts.

More Performance, Excelling Quality

Here's an illustration of just how powerful a tool the Kinetex 1.7 μ m EVO C18 is. In comparison with multiple batches of a common hybrid sub-2- μ m column line, Kinetex EVO C18 columns show

consistently greater performance and better peak shape for basic compounds. This level of quality is what we strive to give you every day with every batch, every column, and even every phone call.

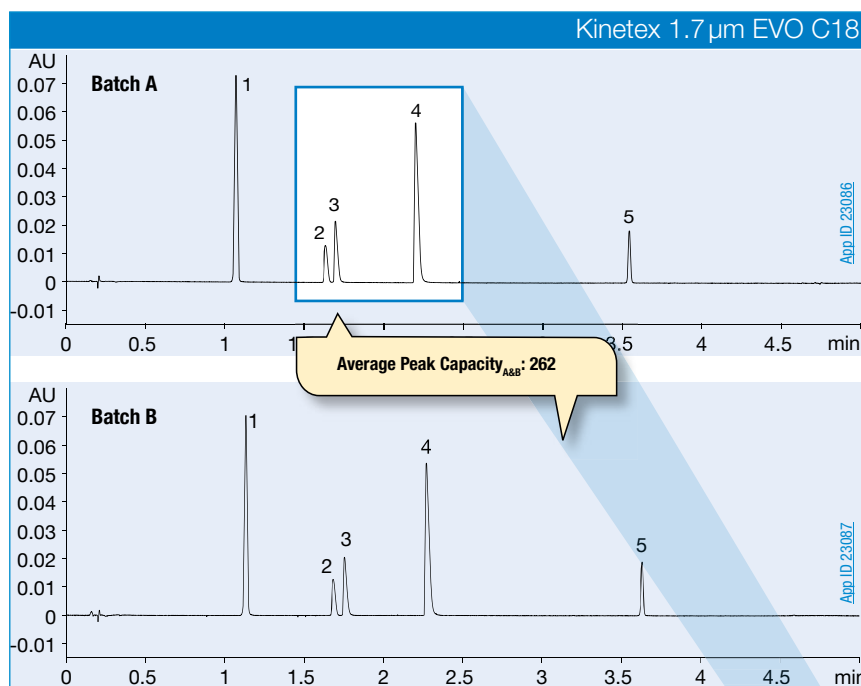

Conditions for both columns:

Column: Kinetex 1.7 μ m EVO C18
ACQUITY BEH 1.7 μ m C18

Dimensions: 150 x 2.1 mm

Mobile Phase: A: 0.1 % Formic Acid in Water
B: 0.1 % Formic Acid in Acetonitrile


Gradient Time (min)	% B
0	5
5	95
6	95
6.5	5
10	5

Flow Rate: 0.5 mL/min


Temperature: 22 °C

Detection: UV @ 254 nm

Sample: 1. 4-Hydroxybenzoic Acid
2. Labetol
3. Propranolol
4. Protriptyline
5. Ibuprofen

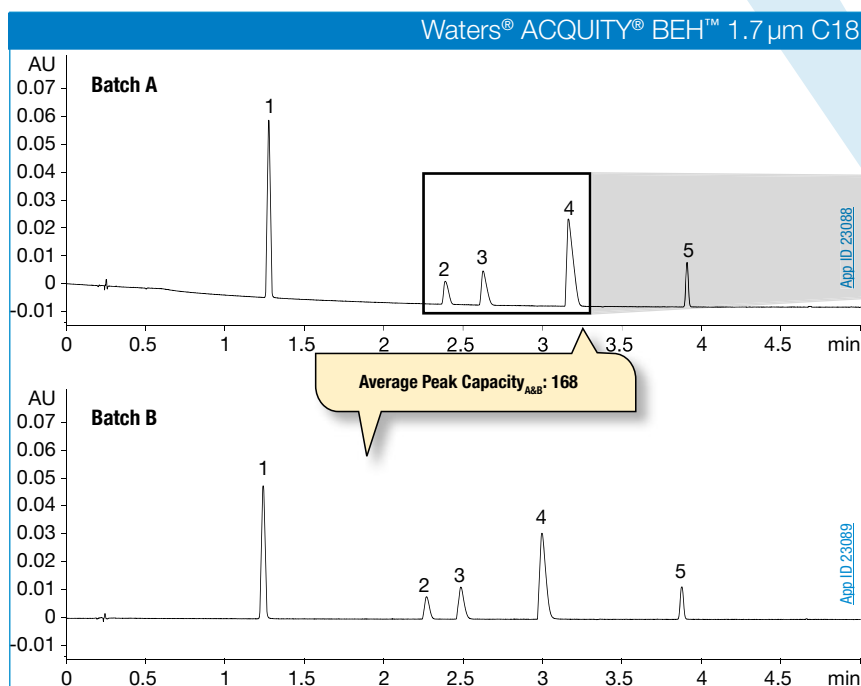

Wow!
Look at my improved
peak shape for bases!



Comparative separations may not be representative of all applications.


Kinetex Polar C18

- 100% aqueous stable
- Enhanced selectivity for polar analytes
- Orthogonal selectivity to traditional C18 phases

A Versatile C18


Who said all C18's are the same? By combining C18 ligands with a polar-modified surface, you can now achieve greater retention of polar and nonpolar compounds while ensuring 100% aqueous stability.

Kinetex Polar C18

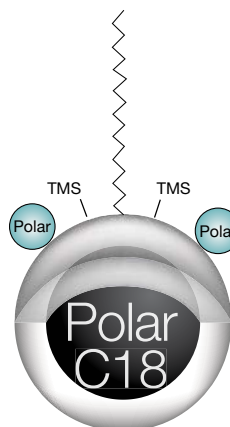


Acids, Bases, and Neutrals

Kinetex 2.6 μ m Polar C18

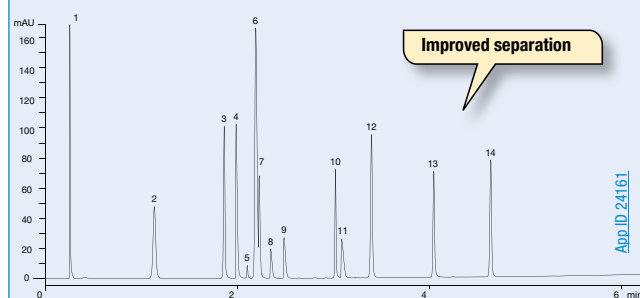

Thermo Scientific[®] 3 μ m Hypercarb[®]

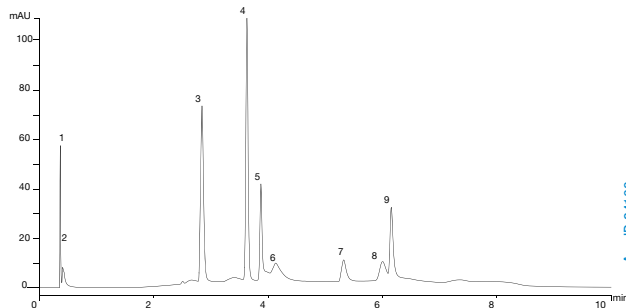

Conditions for both columns:

Columns:	Kinetex 2.6 μ m Polar C18	Thermo Scientific 3 μ m Hypercarb
Dimensions:	50 x 4.6 mm	
Mobile Phase:	A: 0.1% Formic acid in Water B: 0.1% Formic acid in Acetonitrile	
Gradient:	Time (min)	% B
	0	5
	0.5	5
	5.5	95
	7.51	5
	10	5

Flow Rate:	1.85 mL/min	
Temperature:	Ambient	
Detection:	UV @ 254 nm	
Sample:	1. Pyridine	8. Chlorpheniramine
	2. Acetaminophen	9. Triprolidine
	3. Sulfathiazole	10. Prednisolone
	4. Quinidine	11. Nortriptyline
	5. Quinidine Impurity	12. 5MSA
	6. Phenol	13. Diflunisal
	7. Acebutolol	14. Hexanophenone


Comparative separations may not be representative of all applications.

Enhanced Polar Selectivity

The Kinetex Polar C18 contains a C18 ligand alongside a polar modified surface that increases polar compound retention and improves resolution values. Additionally, the advanced proprietary bonding technology used with this phase ensures 100% aqueous stability as well as balanced retention on non-polar compounds.


This is an excellent all purpose phase for use with multi-compound mixes that contain polar and nonpolar compounds, or even single class methods that have closely related compounds, impurities, or metabolites.

UHPLC Analysis of Cyclosporine and Impurities

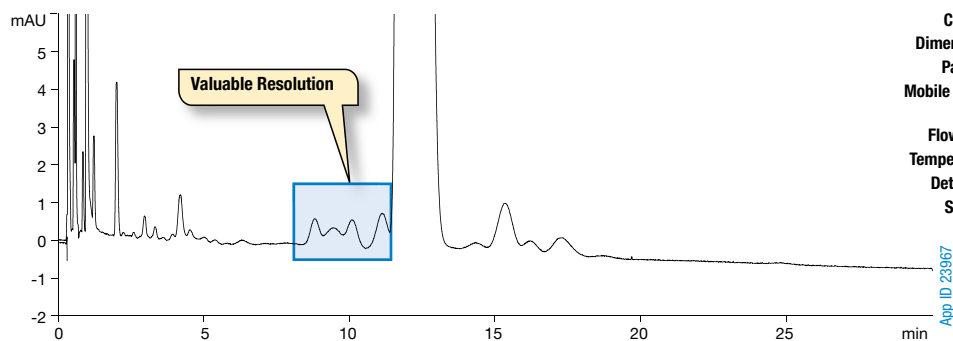

Column: Kinetex 2.6 μ m Polar C18
Dimensions: 50 x 2.1 mm
Part No.: [00B-4759-AN](#)
Mobile Phase: Acetonitrile/Tert-butyl methyl ether/
 Water/Phosphoric acid (430:50:520:1)
Flow Rate: 0.30 mL/min
Temperature: 80 °C
Detection: UV @ 210 nm
Sample: Cyclosporine

Water Soluble Vitamins

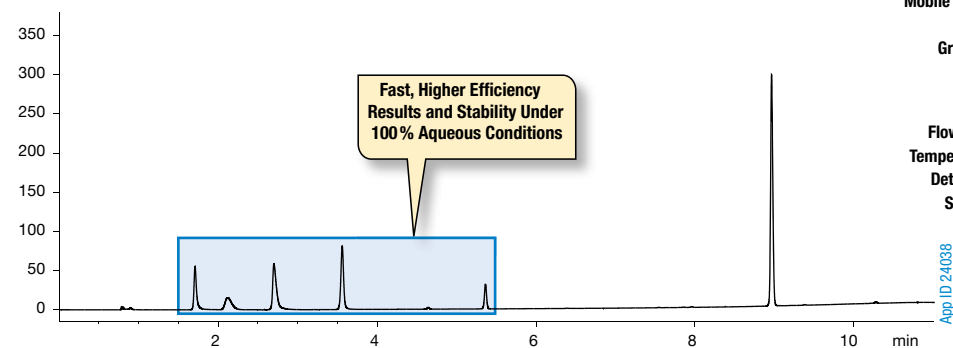


Column: Kinetex 2.6 μ m Polar C18
Dimensions: 100 x 4.6 mm
Part No.: [00D-4759-E0](#)
Mobile Phase: A: 20 mM Potassium Phosphate
 B: Methanol

Gradient:	Time (min)	% B
	0	0
	1	0
	10	60

Flow Rate: 1.2 mL/min
Temperature: Ambient
Detection: UV @ 210 nm
Sample: 1. Thiamine
 2. Nicotinamide
 3. Pyridoxal
 4. Pyridoxine
 5. Pantothenic Acid
 6. Riboflavin

Multi-Class 206 Pesticide Panel Screen

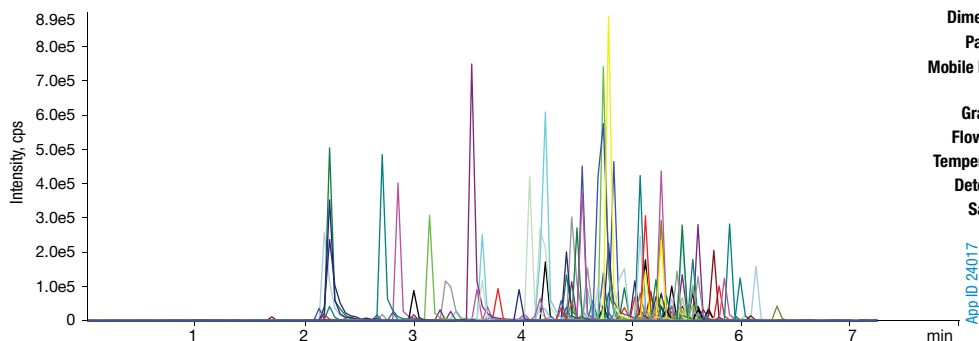

Column: Kinetex 2.6 μ m Polar C18
Dimension: 50 x 4.6 mm
Part No.: [00B-4759-E0](#)
Mobile Phase: A: Water
 B: 0.1% Formic Acid in Methanol
Gradient: 5-100% B in 5 min, hold 1 min
Flow Rate: 0.7 mL/min
Temperature: Ambient
Detection: MS/MS (SCIEX API 4000™)
Sample: 206 Pesticides.
 Find the full compound list online at
www.phenomenex.com/Application/Detail/24017

Kinetex Biphenyl

- Remarkable separation power
- Rugged and reliable
- 100% aqueous stable

Selectivity That a C18 Just Can't Give You!

Think high performance, enhanced retention, and the ability to go where a traditional C18 can't. The Kinetex Biphenyl offers the high performance benefits of a core-shell particle with a unique stationary phase capable of becoming the go-to selectivity for reversed phase method development. Use Kinetex Biphenyl columns to get enhanced retention, higher sensitivity, and overall better results; especially for aromatic compounds.

Aromatic Pi-Pi Interactions


Between aromatic rings and pi electrons of target molecule and the double aromatic rings of the Biphenyl ligand

Hydrophobic Interactions


Between carbon skeleton of Biphenyl ligand and target analytes

Weak Ionic or Dipole-Dipole Interactions

High electron density created by dual ring structure behaves similar to a weak cation exchanger, giving enhanced retention for basic analytes

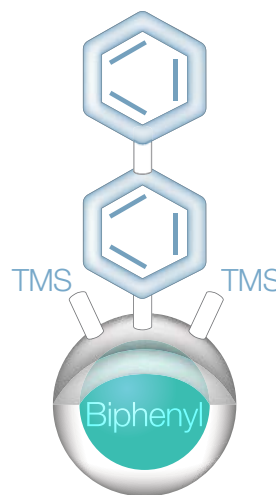

Mycotoxins

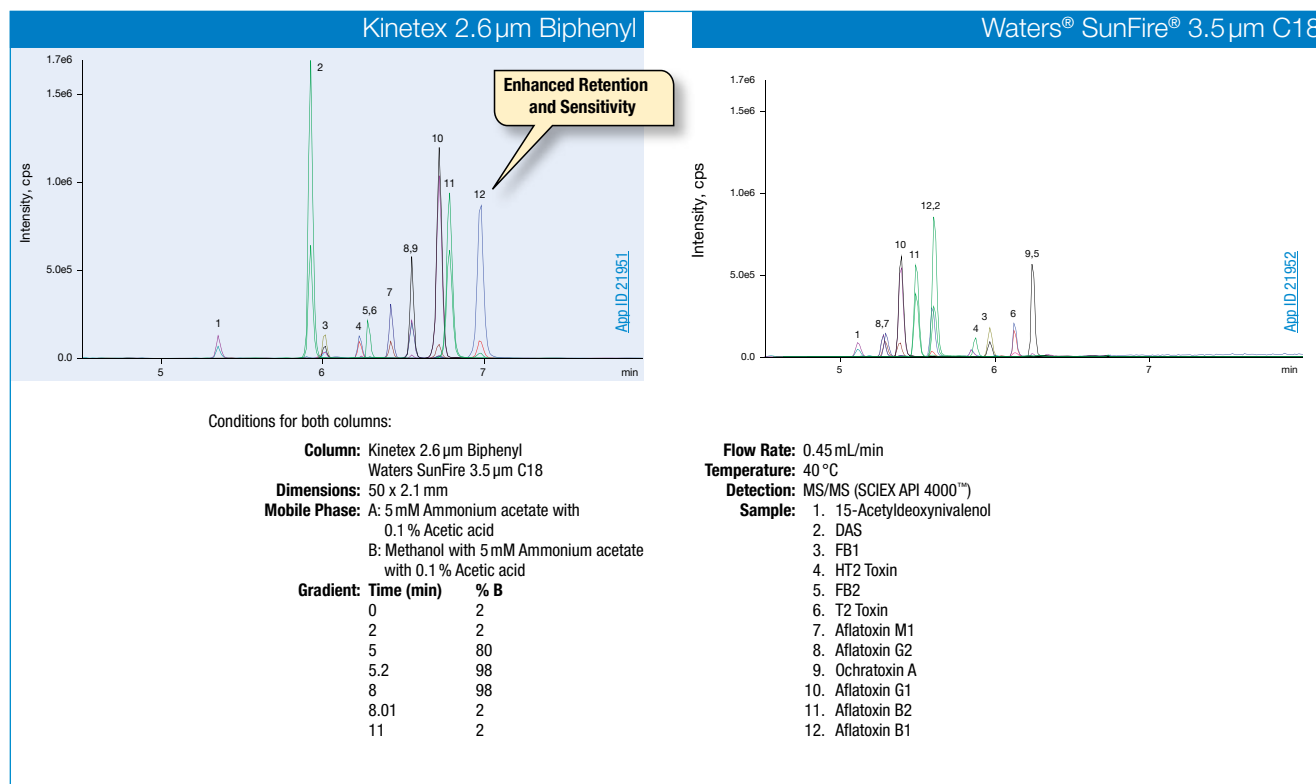


Comparative separations may not be representative of all applications.

Enhanced Separation Power

Kinetex Biphenyl is a high efficiency core-shell product capable of adding extra separation power to your analysis of non-polar and polar compounds.


Opiate Isomers

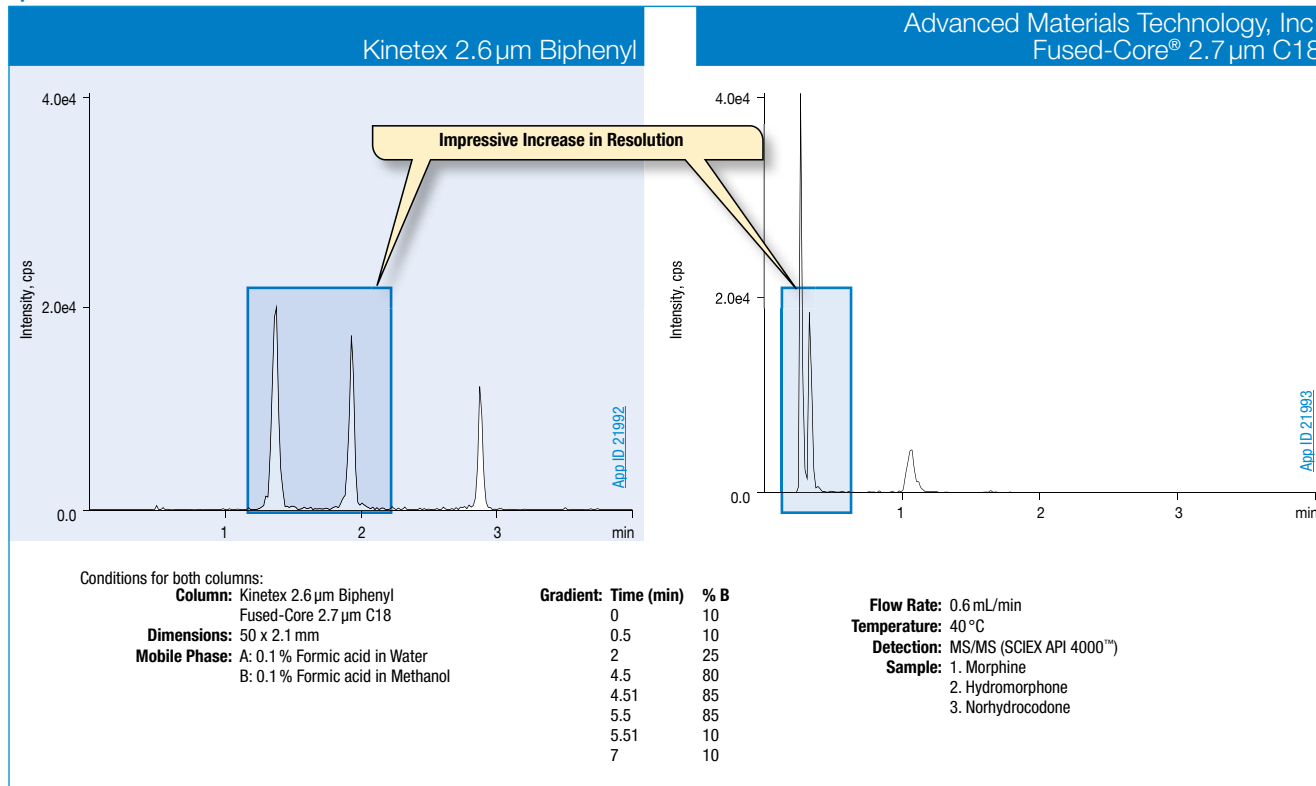

Comparative separations may not be representative of all applications.

Excel With Your Multi-Compound, Multi-Class Screening

Increase the separation and analytical power of your HPLC/UHPLC compound screens with the multi-functional Kinetex Biphenyl stationary phase.

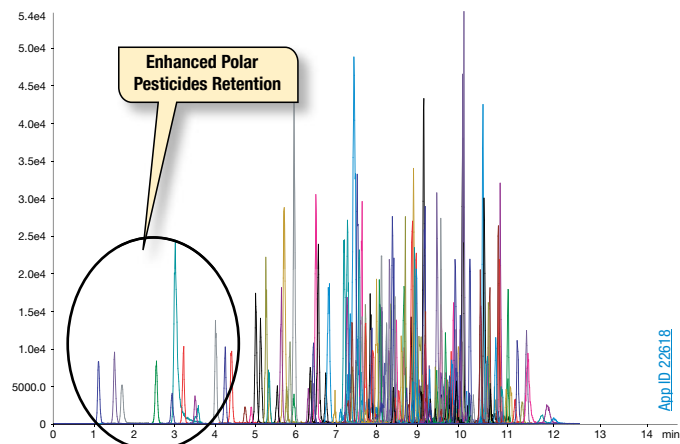

Column: Kinetex 5 μm Biphenyl
Dimensions: 100 x 2.1 mm
Part No.: [00D-4627-AN](#)
Mobile Phase: A: 5 mM Ammonium formate in Water
 B: 5 mM Ammonium formate in Methanol

Gradient:	Time (min)	% B	
	0.01	10	
	1	10	
	10	90	
	15	90	
	15.1	10	
	20	10	

Flow Rate: 0.5 mL/min
Temperature: 35 °C
Detection: Tandem Mass Spectrometer (MS/MS)
Detector: SCIEX 4500 QTRAP[®]
Sample: 175+ Pesticide Mix

Kinetex F5


- Reduce method development time by days
- Greater reproducibility than other PFPs
- 5 glorious interaction mechanisms
- 5 valuable LC separation modes

How I Work

With the astonishing combination of core-shell performance and 5 interaction mechanisms, Kinetex F5 columns will effortlessly drive your orthogonal HPLC/UHPLC development!

Method Development Versatility— 5 Separation Modes

- Reversed Phase
- HILIC
- SFC
- 2D-LC
- 100% Aqueous

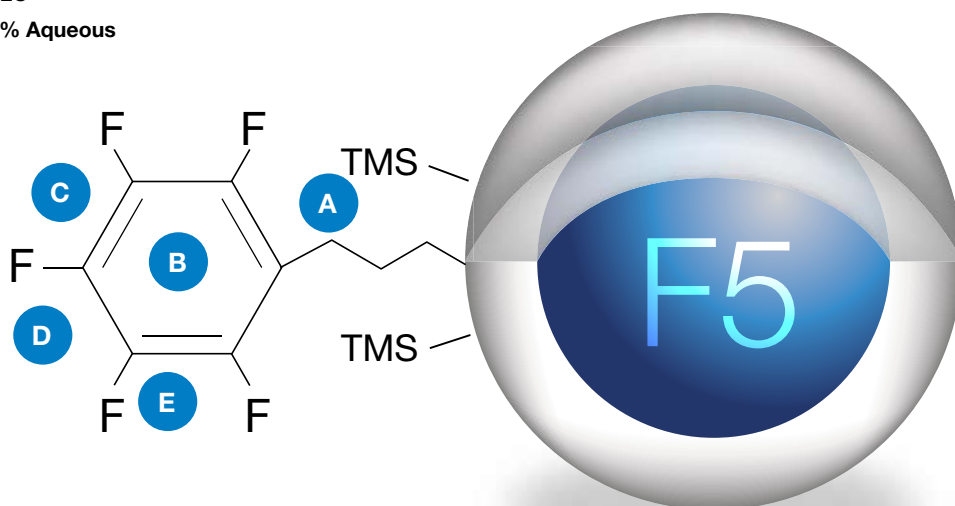


5 Interaction Mechanisms

- A Hydrophobic**
Carbon skeleton of linker and ring encourage neutral/hydrophobic retention
- B Aromatic**
In non-acetonitrile mobile phases, π - π electrons of the carbon ring interact with analyte π - π electrons and result in positive retention increase
- C Electrostatic**
High electronegativity of the fluorine groups create dipole moments, aiding in polar compound retention. Induced dipole moments can also aid neutral compound retention.
- D Steric/Planar**
Shape selectivity allows for isomeric separations that are otherwise impossible on traditional alkyl phases
- E Hydrogen Bonding**
Extremely effective retention mechanism caused as polar functional groups of analyte interact with the electron greedy fluorine

Dependability

Batch-to-Batch, Column-to-Column



Conventional fully porous and core-shell PFP/F5 columns fail to reach the level of repeatability that you deserve. Inconsistencies in their base silica have led to data inaccuracies that waste your time and money. Kinetex F5 columns were specifically designed to avoid these past problems and provide a high degree of reproducibility.

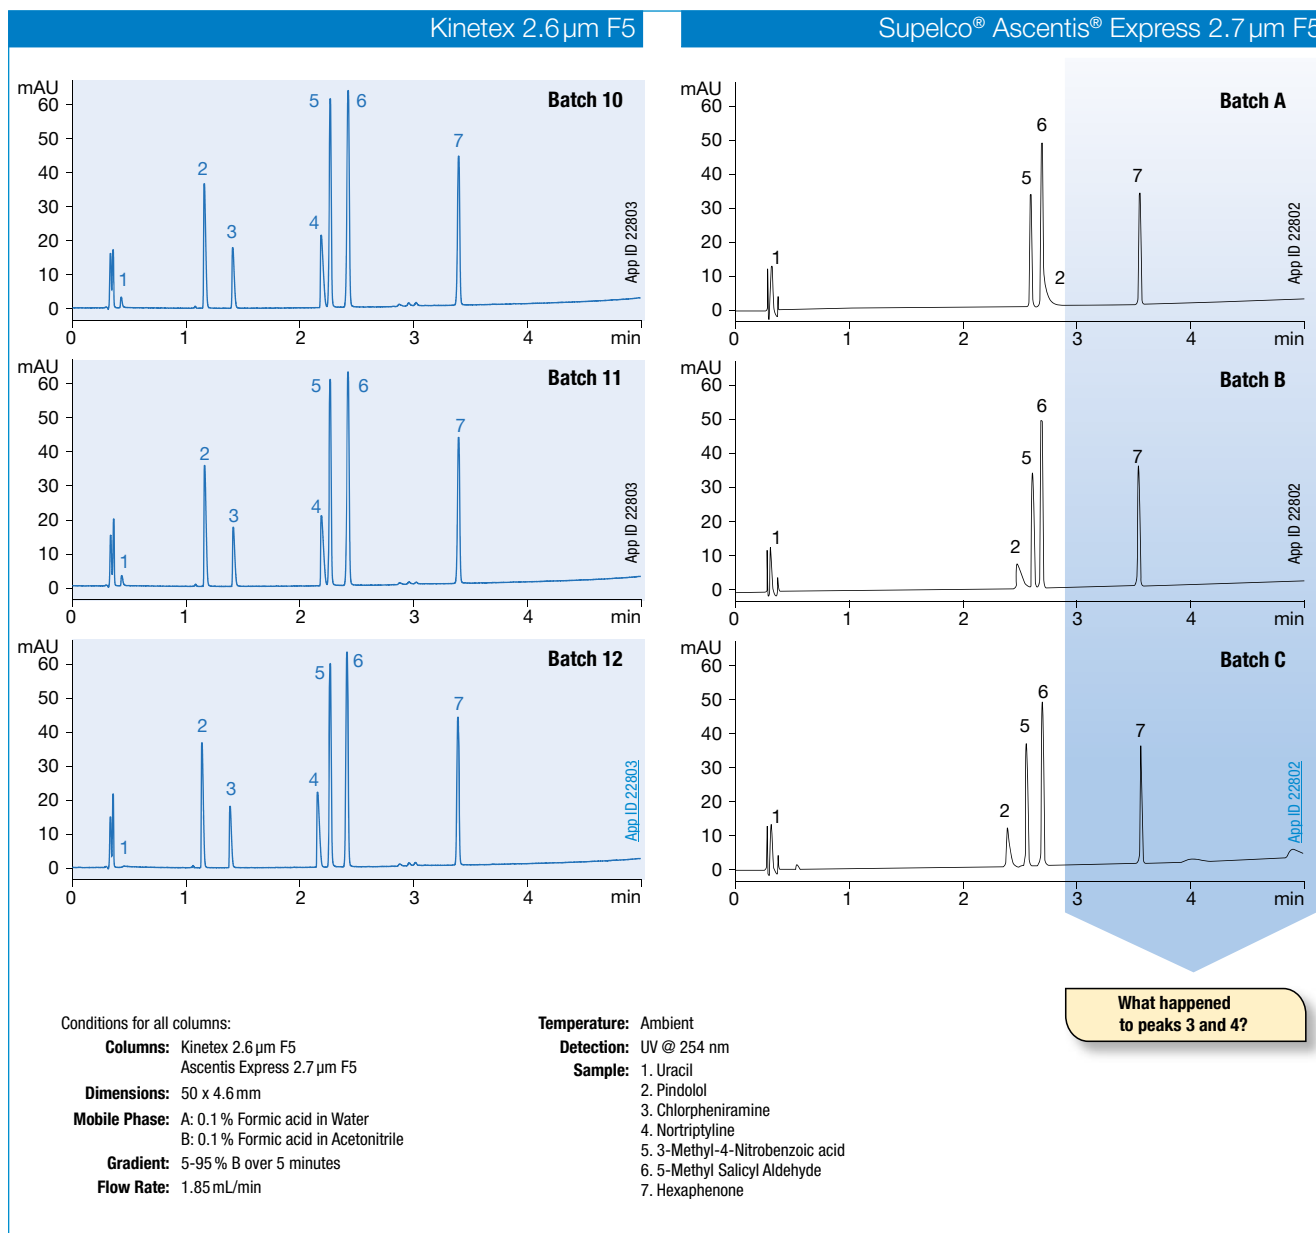


Comparative separations may not be representative of all applications.

Selectivities Built for Your Needs


The extensive range of Kinetex stationary phases allows you to get retention enhancement without performance loss. Use the multi-functional Kinetex Biphenyl or pH stable Kinetex EVO C18 to reach the desired solution for your method.

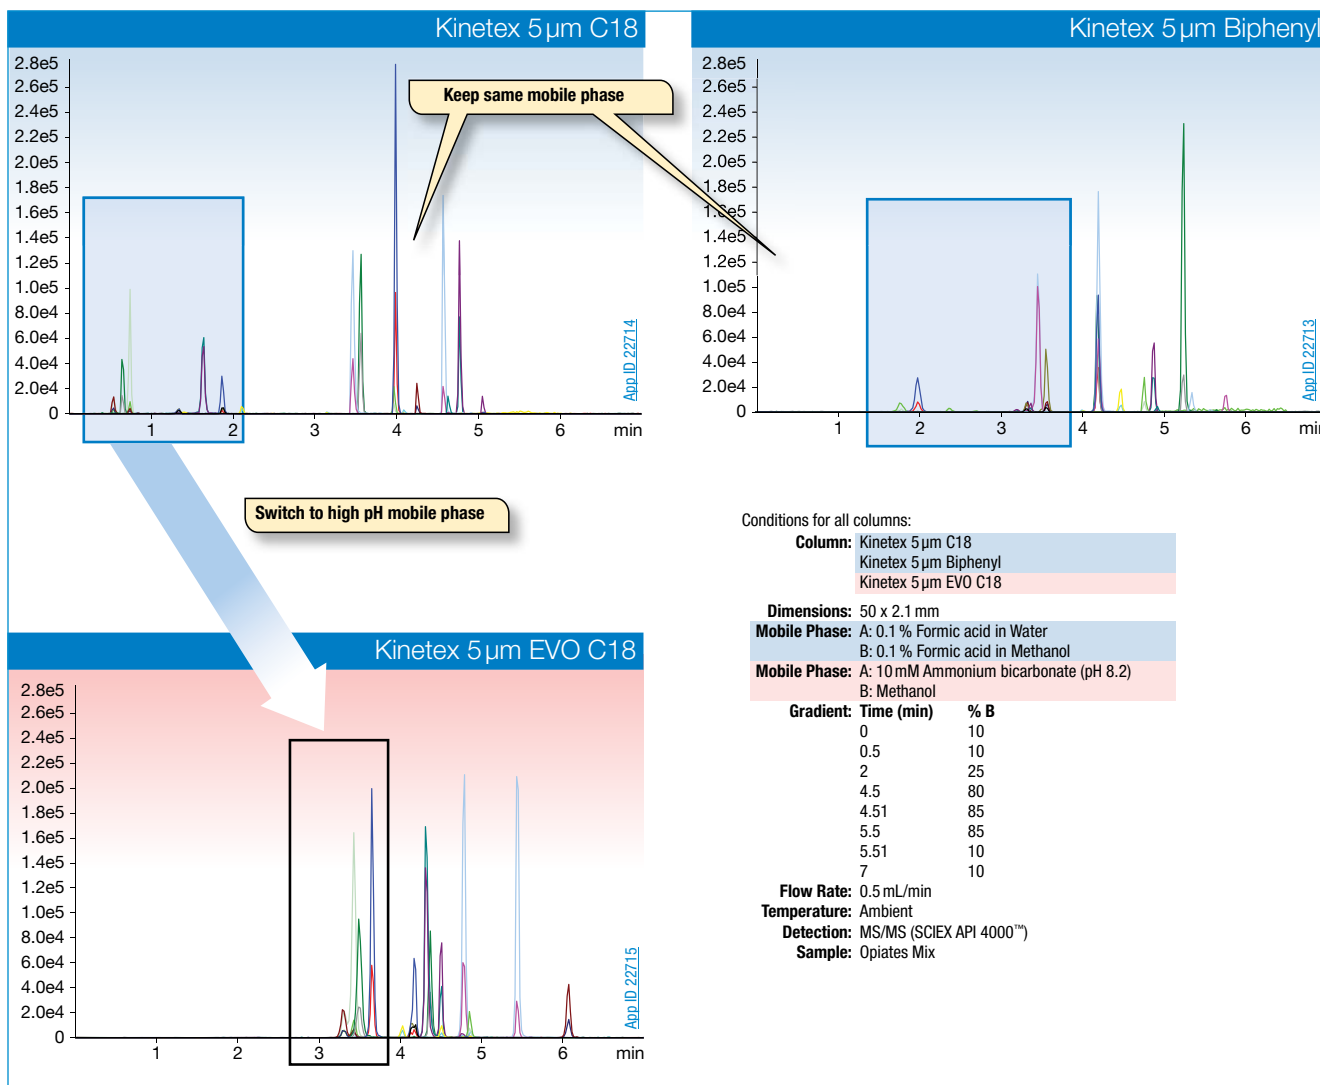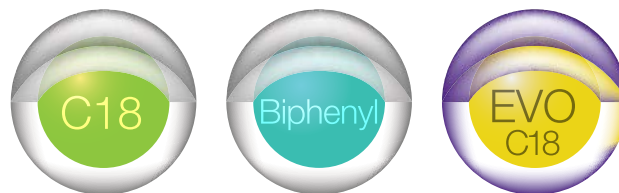


Veterinary Drugs

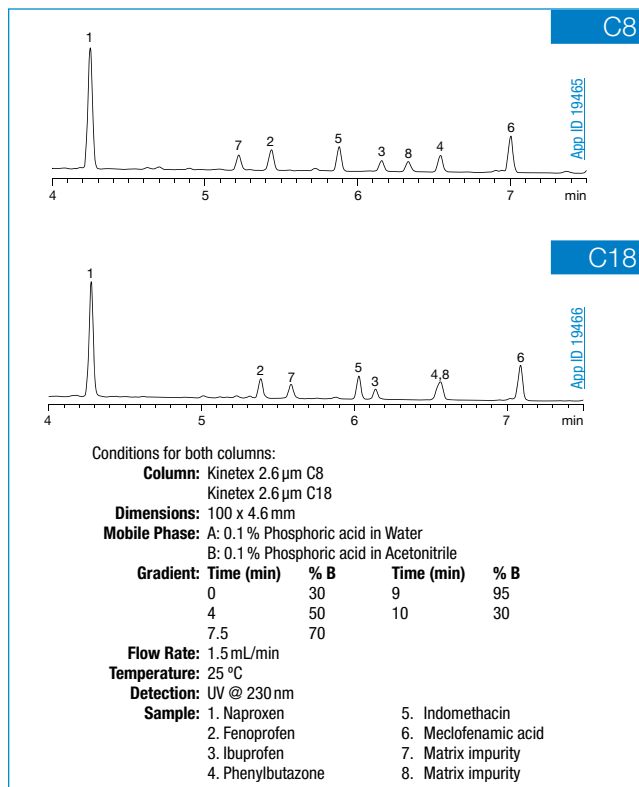


Steroids

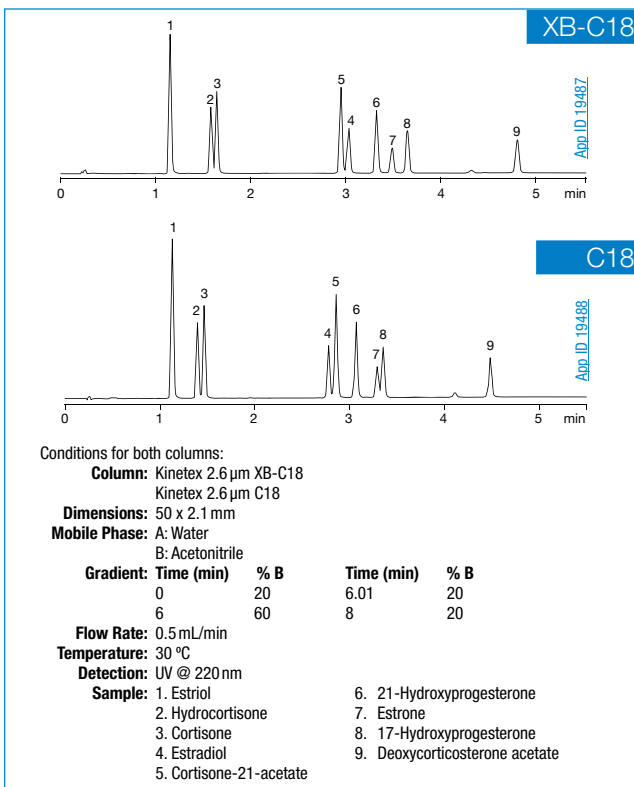

Norepinephrine and Epinephrine

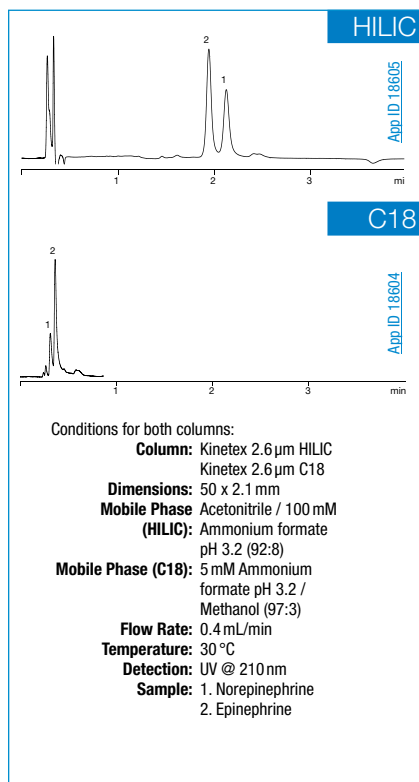

Acids, Bases, and Neutrals Mix

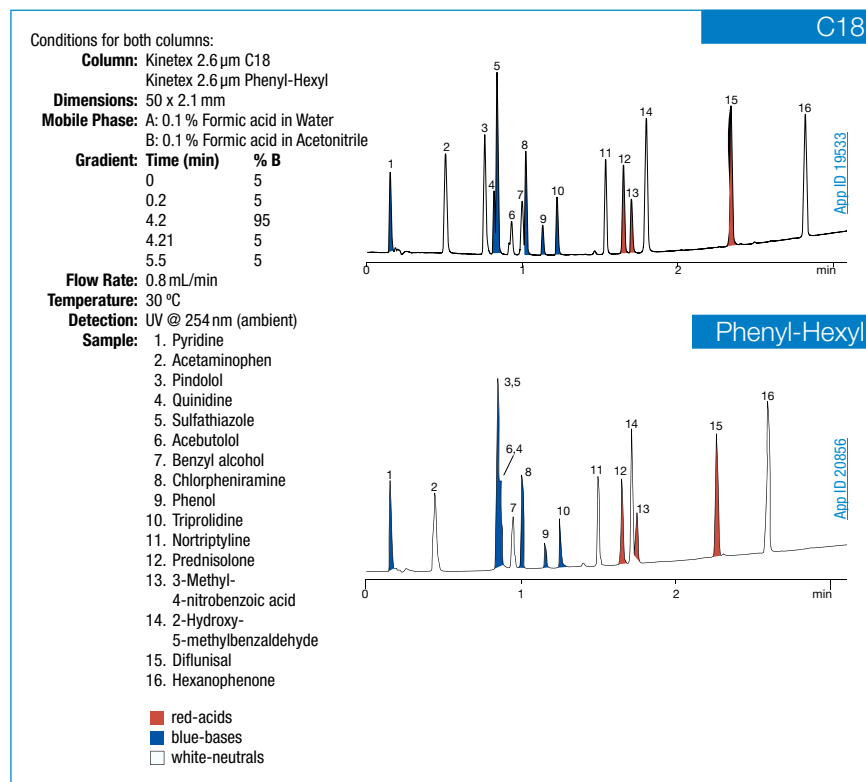


Comparative separations may not be representative of all applications.

NEW Kinetex PAH


- Expanded resolution with chemical selectivity specifically for PAHs
- Increased throughput and sensitivity with core-shell technology for HPLC/UHPLC

Designed and QC Tested for PAH Analysis by HPLC/UHPLC

Kinetex PAH columns were specifically built for the analysis of PAHs. Controlled pore size processing and a proprietary polymerically bonded stationary phase were developed for this product to ensure excellent resolution between priority polycyclic aromatic hydrocarbons (PAHs). Combined with core-shell particle technology, incredibly high efficiency and sensitivity at comfortable LC pressures is very achievable.

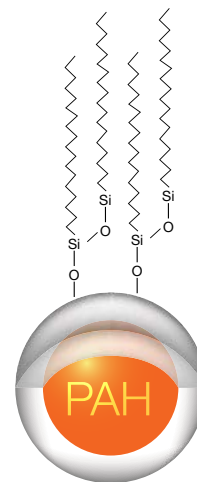

EPA 610 – PAH Analysis

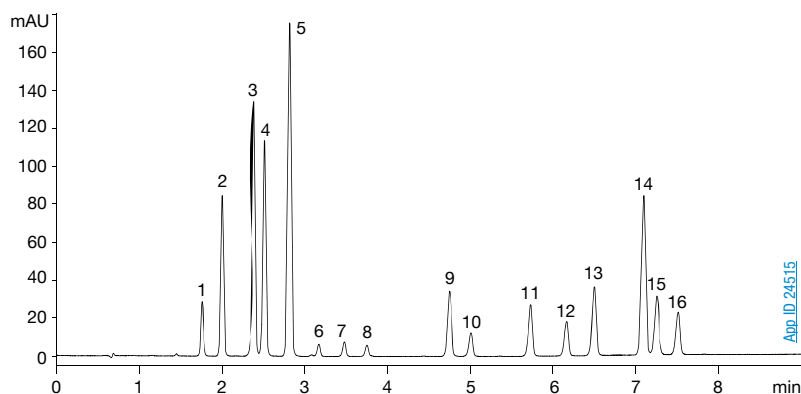

App ID 24515


Column: Kinetex 3.5 μ m PAH
Dimensions: 100 x 4.6 mm
Part No.: [00D-4764-E0](#)
Mobile Phase: A: Water
 B: Acetonitrile
Gradient:

Time (min)	% B
0	50
7	100
8	100
9	50
12	50

Flow Rate: 1.2 mL/min
Backpressure: 136 Bar
Temperature: 35 $^{\circ}$ C
Detection: UV @ 292 nm
Sample:

1. Naphthalene	9. Benz[a]anthracene
2. Acenaphthylene	10. Chrysene
3. Acenaphthene	11. Benzo[b]fluoranthene
4. Fluorene	12. Benzo[k]fluoranthene
5. Phenanthrene	13. Benzo[a]pyrene
6. Anthracene	14. Dibenz[a,h]anthracene
7. Fluoranthene	15. Benzo[g,h,i]perylene
8. Pyrene	16. Indeno[1,2,3-cd]pyrene

EU 15+1 PAH Analysis

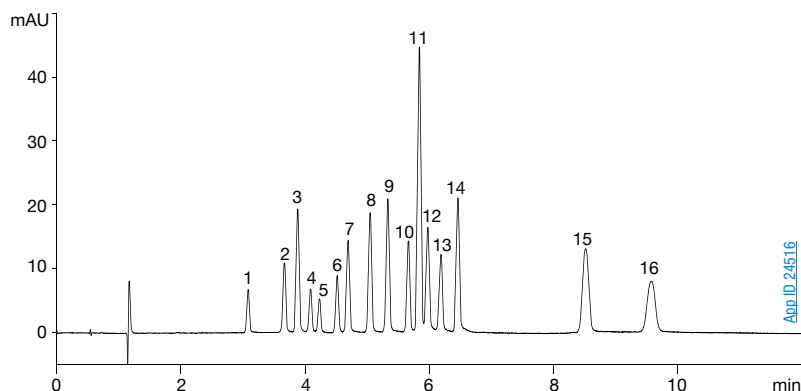

App ID 24516

Column: Kinetex 3.5 μ m PAH
Dimensions: 100 x 4.6 mm
Part No.: [00D-4764-E0](#)
Mobile Phase: A: Water
 B: Acetonitrile
Gradient:


Time (min)	% B
0	50
6	100
11.5	100
12	50
14	50

Flow Rate: 1.5 mL/min
Backpressure: 136 Bar
Temperature: 35 $^{\circ}$ C
Detection: UV @ 292 nm
Sample:

1. Benzo[c]fluorene	9. Benzo[a]pyrene
2. Cyclopenta[cd]pyrene	10. Dibenzo[a,l]pyrene
3. Benzo[a]anthracene	11. Dibenz[a,h]anthracene
4. Chrysene	12. Benzo[g,h,i]perylene
5. 5-Methylchrysene	13. Indeno[1,2,3-cd]pyrene
6. Benzo[j]fluoranthene	14. Dibenzo[a,e]pyrene
7. Benzo[b]fluoranthene	15. Dibenzo[a,i]pyrene
8. Benzo[k]fluoranthene	16. Dibenzo[a,h]pyrene

Applications Clinical Research and Toxicology

Comprehensive Drug Research Panel

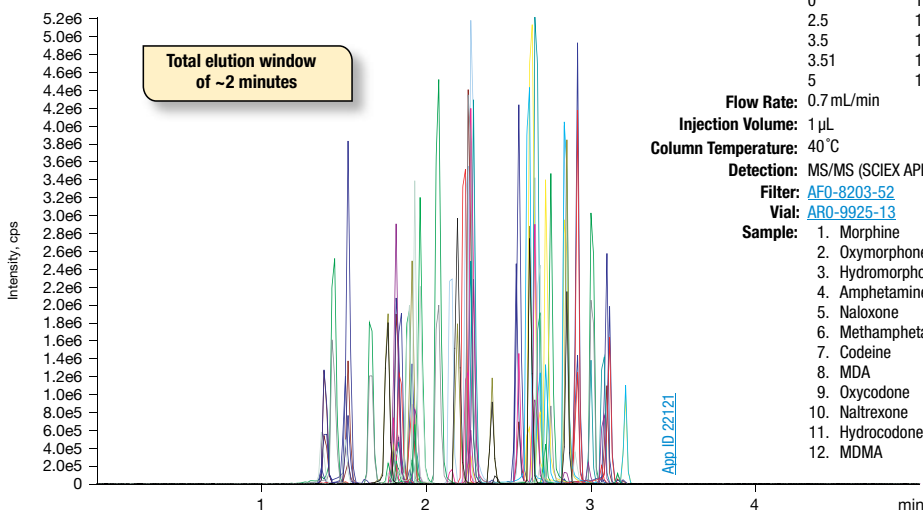

Column: Kinetex 2.6µm Biphenyl
Dimensions: 50 x 3.0 mm
Part No.: [00B-4622-Y0](#)
Guard Cartridge: [AJO-9208](#)
Guard Holder: [AJO-9000](#)
Mobile Phase: A: 0.1% Formic Acid in Water
 B: 0.1% Formic Acid in Methanol
Gradient:

Time (min)	% B
0	10
2.5	100
3.5	100
3.51	10
5	10

Flow Rate: 0.7 mL/min
Injection Volume: 1 µL
Column Temperature: 40°C
Detection: MS/MS (SCIEX API 5000™)
Filter: [AFO-8203-52](#)
Vial: [ARO-9925-13](#)
Sample:

- Morphine
- Oxymorphone
- Hydromorphone
- Amphetamine
- Naloxone
- Methamphetamine
- Codeine
- MDA
- Oxycodone
- Naltrexone
- Hydrocodone
- MDMA

- MDEA
- Norfentanyl
- Tramadol
- Benzoylcegonine
- Meperidine
- Meprobamate
- Norbuprenorphine
- Fentanyl
- Buprenorphine
- Flurazepam
- Carisoprodol
- PCP
- Propoxyphene
- Sufentanil
- 6-MAM
- Midazolam
- Normeperidine
- EDDP
- Methadone
- Lorazepam
- Clonazepam
- Norpropoxyphene
- Oxazepam
- Hydroxalprazolam
- Nordiazepam
- Flunitrazepam
- Temazepam
- Alprazolam
- Diazepam


Vitamin D

Column: Kinetex 2.6µm C18
Dimensions: 30 x 3.0 mm
Guard Cartridge: [AJO-8775](#)
Guard Holder: [AJO-9000](#)
Part No.: [00B-4462-Y0](#)
Mobile Phase: A: 0.1% Formic acid in Water
 B: 0.1% Formic acid in Methanol
Gradient:

Time (min)	% B
0	60
0.5	95
2	95
2.01	60
3.5	60

Flow Rate: 0.6 mL/min
Temperature: 22°C
Detection: Tandem Mass Spectrometer (MS/MS) (22°C)
Detector: SCIEX API 5000™ System
Filter: [AFO-8203-52](#)
Vial: [ARO-9925-13](#)
Sample:

- 25-Hydroxy Vitamin D2 (25-OH D2)
- 25-Hydroxy Vitamin D3-2H3
- 25-Hydroxy Vitamin D3-d6 (25-OH D3-d6)

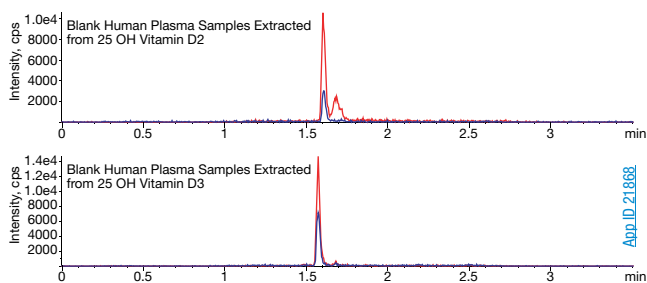


Human Plasma Vitamin C

Column: Kinetex 5µm XB-C18
Dimensions: 150 x 4.6 mm
Guard Cartridge: [AJO-8768](#)
Guard Holder: [AJO-9000](#)
Part No.: [00F-4605-E0](#)
Mobile Phase: A: 0.1% Formic acid in Water
 B: Acetonitrile
Gradient:

Time (min)	% B
0	0
3.5	0
3.6	100
5	100
5.1	0
7	0

Flow Rate: 0.8 mL/min
Temperature: 22°C
Detection: UV @ 245 nm
Filter: [AFO-8103-52](#)
Vial: [ARO-9925-13](#)
Sample:

- Vitamin C (ascorbic acid)
- Uric acid

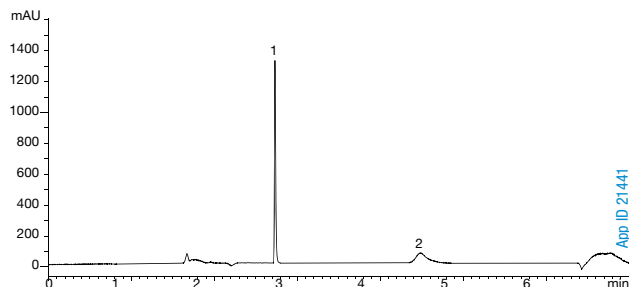

Applications


Food Testing

Multi-Class Antibiotics Screening of Meat

Column: Kinetex 2.6 µm C18
Dimensions: 50 x 2.1 mm
Part No.: [00B-4462-AN](#)
Mobile Phase: A: 0.1 % Formic acid in Water
 B: 0.1 % Formic acid in Methanol

Gradient	Time (min)	% B	Time (min)	% B
	0	2	7.37	99
	0.3	2	8.27	99
	7.27	80	13	2

Flow Rate: 0.5 mL/min
Temperature: 40 °C
Detection: Mass Spectrometer (MS) (300 °C)
Detector: SCIEX API 4000™ System
Note: Analytes spiked at 100 ng/mL
Sample: See full list of analytes at www.phenomenex.com

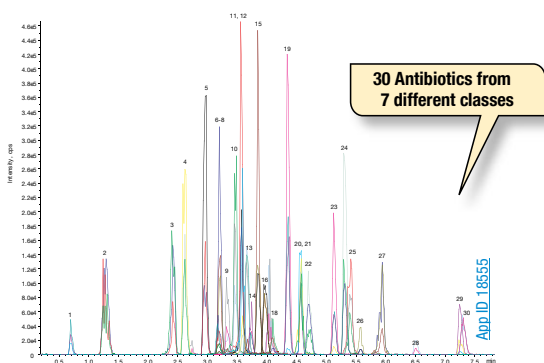

Azo Dyes


Column: Kinetex 2.6 µm C18
Dimensions: 150 x 4.6 mm
Part No.: [00F-4462-EQ](#)
Mobile Phase: A: 0.1 % Phosphoric acid in Water
 B: 0.1 % Phosphoric acid in Acetonitrile

Gradient	Time (min)	% B	Time (min)	% B
	0	25	17.01	25
	15	95	20	25
	17	95		

Flow Rate: 1.8 mL/min
Temperature: 50 °C
Detection: UV @ 215 nm
Backpressure: 380 bar

Sample:

1. Orange II	6. Sudan I
2. Sudan Orange G	7. Sudan II
3. Fast Garnet GBC	8. Sudan III
4. Dimethyl yellow	9. Sudan IV
5. Sudan Red G	

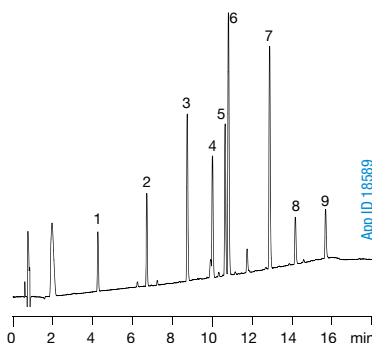

Multi-Toxin Screen

Column: Kinetex 2.6 µm XB-C18 100 Å
Dimensions: 50 x 2.1 mm
Part No.: [00B-4496-AN](#)
Mobile Phase: A: Water with 5 mM Ammonium acetate and 0.5 % Acetic acid
 B: Methanol with 5 mM Ammonium acetate and 0.5 % Acetic acid


Gradient	Time (min)	% B	Time (min)	% B
	0	2	5.2	98
	2	2	8	98
	5	80		

Flow Rate: 0.45 mL/min
Temperature: Ambient (22 °C)
Detection: Tandem Mass Spectrometer (MS/MS) (550 °C)
Detector: SCIEX API 5500™


Sample:

1. 15-Acetyldeoxynivalenol	7. Deoxynivalenol	13. Monoacetoxyscirpenol
2. 3-Acetyldeoxynivalenol	8. Diacetoxyscirpenol	14. Nivalenol
3. Aflatoxin B1	9. Fumonisin B1	15. Ochratoxin
4. Aflatoxin B2	10. Fumonisin B2	16. T-2 toxin
5. Aflatoxin G1	11. Fusarenon X	17. Zearalenon
6. Aflatoxin G2	12. HT-2 toxin	

Negative Polarity

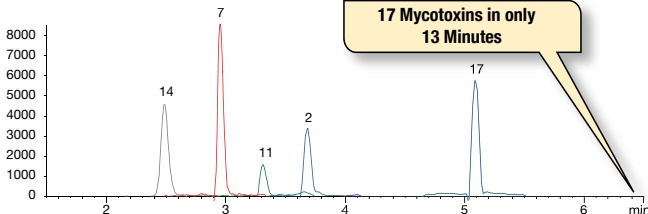

Positive Polarity

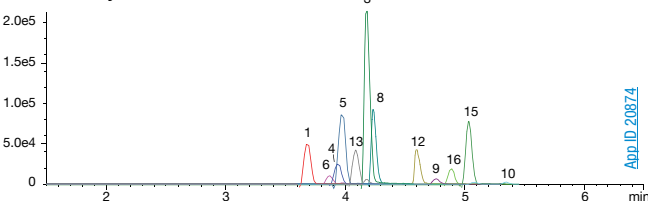

TIC of all analytes with negative and positive fast polarity switching.

Pharmaceutical

Tricyclic Antidepressants


Column: Kinetex 2.6 µm C18
Dimensions: 50 x 2.1 mm
Part No.: [00B-4462-AN](#)
Mobile Phase: A: 0.1 % Formic acid in Water
 B: 0.1 % Formic acid in Methanol

Gradient	Time (min)	% B	Time (min)	% B
	0	40	4.01	40
	3.5	80	5	40
	4	80		

Flow Rate: 0.4 mL/min
Temperature: 22 °C
Detection: MS/MS
Detector: SCIEX API 4000™ System

Sample:

1. Doxepin	8. Nortriptyline
2. DM-Doxepin	9. Amitriptyline
3. Imipramine-D3 (IS)	10. Protriptyline-D3 (IS)
4. Imipramine	11. Protriptyline
5. Desipramine-D3 (IS)	12. Clomipramine-D3 (IS)
6. Desipramine	13. Clomipramine
7. Nortriptyline-D3 (IS)	14. DM-Clomipramine

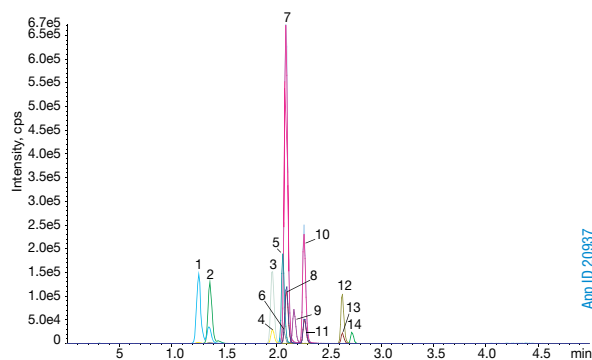


Applications Environmental

Carbamate Pesticides: EPA Method 531.1

Column: Kinetex 2.6 µm C18
Dimensions: 50 x 2.1 mm
Part No.: [00B-4462-AN](#)
Guard Cartridge: [AJ0-8782](#)
Guard Holder: [AJ0-9000](#)
Mobile Phase: A: 0.1 % Phosphoric acid in Water
 B: 0.1 % Phosphoric acid in Acetonitrile
Gradient: (95:5) A/B to (5:95) A/B over 3 min
Flow Rate: 1.0 mL/min
Temperature: 40 °C
Detection: UV @ 210 nm
Filter: [AF0-8203-52](#)
Vial: [ARO-9925-13](#)

Sample :

1. Aldicarb sulfoxide	7. Aldicarb
2. Oxamyl	8. Baygon [®] (Propoxur)
3. Aldicarb sulfone	9. Carbofuran
4. Methomyl	10. Carbaryl
5. 3-OH-Carbofuran	11. 1-Naphthol
6. Aldicarb sulfone-related impurity	12. Methiocarb

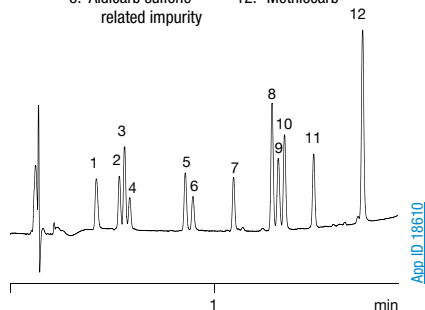


Polyaromatic Hydrocarbons (PAHs): EPA Method 610

Column: Kinetex 2.6 µm C18
Dimensions: 100 x 4.6 mm
Part No.: [00D-4462-E0](#)
Guard Cartridge: [AJ0-8768](#)
Guard Holder: [AJ0-9000](#)
Mobile Phase: A: Water
 B: Acetonitrile
Gradient: (30:70) A/B to (0:100) A/B over 10 min
Flow Rate: 1.5 mL/min
Temperature: 30 °C
Detection: UV @ 254 nm
Filter: [AF0-8203-52](#)
Vial: [ARO-9925-13](#)

Sample :

1. Naphthalene	9. Chrysene
2. Acenaphthylene	10. Benz[a]anthracene
3. Fluorene	11. Benzo[b]fluoranthene
4. Acenaphthene	12. Benzo[k]fluoranthene
5. Phenanthrene	13. Benzo[a]pyrene
6. Anthracene	14. Dibenzo[a,h]anthracene
7. Fluoranthene	15. Indeno[1,2,3-cd]pyrene
8. Pyrene	16. Benzo[g,h,i]perylene

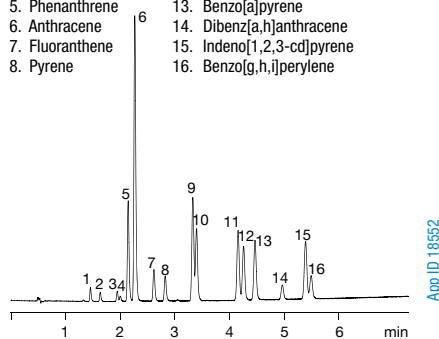

Triazine Pesticides: EPA Method 536


Column: Kinetex 2.6 µm XB-C18
Dimensions: 50 x 2.1 mm
Part No.: [00B-4496-AN](#)
Guard Cartridge: [AJ0-8782](#)
Guard Holder: [AJ0-9000](#)
Mobile Phase: A: 5 mM Ammonium Acetate
 B: Methanol

Gradient: Time (min)	% B
0	5
0.25	40
2	40
3	75
4	75
4.1	5

Flow Rate: 0.3 mL/min
Temperature: 25 °C
Detection: MS/MS
Filter: [AF0-8203-52](#)
Vial: [ARO-9925-13](#)
Detector: SCIEX API 4000[™] System

Sample :

1. Atrazine-desethyl-desisopropyl	7. Propazine
2. Atrazine-desisopropyl	
3. Atrazine-desethyl	
4. Cyanazine	
5. Simazine	
6. Atrazine	

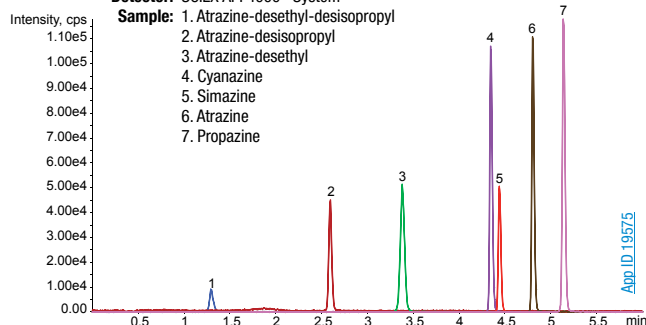

Carbonyl Compounds in Drinking Water


Column: Kinetex 5 µm C18
Dimensions: 150 x 4.6 mm
Part No.: [00F-4601-E0](#)
Guard Cartridge: [AJ0-8768](#)
Guard Holder: [AJ0-9000](#)
Mobile Phase: A: Water
 B: Acetonitrile

Gradient: Time (min)	% B
0	50
15	100
20	100

Flow Rate: 2 mL/min
Temperature: 30 °C
Detection: UV @ 360 nm (ambient)
Filter: [AF0-8103-52](#)
Vial: [ARO-9925-13](#)

Sample :

1. Formaldehyde	7. Pentanal
2. Acetaldehyde	8. Hexanal
3. Propanal	9. Heptanal
4. Crotonaldehyde	10. Octanal
5. Butanal	11. Nonanal
6. Cyclohexanone	12. Decanal

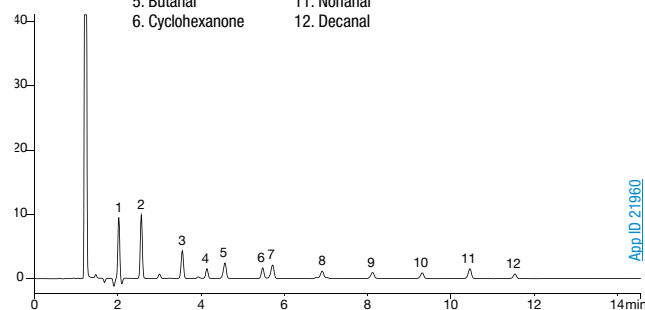

If Kinetex core-shell columns do not provide at least an equivalent separation as compared to a competing column of the same phase, return the column with the comparative data within 45 days for a FULL REFUND.



Material Characteristics

Packing Material	pH Stability	Available Particle Sizes (µm)	Pore Size (Å)	Effective Surface Area (m ² /g)	Effective Carbon Load (%)	USP Classification	Pressure Stability
Polar C18	1.5-8.5*	2.6	100	200	9	L1	1000/600* bar
EVO C18	1-12	5, 2.6, 1.7	100	200	11	L1	1000/600* bar
C18	1.5-8.5**	5, 2.6, 1.7, 1.3	100	200	12	L1	1000/600* bar
XB-C18	1.5-8.5**	5, 3.5, 2.6, 1.7	100	200	10	L1	1000/600* bar
C8	1.5-8.5**	5, 2.6, 1.7	100	200	8	L7	1000/600* bar
Biphenyl	1.5-8.5**	5, 2.6, 1.7	100	200	11	L11	1000/600* bar
Phenyl-Hexyl	1.5-8.5**	5, 2.6, 1.7	100	200	11	L11	1000/600* bar
F5	1.5-8.5	5, 2.6, 1.7	100	200	9	L43	1000/600* bar
HILIC	2.0-7.5	5, 2.6, 1.7	100	200	0	L3	1000/600* bar

**Columns are pH stable from 1.5-10 under isocratic conditions. Columns are pH stable 1.5-8.5 under gradient conditions.

*2.1 mm ID Kinetex columns are pressure stable up to 1000 bar. 3.0 mm and 4.6 mm ID Kinetex 2.6 µm columns are stable up to 600 bar. When using Kinetex 1.3 µm or 1.7 µm, increased performance can be achieved, however high pressure-capable instrumentation is required.

Ordering Information

5 µm Minibore Columns (mm)					SecurityGuard [™] ULTRA Cartridges [†]
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	3/pk
EVO C18	00A-4633-AN	00B-4633-AN	00D-4633-AN	00F-4633-AN	AJ0-9298
F5	00A-4724-AN	00B-4724-AN	00D-4724-AN	00F-4724-AN	AJ0-9322
Biphenyl	00A-4627-AN	00B-4627-AN	00D-4627-AN	—	AJ0-9209
XB-C18	00A-4605-AN	00B-4605-AN	00D-4605-AN	—	AJ0-8782
C18	00A-4601-AN	00B-4601-AN	00D-4601-AN	00F-4601-AN	AJ0-8782
C8	—	00B-4608-AN	00D-4608-AN	—	AJ0-8784
Phenyl-Hexyl	—	00B-4603-AN	—	—	AJ0-8788

for 2.1 mm ID

5 µm MidBore [™] Columns (mm)				SecurityGuard [™] ULTRA Cartridges [†]
Phases	50 x 3.0	100 x 3.0	150 x 3.0	3/pk
EVO C18	00B-4633-Y0	00D-4633-Y0	00F-4633-Y0	AJ0-9297
F5	00B-4724-Y0	00D-4724-Y0	00F-4724-Y0	AJ0-9321
Biphenyl	00B-4627-Y0	00D-4627-Y0	00F-4627-Y0	AJ0-9208
XB-C18	00B-4605-Y0	00D-4605-Y0	00F-4605-Y0	AJ0-8775
C18	00B-4601-Y0	00D-4601-Y0	00F-4601-Y0	AJ0-8775
C8	00B-4608-Y0	00D-4608-Y0	—	AJ0-8777
Phenyl-Hexyl	00B-4603-Y0	00D-4603-Y0	—	AJ0-8781

for 3.0 mm ID

5 µm Semi-Preparative Columns (mm)			SecurityGuard [™] SemiPrep Cartridges ^{***}
Phases	150 x 10	250 x 10	10 x 10 3/pk
EVO C18	00F-4633-N0	00G-4633-N0	AJ0-9306
F5	—	00G-4724-N0	AJ0-9323
C18	00F-4601-N0	00G-4601-N0	AJ0-9278
Biphenyl	00F-4627-N0	00G-4627-N0	AJ0-9280

for ID: 9-16 mm

5 µm Analytical Columns (mm)					SecurityGuard [™] ULTRA Cartridges [†]
Phases	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	3/pk
EVO C18	00B-4633-E0	00D-4633-E0	00F-4633-E0	00G-4633-E0	AJ0-9296
F5	00B-4724-E0	00D-4724-E0	00F-4724-E0	00G-4724-E0	AJ0-9320
Biphenyl	00B-4627-E0	00D-4627-E0	00F-4627-E0	00G-4627-E0	AJ0-9207
XB-C18	00B-4605-E0	00D-4605-E0	00F-4605-E0	00G-4605-E0	AJ0-8768
C18	00B-4601-E0	00D-4601-E0	00F-4601-E0	00G-4601-E0	AJ0-8768
C8	00B-4608-E0	00D-4608-E0	00F-4608-E0	00G-4608-E0	AJ0-8770
Phenyl-Hexyl	00B-4603-E0	00D-4603-E0	00F-4603-E0	00G-4603-E0	AJ0-8774

for 4.6 mm ID

5 µm Axia [™] Packed Preparative Columns (mm)					SecurityGuard [™] PREP Cartridges ^{**}
Phases	50 x 21.2	100 x 21.2	150 x 21.2	250 x 21.2	15 x 21.2 /ea
EVO C18	00B-4633-P0-AX	00D-4633-P0-AX	00F-4633-P0-AX	00G-4633-P0-AX	AJ0-9304
F5	—	—	00F-4724-P0-AX	00G-4724-P0-AX	AJ0-9324
Biphenyl	00B-4627-P0-AX	00D-4627-P0-AX	00F-4627-P0-AX	00G-4627-P0-AX	AJ0-9272
XB-C18	00B-4605-P0-AX	00D-4605-P0-AX	00F-4605-P0-AX	00G-4605-P0-AX	AJ0-9145
C18	00B-4601-P0-AX	00D-4601-P0-AX	00F-4601-P0-AX	00G-4601-P0-AX	AJ0-9145
C8	00B-4608-P0-AX	00D-4608-P0-AX	00F-4608-P0-AX	00G-4608-P0-AX	AJ0-9205
Phenyl-Hexyl	00B-4603-P0-AX	00D-4603-P0-AX	00F-4603-P0-AX	00G-4603-P0-AX	AJ0-9147
HILIC	—	00D-4606-P0-AX	00F-4606-P0-AX	00G-4606-P0-AX	AJ0-9277

for ID: 18-29 mm

[†]SecurityGuard ULTRA Cartridges require holder, Part No.: [AJ0-9000](#)
^{**}SemiPrep SecurityGuard Cartridges require holder, Part No.: [AJ0-9281](#)
^{***}PREP SecurityGuard Cartridges require holder, Part No.: [AJ0-8223](#)

Kinetex[®] Core-Shell LC Columns

Ordering Information (continued)

5 µm Axia Packed Preparative Columns (mm)					SecurityGuard PREP Cartridges**
Phases	50 x 30	100 x 30	150 x 30	250 x 30	15 x 30
EVO C18	00B-4633-UO-AX	00D-4633-UO-AX	00F-4633-UO-AX	00G-4633-UO-AX	AJ0-9305
F5	00B-4724-UO-AX	00D-4724-UO-AX	00F-4724-UO-AX	00G-4724-UO-AX	AJ0-9325
Biphenyl	—	—	00F-4627-UO-AX	—	AJ0-9273
XB-C18	00B-4605-UO-AX	00D-4605-UO-AX	00F-4605-UO-AX	00G-4605-UO-AX	AJ0-9204
C18	00B-4601-UO-AX	00D-4601-UO-AX	00F-4601-UO-AX	00G-4601-UO-AX	AJ0-9204
C8	—	—	00F-4608-UO-AX	00G-4608-UO-AX	AJ0-9217
Phenyl-Hexyl	—	00D-4603-UO-AX	00F-4603-UO-AX	00G-4603-UO-AX	AJ0-9216

for ID: 30-49 mm

3.5 µm Minibore and MidBore™ Columns (mm)					SecurityGuard™ ULTRA Cartridges [†]	
Phases	50 x 2.1	100 x 2.1	150 x 2.1	100 x 3.0	3/pk	3/pk
PAH	00B-4764-AN	00D-4764-AN	00F-4764-AN	00D-4764-YO	AJ0-9535	AJ0-9534

for 2.1 mm ID

for 3.0 mm ID

3.5 µm Analytical Columns (mm)		SecurityGuard™ ULTRA Cartridges [†]		
Phases	100 x 4.6	150 x 4.6	250 x 4.6	3/pk
XB-C18	00D-4744-E0	00F-4744-E0	—	AJ0-8768
PAH	00D-4764-E0	00F-4764-E0	00G-4764-E0	AJ0-9533

for 4.6 mm ID

2.6 µm Microbore Columns (mm)			
Phases	50 x 1.0	100 x 1.0	150 x 1.0
XB-C18	00B-4496-A0	00D-4496-A0	00F-4496-A0

2.6 µm MercuryMS™ LC-MS Cartridges (mm)		
Phases	20 x 2.0	20 x 4.0
Biphenyl	00M-4622-B0-CE	00M-4622-D0-CE

MercuryMS Cartridge Holders		
Part No.	Description	Unit
CH0-7188	Direct-Connect Cartridge Holder, 20 mm	ea
CH0-5845	Standard Cartridge Holder, 20 mm	ea

2.6 µm Minibore Columns (mm)						SecurityGuard ULTRA Cartridges [†]
Phases	30 x 2.1	50 x 2.1	75 x 2.1	100 x 2.1	150 x 2.1	3/pk
EVO C18	00A-4725-AN	00B-4725-AN	—	00D-4725-AN	00F-4725-AN	AJ0-9298
Polar C18	00A-4759-AN	00B-4759-AN	—	00D-4759-AN	00F-4759-AN	AJ0-9532
Biphenyl	00A-4622-AN	00B-4622-AN	—	00D-4622-AN	00F-4622-AN	AJ0-9209
XB-C18	00A-4496-AN	00B-4496-AN	00C-4496-AN	00D-4496-AN	00F-4496-AN	AJ0-8782
C18	00A-4462-AN	00B-4462-AN	00C-4462-AN	00D-4462-AN	00F-4462-AN	AJ0-8782
C8	00A-4497-AN	00B-4497-AN	00C-4497-AN	00D-4497-AN	00F-4497-AN	AJ0-8784
HILIC	00A-4461-AN	00B-4461-AN	00C-4461-AN	00D-4461-AN	00F-4461-AN	AJ0-8786
Phenyl-Hexyl	00A-4495-AN	00B-4495-AN	00C-4495-AN	00D-4495-AN	00F-4495-AN	AJ0-8788
F5	00A-4723-AN	00B-4723-AN	—	00D-4723-AN	00F-4723-AN	AJ0-9322

for 2.1 mm ID

2.6 µm MidBore™ Columns (mm)						SecurityGuard ULTRA Cartridges [†]
Phases	30 x 3.0	50 x 3.0	75 x 3.0	100 x 3.0	150 x 3.0	3/pk
EVO C18	—	00B-4725-Y0	—	00D-4725-Y0	00F-4725-Y0	AJ0-9297
Polar C18	—	00B-4759-Y0	—	00D-4759-Y0	00F-4759-Y0	AJ0-9531
Biphenyl	—	00B-4622-Y0	—	00D-4622-Y0	00F-4622-Y0	AJ0-9208
XB-C18	00A-4496-Y0	00B-4496-Y0	00C-4496-Y0	00D-4496-Y0	00F-4496-Y0	AJ0-8775
C18	00A-4462-Y0	00B-4462-Y0	00C-4462-Y0	00D-4462-Y0	00F-4462-Y0	AJ0-8775
C8	00A-4497-Y0	00B-4497-Y0	00C-4497-Y0	00D-4497-Y0	00F-4497-Y0	AJ0-8777
HILIC	00A-4461-Y0	—	—	—	00F-4461-Y0	AJ0-8779
Phenyl-Hexyl	—	00B-4495-Y0	—	00D-4495-Y0	00F-4495-Y0	AJ0-8781
F5	—	00B-4723-Y0	—	00D-4723-Y0	00F-4723-Y0	AJ0-9321

for 3.0 mm ID

*SecurityGuard Ultra Cartridges require holder, Part No.: [AJ0-9000](#)
 *PREP SecurityGuard Cartridges require holder, Part No. [AJ0-8223](#)
 **PREP SecurityGuard Cartridges require holder, Part No. [AJ0-8277](#)

If Kinetex core-shell columns do not provide at least an equivalent separation as compared to a competing column of the same phase, return the column with the comparative data within 45 days for a FULL REFUND.

Ordering Information (continued)

2.6 µm Analytical Columns (mm)						SecurityGuard ULTRA Cartridges [†]
Phases	30 x 4.6	50 x 4.6	75 x 4.6	100 x 4.6	150 x 4.6	3/pk
EVO C18	—	00B-4725-E0	—	00D-4725-E0	00F-4725-E0	AJ0-9296
Polar C18	—	00B-4759-E0	—	00D-4759-E0	00F-4759-E0	AJ0-9530
Biphenyl	—	00B-4622-E0	—	00D-4622-E0	00F-4622-E0	AJ0-9207
XB-C18	—	00B-4496-E0	00C-4496-E0	00D-4496-E0	00F-4496-E0	AJ0-8768
C18	00A-4462-E0	00B-4462-E0	00C-4462-E0	00D-4462-E0	00F-4462-E0	AJ0-8768
C8	—	00B-4497-E0	00C-4497-E0	00D-4497-E0	00F-4497-E0	AJ0-8770
HILIC	—	00B-4461-E0	00C-4461-E0	00D-4461-E0	00F-4461-E0	AJ0-8772
Phenyl-Hexyl	—	00B-4495-E0	00C-4495-E0	00D-4495-E0	00F-4495-E0	AJ0-8774
F5	—	00B-4723-E0	—	00D-4723-E0	00F-4723-E0	AJ0-9320

for 4.6 mm ID

1.7 µm Minibore Columns (mm)					SecurityGuard™ ULTRA Cartridges [†]
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	3/pk
EVO C18	—	00B-4726-AN	00D-4726-AN	00F-4726-AN	AJ0-9298
Biphenyl	—	00B-4628-AN	00D-4628-AN	00F-4628-AN	AJ0-9209
XB-C18	00A-4498-AN	00B-4498-AN	00D-4498-AN	00F-4498-AN	AJ0-8782
C18	00A-4475-AN	00B-4475-AN	00D-4475-AN	00F-4475-AN	AJ0-8782
C8	00A-4499-AN	00B-4499-AN	00D-4499-AN	00F-4499-AN	AJ0-8784
HILIC	00A-4474-AN	00B-4474-AN	00D-4474-AN	—	AJ0-8786
Phenyl-Hexyl	—	00B-4500-AN	00D-4500-AN	00F-4500-AN	AJ0-8788
F5	—	00B-4722-AN	00D-4722-AN	00F-4722-AN	AJ0-9322

for 2.1 mm ID



For Column Heater, see p. 408

1.7 µm MidBore™ Columns (mm)				SecurityGuard ULTRA Cartridges [†]
Phases	30 x 3.0	50 x 3.0	100 x 3.0	3/pk
XB-C18	00A-4498-Y0	00B-4498-Y0	00D-4498-Y0	AJ0-8775
C18	—	00B-4475-Y0	00D-4475-Y0	AJ0-8775
C8	00A-4499-Y0	00B-4499-Y0	00D-4499-Y0	AJ0-8777
HILIC	—	00B-4474-Y0	—	AJ0-8779

for 3.0 mm ID



1.7 µm Microbore Columns (mm)			
Phases	50 x 1.0	100 x 1.0	150 x 1.0
EVO C18	00B-4726-A0	00D-4726-A0	00F-4726-A0

1.3 µm Minibore Columns (mm)		
Phases	30 x 2.1	50 x 2.1
C18	00A-4515-AN	00B-4515-AN

[†]SecurityGuard ULTRA Cartridges require holder, Part No.: [AJ0-9000](#)

Core-Shell Performance Enhancement Kit

Ordering Information

Part No.	Unit
AQ0-8892	ea

SecurityGuard™ ULTRA Cartridge System

The SecurityGuard ULTRA cartridge system protects ultra-high performance columns, like Kinetex, from damaging contaminants and microparticulates.

- Extend Kinetex column lifetime
- Simple to use
- Pressure rated to 20000 psi (1378 bar)
- Fits virtually all manufacturers' columns 2.1 to 4.6 mm ID

High Pressure
Rated Format

SecurityGuard ULTRA Cartridge Holder

Ordering Information

Part No.	Description	Unit
AJ0-9000	SecurityGuard ULTRA Cartridge Holder	ea



For Core-Shell Performance Enhancement Kit description, see p. 411

For more information on the SecurityGuard ULTRA Cartridge System, see p. 331

UHPLC / HPLC Sure-Lok™ High Pressure PEEK Male Nut Fittings

Ordering Information

Part No.	Description	Unit
AQ0-8503	Sure-Lok High Pressure PEEK 1-Pc Nut 10-32, for 1/16 in. Tubing, 12000 psi (827 bar)	10/pk
AQ0-8530	Sure-Lok Fitting Tightening Tool, Aluminum	ea

See p. 410 for more information.



For Ultra-High Performance Stainless Steel Nut and Ferrule Set, see p. 410

Kromasil®

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/kromasil

LiChrosorb®

- Quality-packed columns by Phenomenex

LiChrosorb® is a well-established, rugged, irregular silica material, with high surface area (60 Å, 500 m²/g).

Ordering Information

SecurityGuard™ Analytical Cartridges require universal holder Part No.: [KJO-4282](#)

5 µm Columns (mm)	SecurityGuard Cartridges (mm)				
	125 x 4.0	250 x 4.0	150 x 4.6	250 x 4.6	4 x 3.0
Phases					/10pk
RP-8	00E-0233-DO	00G-0233-DO	00F-0233-EO	00G-0233-EO	AJO-4290

for ID: 3.2-8.0 mm

LiChrospher®

- Quality-packed by Phenomenex

LiChrospher® (the 4 µm material is also known as Superspher® in Europe) is a spherical alternative to the well-established LiChrosorb irregular material. It offers higher efficiencies than the LiChrosorb material.

Ordering Information

SecurityGuard™ Analytical Cartridges require universal holder Part No.: [KJO-4282](#)

4 µm (Superspher) Columns (mm)	SecurityGuard Cartridges (mm)			
	125 x 4.0	250 x 4.0	4 x 2.0	4 x 3.0
Phases			/10pk	/10pk
RP-8	00E-3042-DO	00G-3042-DO	AJO-4289	AJO-4290
RP-18	00E-3043-DO	00G-3043-DO	AJO-4286	AJO-4287

for ID: 2.0-3.0 mm 3.2-8.0 mm

5 µm Columns (mm)	SecurityGuard Cartridges (mm)					
	125 x 4.0	250 x 4.0	150 x 4.6	250 x 4.6	4 x 2.0	4 x 3.0
Phases					/10pk	/10pk
RP-8	00E-3049-DO	00G-3049-DO	00F-3049-EO	00G-3049-EO	AJO-4289	AJO-4290
RP-18	00E-3050-DO	00G-3050-DO	00F-3050-EO	00G-3050-EO	AJO-4286	AJO-4287
RP-8 endcapped	00E-3051-DO	00G-3051-DO	—	00G-3051-EO	AJO-4289	AJO-4290
RP-18 endcapped	00E-3052-DO	00G-3052-DO	00F-3052-EO	00G-3052-EO	AJO-4286	AJO-4287
CN	00E-3053-DO	00G-3053-DO	—	00G-3053-EO	AJO-4304	AJO-4305
RP-Select B	00E-3156-DO	00G-3156-DO	—	00G-3156-EO	—	—

for ID: 2.0-3.0 mm 3.2-8.0 mm



Other column dimensions available upon request.


If Luna analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Explore Successful Separations

Your success begins with our commitment to provide the essential solutions to HPLC separations in the Luna brand. Some of the highest quality and performance standards are incorporated into Luna products, making them an indispensable platform for all areas of HPLC.

Explore Resolution with Luna Selectivities

Phase selectivity has the strongest impact on overall chromatographic resolution. Choosing the optimal selectivity can drive your separation to success. Luna phases span through 10 different chemistries, each offering its own unique selectivity.

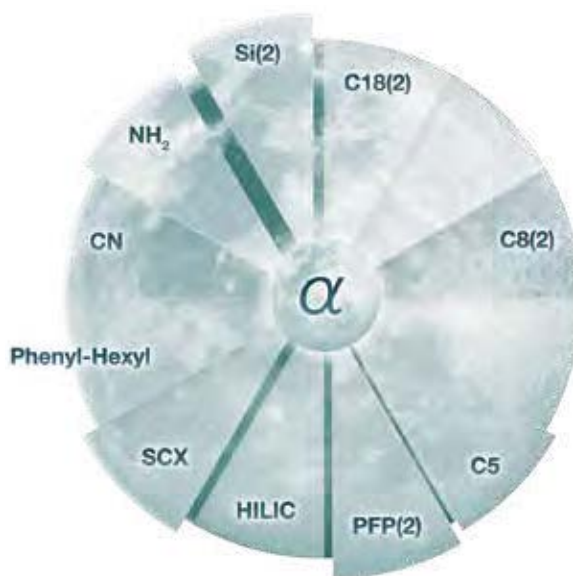

Luna Bonded Phase Selectivity Chart

Luna Phases	Description	Particle Sizes (µm)	Pore Size (Å)	Surface Area (m ² /g)	Carbon Load (%)	pH Stability	Reversed Phase	Normal Phase	HILIC	IEX	USP Column Classification
Silica(2)	Unbonded silica	3, 5, 10, 10-PREP, 15	100	400	—	2.0 - 7.5			☾	☾	L3
C5	5 Carbon ligand	5, 10	100	440	12.5	1.5 - 9.0*	☾				—
C8(2)	C8 ligand optimized for improved peak shape	3, 5, 10, 10-PREP, 15	100	400	13.5	1.5 - 9.0*	☾				L7
C18(2)	C18 ligand optimized for improved peak shape	2.5, 3, 5, 10, 10-PREP, 15	100	400	17.5	1.5 - 9.0*	☾				L1
CN	Versatile CN phase	3, 5, 10	100	400	7.0	1.5 - 7.0	☾	☾			L10
NH₂	Rugged and reproducible NH ₂	3, 5, 10	100	400	9.5	1.5 - 11	☾	☾	☾	☾	L8
Phenyl-Hexyl	Phenyl phase attached to C6 (hexyl) ligand	3, 5, 10, 10-PREP, 15	100	400	17.5	1.5 - 9.0*	☾				L11
SCX	Benzene sulfonic acid	5, 10	100	400	Binding Capacity: 0.15 meq/g	2.0 - 7.0				☾	L9
HILIC	Reproducible, cross-linked diol	3, 5	200	200	5.7	1.5 - 8.0			☾		L20
PFP(2)	Pentafluorophenyl with a C3 (propyl) linkage	3, 5	100	400	11.5	1.5 - 8.0	☾		☾		L43

* pH range is 1.5 - 9 under gradient conditions. pH range is 1.5 - 10 under isocratic conditions.



Luna Omega UHPLC Columns will boost your UHPLC instrumentation (see page 284).



Try Gemini for 1.0 - 12.0 pH stability. (see page 226).



Luna Silica

A Backbone and Phase Designed for Long Column Lifetimes

Luna columns' excellent performance is not simply the result of ultra-pure metal-free silica (99.99% purity). Meticulous care is given to the quality control of surface smoothness, pore structure and pore consistency to ensure particles of uniform structure and enhanced mechanical strength. Either bonded or unbonded, Luna silica produces highly advanced HPLC columns:

- Low percentage of "fines" from damaged silica leading to lower backpressures and enhanced column performance and lifetimes
- High column bed stability enhanced by particle shape uniformity

Incredible Silica Smoothness


Luna silica is extremely smooth and spherical. For bonded phases, this provides a uniform bonding surface for consistent and even bonded phase coverage. The likelihood of silica particle shearing and breakage during bonding and packing is very low; thus, Luna columns have high efficiencies and long column lifetimes.

- Recommended for preparative and bulk packing into DAC systems, see page 383 for more information


Long Column Lifetimes and Excellent Performance

Ultra-pure, metal-free silica (99.99% purity) is the backbone of all Luna material. The resulting high quality particles have a surface smoothness, pore structure, and pore consistency to ensure a more uniform particle shape and greater reproducibility.


Superior Particle Smoothness



Agilent Technologies[®]
ZORBAX[®] 5 µm SB-C18



Waters[®]
Symmetry[®] 5 µm C18



Phenomenex
Luna 5 µm C18

Luna Silica(2)

USP: L3

pH Stability: 2.0 – 7.5


Particle Size: 3 µm, 5 µm, 10 µm, 10 µm-PREP, and 15 µm

Phase: Unbonded silica

Application: Polar compounds

Natural Products (Kava Kava)

Column: Luna 5 µm Silica(2)
Dimensions: 150 x 4.6 mm
Part No.: [00F-4274-EQ](#)
Guard Cartridge: [AJ0-4348](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: Hexane/Dioxane (85:15)
Flow Rate: 1.5 mL/min
Detection: UV @ 230 nm
Vial: [AR0-9925-13](#)
Filter: [AF0-8103-52](#)
Sample: 1. Dihydrokavain
2. Yangonin
3. Kavain
4. Dihydrmethysticin
5. Methysticin

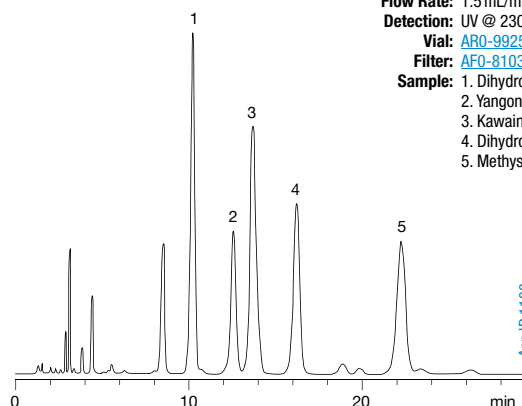

Luna C18(2), C8(2), C5

Your Starting Point for Reversed Phase Methods

The Luna column has found a place as one of the world's top reversed phase columns because it provides a measurable improvement over many HPLC columns for two important chromatographic properties: resolution and peak shape. The high efficiencies and bonded phase surface coverage provide for sharp peaks. The result:


- Free exposed silanols virtually eliminated by complete bonding and endcapping
- Sharp peak shape for good method sensitivity
- pH stable from 1.5 to 10.0 for over 10000 hours

Applications

Polar, Acidic Drugs

■ Phenomenex Luna® 3 µm C18(2)

■ Waters® Symmetry® 3.5 µm C18

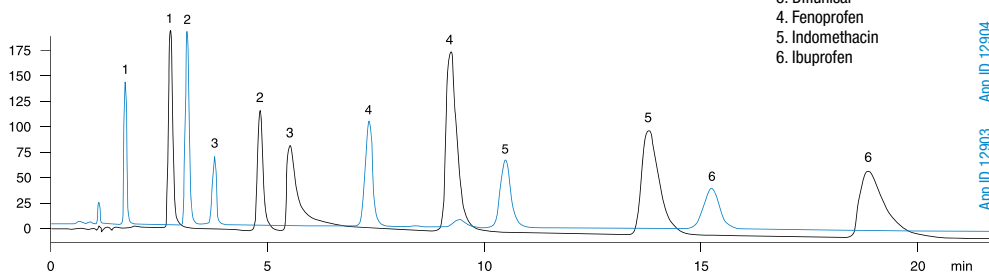

Conditions same for both columns:

Dimensions: 75 x 4.6 mm

Mobile Phase: 20 mM KH₂PO₄ / Acetonitrile(70:30)


Flow Rate: 0.75 mL/min

Detection: UV @ 202 nm

- Sample:**
1. Tolmetin
 2. Naproxen
 3. Difunisal
 4. Fenoprofen
 5. Indomethacin
 6. Ibuprofen

App ID: 12903 App ID: 12904

Fatty Acids

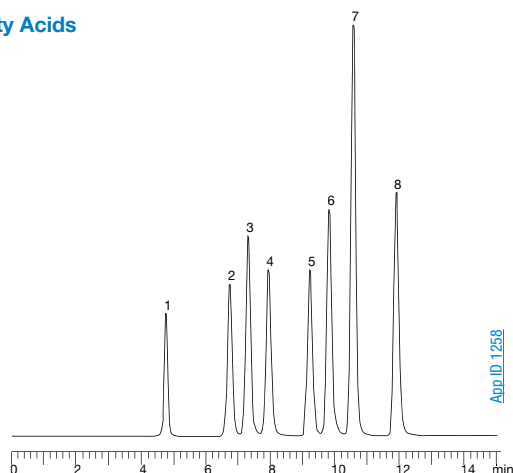

Columns: Luna 5 µm C8(2)

Dimensions: 150 x 4.6 mm

Part No.: 00F-4249-EO

Mobile Phase: A: Acetonitrile
B: Water (18 Mohms DI)

Gradient: A/B (70:30) to A/B (90:10) in 10 min,
A/B (90:10) to A/B (70:30) in 2 min,
hold for 4 min

Flow Rate: 0.3 mL/min

Detection: Evaporative Light Scattering (ELSD)

Temperature: 22 °C

- Sample:**
1. Lauric acid
 2. Myristic acid
 3. Palmitoleic acid
 4. Linoleic acid
 5. Palmitic acid
 6. Oleic acid
 7. Heptadecanoic acid
 8. Stearic acid


App ID: 1258

The comparative data presented here may not be representative for all applications.

Luna C18(2), C8(2), C5 (cont'd)


Steroids

Column: Luna 5 µm C18(2)
Dimensions: 150 x 4.6 mm
Part No.: [00F-4252-E0](#)
Mobile Phase: 0.1% H₃PO₄ / Acetonitrile/Methanol (54:35:11)
Flow Rate: 0.75 mL/min
Detection: UV @ 254 nm
Sample: 1. Hydrocortisone
 2. Corticosterone
 3. 11- α -Hydroxyprogesterone
 4. Cortisone Acetate
 5. 11-Ketoprogesterone

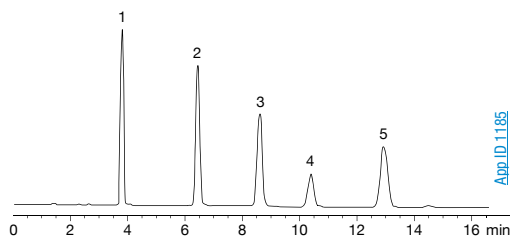


Narcotics

Columns: Luna 5 µm C18(2)
Dimensions: 150 x 4.6 mm
Part No.: [00F-4252-E0](#)
Mobile Phase: A: 10 mM NH₄OAc, pH 5.5
 B: Acetonitrile
Gradient: A/B (95:5) for 3 minutes, then A/B (95:5) to A/B (60:40) in 23 minutes
Flow Rate: 1.0 mL/min
Temperature: 45 °C
Detection: UV @ 254 nm (ambient)
Sample: 1. Normorphine
 2. Morphine
 3. Hydromorphone
 4. Norcodeine
 5. Codeine
 6. Hydrocodone
 7. Cocaine
 8. Norcocaine

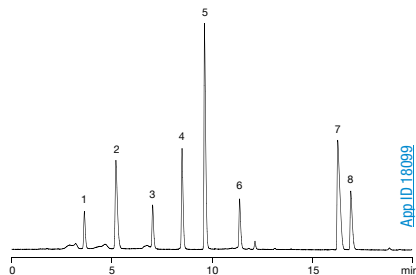


Basic Compounds

Conditions same for both columns:
Dimensions: 150 x 4.6 mm
Mobile Phase: 20 mM Potassium phosphate, pH 2.5 / Acetonitrile (75:25)
Flow Rate: 1.5 mL/min
Temperature: 30 °C
Detection: UV @ 210 nm
Sample: 1. Maleic acid
 2. Triprolidine*
 3. Chlorpheniramine*
 4. Diphenhydramine*
 *Peaks 2-4 adsorb on Nucleosil C18

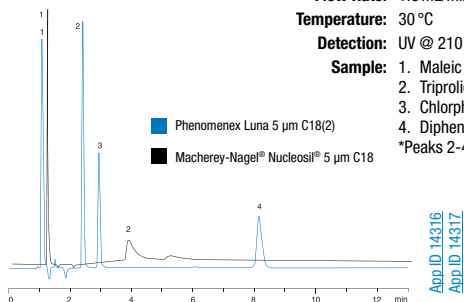


Acetaminophen, USP Method

Column: Luna 5 µm C18(2)
Dimensions: 150 x 4.6 mm
Part No.: [00F-4252-E0](#)
Mobile Phase: Water/Methanol/Acetic Acid (69:28:3)
Flow Rate: 1.5 mL/min
Detection: UV @ 275 nm
Sample: 1. Acetaminophen
 2. Caffeine
 3. Benzoic Acid

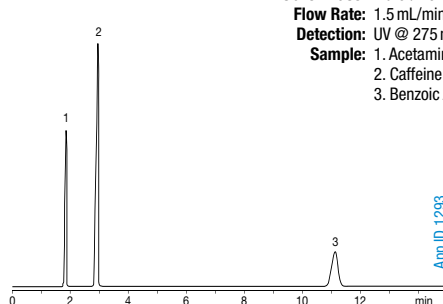


Pharmaceutical Preservatives

Column: Luna 5 µm C5
Dimensions: 150 x 4.6 mm
Part No.: [00F-4043-E0](#)
Mobile Phase: A: 0.5% Acetic acid in water/acetonitrile (80:20)
 B: 0.5% Acetic acid in water/acetonitrile (20:80)
Gradient: A/B (100:0) to A/B (0:100) in 30 min
Flow Rate: 1 mL/min
Temperature: 25 °C
Detection: UV @ 254 nm
Sample: 1. Propylparaben impurity
 2. Benzyl alcohol
 3. Phenol
 4. Benzoic acid
 5. Methylparaben
 6. Benzaldehyde
 7. Ethylparaben
 8. Propylparaben

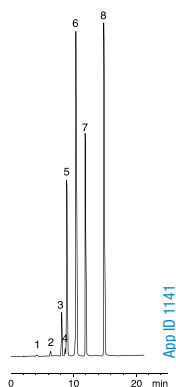

α - and β -acids in Hop Extract

Column: Luna 5 µm C18(2)
Dimensions: 250 x 4.6 mm
Part No.: [00G-4252-E0](#)
Mobile Phase: Methanol with 0.1% H₃PO₄ / Water with 0.1% H₃PO₄ (90:10)
Flow Rate: 1.5 mL/min
Temperature: 30 °C
Detection: UV @ 314 nm
Sample: 1. Cohumulone
 2. Ad-+humulone
 3. Colupulone
 4. Ad-+lupulone

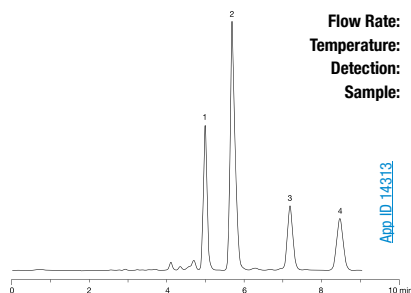

Luna Phenyl-Hexyl Engineered for Stability

Luna Phenyl-Hexyl columns provide separations not achievable on C18 or C8 columns; such as increased retention for polar, aromatic compounds as well as reversals in analyte elution order. Luna Phenyl-Hexyl columns are a reproducible, extremely stable phenyl phase. Most phenyl phases use a short propyl (3 carbon) linker, which limits phase stability. The Phenyl-Hexyl bonded phase employs a phenyl ring with a hexyl (6 carbon) linker and is densely bonded to Luna silica surface, reducing bonded phase hydrolysis and increasing chemical stability. The result:

- **Highly reproducible and stable phenyl phase**
- **Dual selectivity of both phenyl phase and a short alkyl phase (C5 or C8)**
- **Excellent retention of aromatic and polar, amine compounds**
- **Recommended for US EPA Method 8330B for explosives analysis**
- **1.5 to 10 pH stability for over 10000 hours**

Luna Phenyl-Hexyl

USP: L11

LC/MS
Certified

pH Stability: 1.5-9.0*


Particle Size: 3 µm, 5 µm, 10 µm, 10 µm-PREP, and 15 µm

Phase: Phenyl with Hexyl (C6) linker, endcapped

Application: Non-polar compounds


Strength: Aromatic selectivity enhanced by higher hydrophobicity due to hexyl linker

* pH range is 1.5 - 10 under isocratic conditions.
pH range is 1.5 - 9 under gradient conditions.




Luna Phenyl-Hexyl

Our most hydrophobic phenyl column and it will also provide good hydrogen accepting functionality for acidic retention.

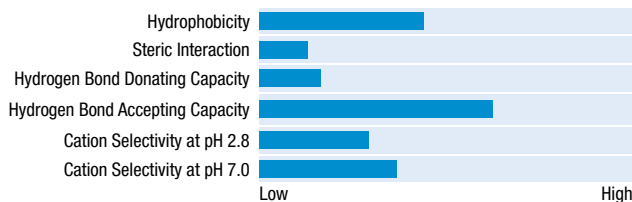

Chromatographic Comparisons of Phenyl Columns**

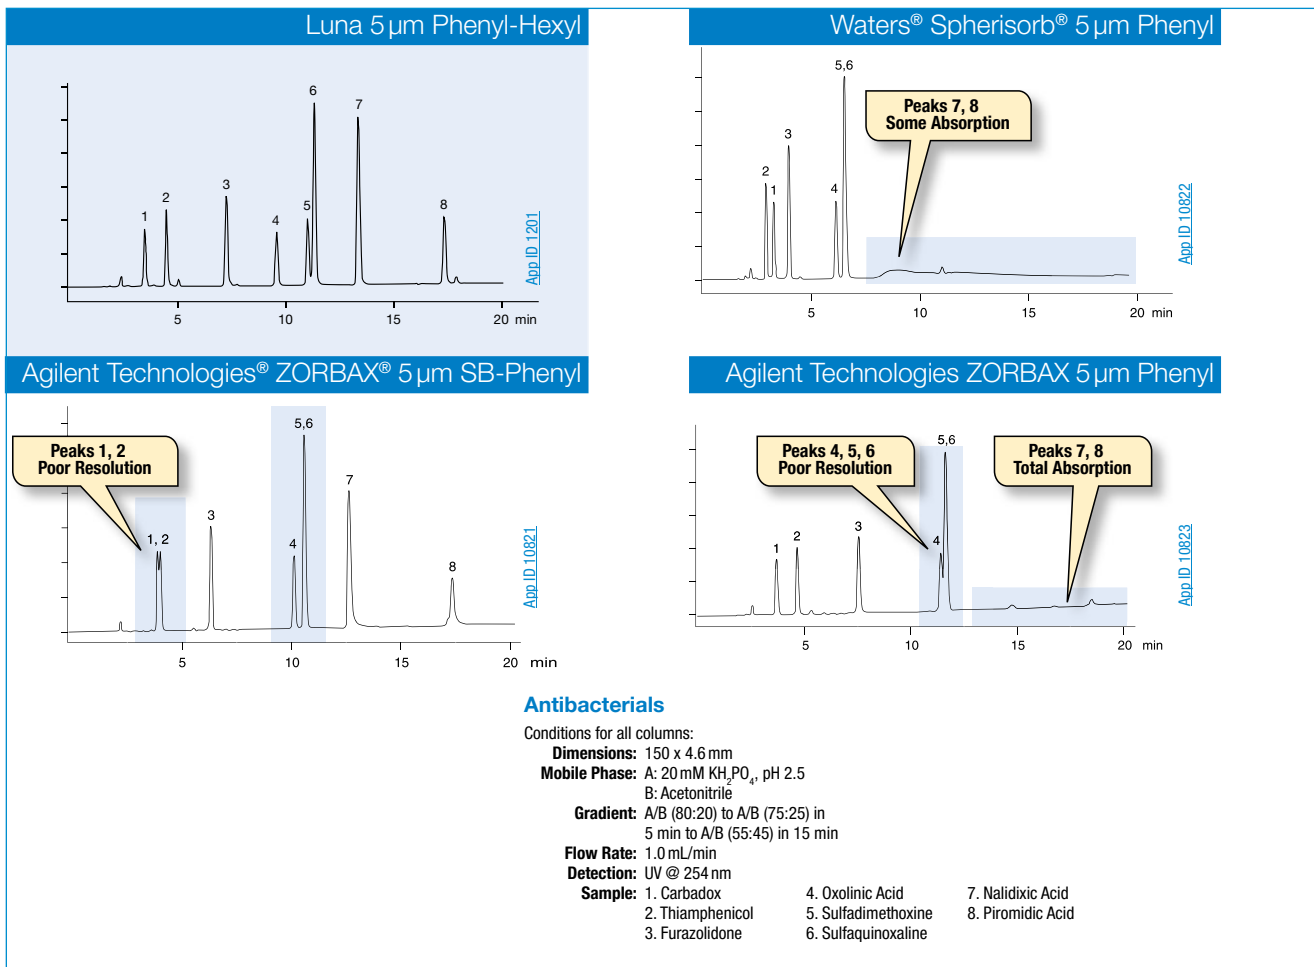

**The comparative data presented here may not be representative for all applications.



Luna CN (cyano)


Proven Reproducibility

For carboxyl, carbonyl, and amine containing compounds, Luna CN columns offer a unique polar selectivity in reversed phase and normal phase modes. Luna CN columns provide sharp peaks and great reproducibility run-to-run, column-to-column and batch-to-batch. State of the art modification of the silica surface ensures improved resistance to bonded phase hydrolysis providing one of the most stable CN phases on the market. The result:

- Excellent polar selectivity
- Improved peak shapes
- One of the most stable CN columns under reversed phase or normal phase conditions
- pH stable from 1.5 to 7.0


Batch-to-Batch Reproducibility

Column: Luna 5 µm CN
Dimensions: 150 x 4.6 mm
Mobile Phase: A: Hexane, B: Methylene chloride/Methanol(80:20), A/B (80:20)
Flow Rate: 2.0 mL/min
Detection: UV @ 254 nm
Injection: 1.0 µL
Temperature: Ambient
Sample: 1. Hydrocortisone
 2. Prednisone
 3. Cortisone
 4. Hydrocortisone Acetate



Chromatographic Comparisons of CN Columns**

Luna 5 µm CN

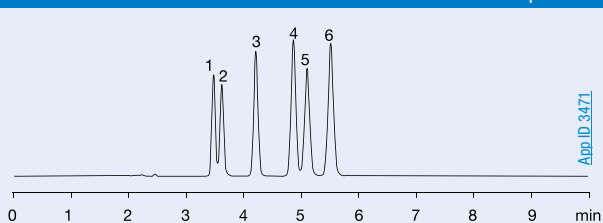

Phthalate Esters

Normal Phase Conditions for all columns:
Dimensions: 150 x 4.6 mm
Mobile Phase: A: Hexane, B: Methylene chloride/Methanol (80:20), A/B (99:1)
Flow Rate: 1.0 mL/min
Detection: UV @ 254 nm
Temperature: Ambient
Sample: 1. Di-n-octyl phthalate
 2. Bis (2-Ethylhexyl) phthalate
 3. Butylbenzyl phthalate
 4. Di-n-butyl phthalate
 5. Diethyl phthalate
 6. Dimethyl phthalate

Luna CN

USP: L10


pH Stability: 1.5-7.0

Particle Size: 3 µm, 5 µm, and 10 µm

Phase: Cyano, endcapped


Application: Compounds with COOH, CO, NH₂, NHR₂, or NR₂

Strength: Improved reproducibility for more consistent results run-to-run, column-to-column, batch-to-batch




Luna CN

Nitrile groups bound to the silica surface offer a unique polar selectivity under reversed phase or normal phase conditions.

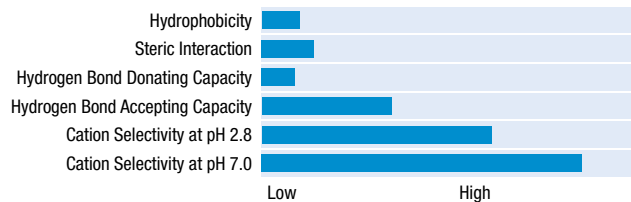


Column-to-Column Reproducibility


Column: Luna 5 µm CN
Dimensions: 150 x 4.6 mm
Mobile Phase: A: Hexane, B: Methylene chloride/Methanol(80:20), A/B (95:5)
Flow Rate: 1.0 mL/min
Injection: 5 µL
Detection: UV @ 254 nm
Temperature: Ambient
Sample: 1. Dimethyl phthalate
 2. Diethyl phthalate
 3. Dibutyl phthalate
 4. Dioctyl phthalate



Waters® Spherisorb® 5 µm CN

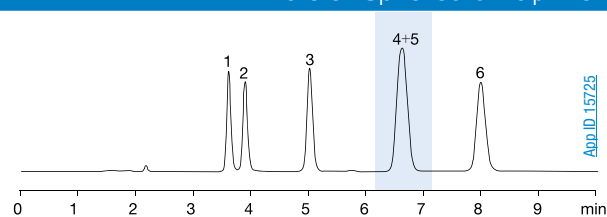

Agilent Technologies® ZORBAX® 5 µm SB-CN

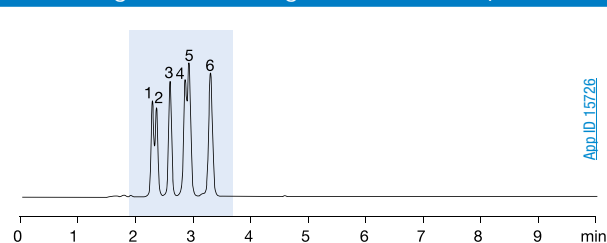

**The comparative data presented here may not be representative for all applications.

Luna NH₂ (amino)

Developed for Ruggedness

Luna NH₂ columns were developed to provide improved amino column lifetime. Column life for most amino columns can be problematic as the amino bonding easily strips off the silica. Luna NH₂ columns, however, show good bonded phase stability under both normal and reversed phase modes and across a pH range of 1.5 to 11.0. Such a broad pH range indicates the bonded phase ruggedness and the density of the bonded phase coverage. The result:

- Long lifetimes and low phase bleed for more reproducible methods
- Excellent retention of simple sugars, complex sugars, sugar alcohols by reversed phase conditions, and hydrogen bonding compounds under normal phase conditions
- pH stable from 1.5 to 11.0
- Stable in 100 % aqueous mobile phases

Luna NH₂

USP: L8

pH Stability: 1.5-11.0

Particle Size: 3 μm, 5 μm, and 10 μm


Phase: Amino

Application: Compounds with COOH, CO, NH₂, NHR₂, or NR₂

Strength: Sugars by reversed phase, steroids by normal phase, oligonucleotides by ion exchange

Simple Sugars


Column: Luna 5 μm NH₂
Dimensions: 250 x 4.6 mm
Part No.: [00G-4378-E0](#)
Guard Cartridge: [AJ0-4302](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: Acetonitrile/Water (80:20)
Flow Rate: 3 mL/min
Temperature: 40 °C
Detection: RI
Vial: [AR0-9925-13](#)
Filter: [AF0-8103-52](#)
Sample: 1. Xylose 5. Maltose
 2. Fructose 6. Melezitose
 3. Glucose 7. Raffinose
 4. Sucrose

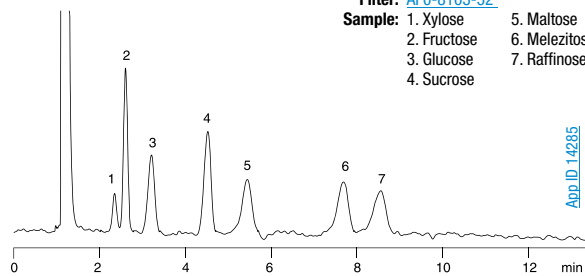

App ID 14285

Nucleic Acid Bases


Column: Luna 5 μm NH₂
Dimension: 150 x 4.6 mm
Part No.: [00F-4378-E0](#)
Mobile Phase: Acetonitrile/Water (80:20)
Flow Rate: 1.0 mL/min
Detection: UV @ 254 nm
Temperature: 40 °C
Sample: 1. Thymine
 2. Uracil
 3. Cytosine
 4. Adenine
 5. Guanosine

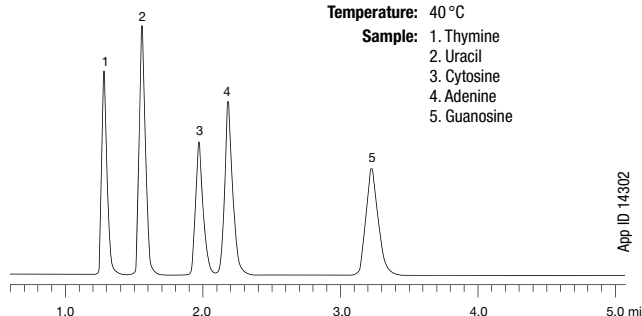

App ID 14302

Steroids


Column: Luna 5 μm NH₂
Dimensions: 250 x 4.6 mm
Part No.: [00G-4378-E0](#)
Guard Cartridge: [AJ0-4302](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: Hexane/Ethanol (85:15)
Flow Rate: 2 mL/min
Temperature: 22 °C
Detection: UV @ 240 nm
Vial: [AR0-9925-13](#)
Filter: [AF0-8103-52](#)
Sample: 1. 11-Ketoprogesterone
 2. 11-Hydroxyprogesterone
 3. Cortisone Acetate
 4. Prednisolone 21-Acetate
 5. Cortisone
 6. Prednisolone

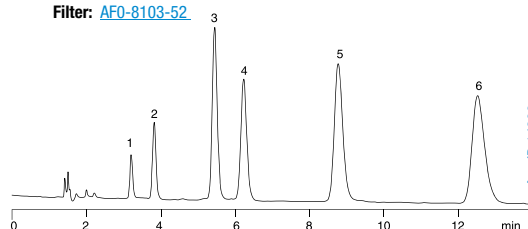

App ID 14299

Stability in 100% Aqueous Mobile Phase

Column: Luna 5 μm NH₂
Dimensions: 250 x 4.6 mm
Part No.: [00G-4378-E0](#)
Guard Cartridge: [AJ0-4302](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 20 mM Potassium Phosphate Buffer pH 2.7
Flow Rate: 1.5 mL/min
Detector: UV @ 254 nm
Vial: [AR0-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: Ambient
Injection: 2.5 μL
Conditions: Continuously flushed at 1.0 mL/min using 100 % 20 mM Potassium Phosphate Buffer pH 2.7 between injections

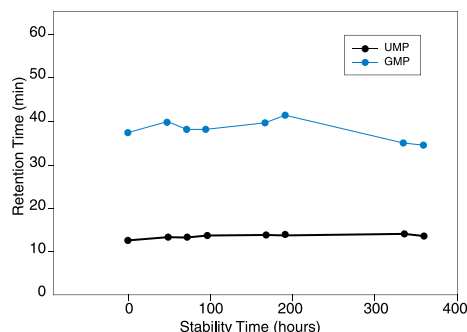


Luna SCX (strong cation exchange) Develop Robust Methods

Luna SCX columns provide excellent resolution and peak shape of basic, cationic compounds. However, most SCX columns show poor peak shape and bad resolution causing many chromatographers to ignore this important phase for small molecule method development, until now. Luna SCX columns contain a benzene sulfonic acid ligand providing ion-exchange, reversed phase, and aromatic interactions. Such interactions make Luna SCX columns great as a first dimension for 2D LC applications as well as improved resolution for small molecules. The result:

- Resolving power and sharp peak shape to separate complex cationic/basic and nitrogen containing compounds
- 5 and 10 μm columns and bulk media for analytical through preparative separations
- Benzene sulfonic acid ligand provides mixed-mode interaction improving separation for 2D peptide applications

Childrens Tylenol Cold Syrup

Column: Luna 5 μm SCX
Dimensions: 150 x 4.6 mm
Part No.: [00F-4398-E0](#)
Guard Cartridge: [AJ0-4308](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 50 mM KH_2PO_4 , pH 2.5/Acetonitrile (35:65)
Injection Volume: 1 μL
Flow Rate: 1.5 mL/min
Detection: UV @ 210 nm
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Sample Prep: Dissolve 1 part Childrens Tylenol Cold in 10 parts Methanol
Sample: 1. Acetaminophen
 2. Pseudoephedrine
 3. Dextromethorphan
 4. Chlorpheniramine

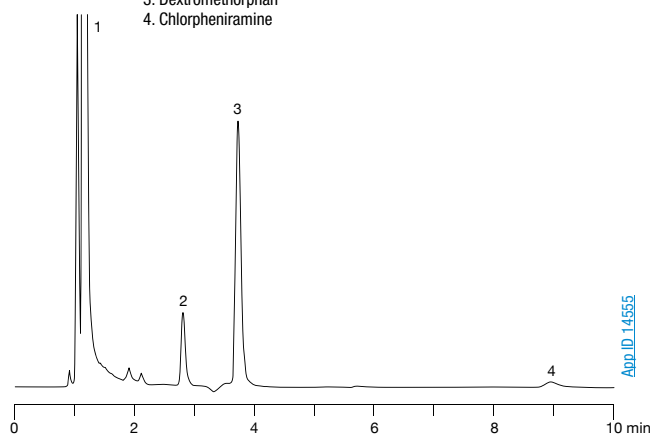

SCX Method Development and pH: The standard operating pH range for Luna SCX columns is 2.0 to 7.0. Most SCX methods are typically run between pH 2.0 and 5.0 for optimal performance. This ensures that nitrogen-containing analytes, especially those with adjacent conjugated system are protonated. Running in highly acidic (pH < 2.0) or basic (pH > 7.0) mobile phases may cause this phase to undergo degradation, as is common for all silica-based SCX phases.


Luna SCX

USP: L9

pH Stability: 2.0-7.0
Particle Size: 5 μm and 10 μm
Phase: Benzene Sulfonic Acid, Strong Cation Exchange
Application: Amine and polyamine containing compounds
Strength: Guaranteed to provide sharper peak shape and better resolution compared to traditional SCX columns


Peptides

Column: Luna 5 μm SCX
Dimensions: 150 x 4.6 mm
Part No.: [00F-4398-E0](#)
Guard Cartridge: [AJ0-4308](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: A: 20 mM Potassium Phosphate, 25% Acetonitrile, pH 2.5
 B: 20 mM Potassium Phosphate, 25% Acetonitrile, 400 mM Potassium Chloride, pH 2.5
Gradient: A/B (95:5) to A/B (10:90) in 45 minutes
Flow Rate: 1 mL/min
Temperature: 35 $^{\circ}\text{C}$
Detection: UV @ 215 nm
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Injection Volume: 2 μL (5 μg on column)
Sample: Peptide Mixture - Substance P
 1. Fragment 5-11 (+1)
 2. Fragment 4-11 (+1)
 3. Fragment 2-11 (+2)
 4. Fragment 1-9 (+3)
 5. Intact (+3)
 6. (ARG-PHE-TRP-LEU) (+3)

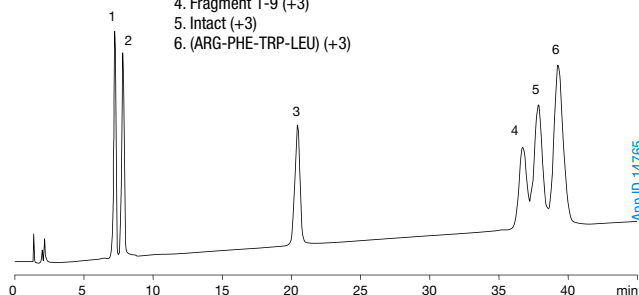

Tryptic Digest of Bovine Cytochrome c

Column: Luna 5 μm SCX
Dimensions: 150 x 4.6 mm
Part No.: [00F-4398-E0](#)
Guard Cartridge: [AJ0-4308](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: A: 20 mM Potassium Phosphate, pH 2.5 / 25% Acetonitrile
 B: 20 mM Potassium Phosphate, pH 2.5 / 25% Acetonitrile / 350 mM Potassium Chloride
Gradient: 100% A to 100% B in 50 minutes
Flow Rate: 1 mL/min
Temperature: 35 $^{\circ}\text{C}$
Detection: UV @ 215 nm
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Injection Volume: 50 μL (20 μg on column)
Sample: Bovine Cytochrome c trypsin digest

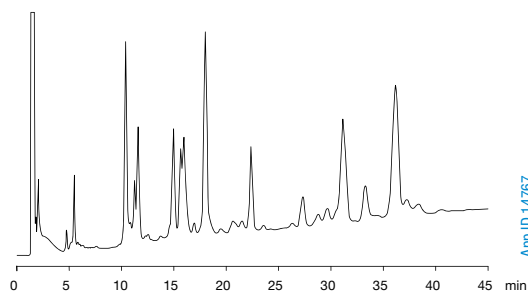

Luna HILIC


Increase MS Sensitivity and Retention for Polar Compounds

Luna HILIC columns retain a water-enriched layer on the surface of the silica. This water layer facilitates the transfer of polar compounds onto the stationary phase for increased retention.

Hydrophilic Interaction Liquid Chromatography (HILIC) is a separation mode where the partitioning of polar solutes from the high concentration, water-miscible, organic mobile phase into the hydrophilic surface environment creates separations. Polar solutes exhibit increased retention and elute in the order of increasing hydrophilicity.


Finally, reproducible, robust HILIC separations!

- Made for retention of polar compounds
- Increase mass spectrometry sensitivity
- Increase laboratory throughput and productivity

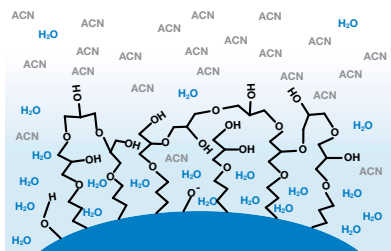

Vitamin Mix on Luna HILIC

Vitamins provide an excellent platform to demonstrate the benefits of HILIC. The effect of increased polar compound retention can be easily seen in this application.

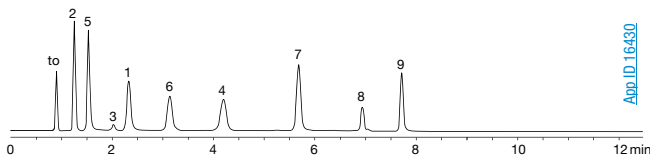


App ID: 16430

Column: Luna 5 µm HILIC
Dimensions: 150 x 4.6 mm
Part No.: [00F-4450-E0](#)
Guard Cartridge: [AJ0-8329](#)
Guard Holder: [KJO-4282](#)
Mobile Phase: A: Acetonitrile
 B: Water
 C: 100 mM Ammonium Acetate, pH 5.8
Gradient: A/B/C (90:5:5) for 2.5 min to A/B/C (50:45:5) in 7.5 min, hold for 2.5 min. Re-equilibrate @ A/B/C (90:5:5) for 7.5 min
Flow Rate: 2.0 mL/min
Detection: UV @ 260 nm
Vial: [AR0-9925-13](#)
Filter: [AF0-8103-52](#)
Sample: 1. p-Aminobenzoic Acid pK_a 4.7, H⁺ pK_s 2.7 logP 0.83
 2. Nicotinamide H⁺ pK_s 3.35 logP -0.37
 3. Riboflavin pK_s 10.2 logP -1.46
 4. Nicotinic Acid pK_s 4.7, H+pK_s 3.0 logP 0.36
 5. Pyridoxine H⁺ pK_s 5.6, pK_s 8.6 logP -0.77
 6. Thiamine H⁺ pK_s 5.5 logP -4.6
 7. Ascorbic Acid pK_s 4.1, 11.2 logP -1.85
 8. Cyanocobalamin pK_s 1.59 logP -0.90
 9. Folic Acid pK_s 2.7, 4.1, 8.9 logP -0.02

Improved Mass Spec Sensitivity

Luna HILIC columns allow low level polar metabolites to be retained on column past the critical ion suppression zone, allowing: Increased MS sensitivity and Higher signal-to-noise ratio (S/N).


Bamethan

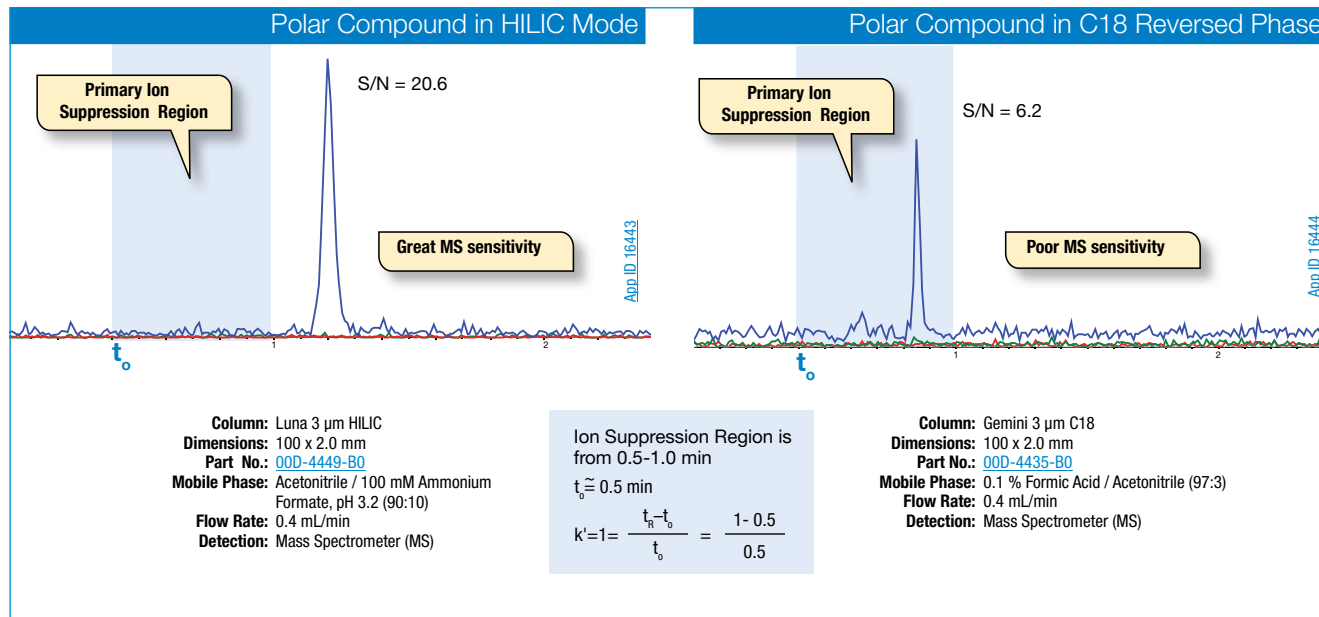

Luna HILIC (cont'd) Improved Mass Spec Sensitivity (cont'd)

The increased retention in HILIC allows elution of the analytes outside the suppression region and thus increases detector sensitivity. In addition, the Luna HILIC column also resolves the compounds with the reverse order of that seen in reversed phase LC.


Nicotine and Metabolites

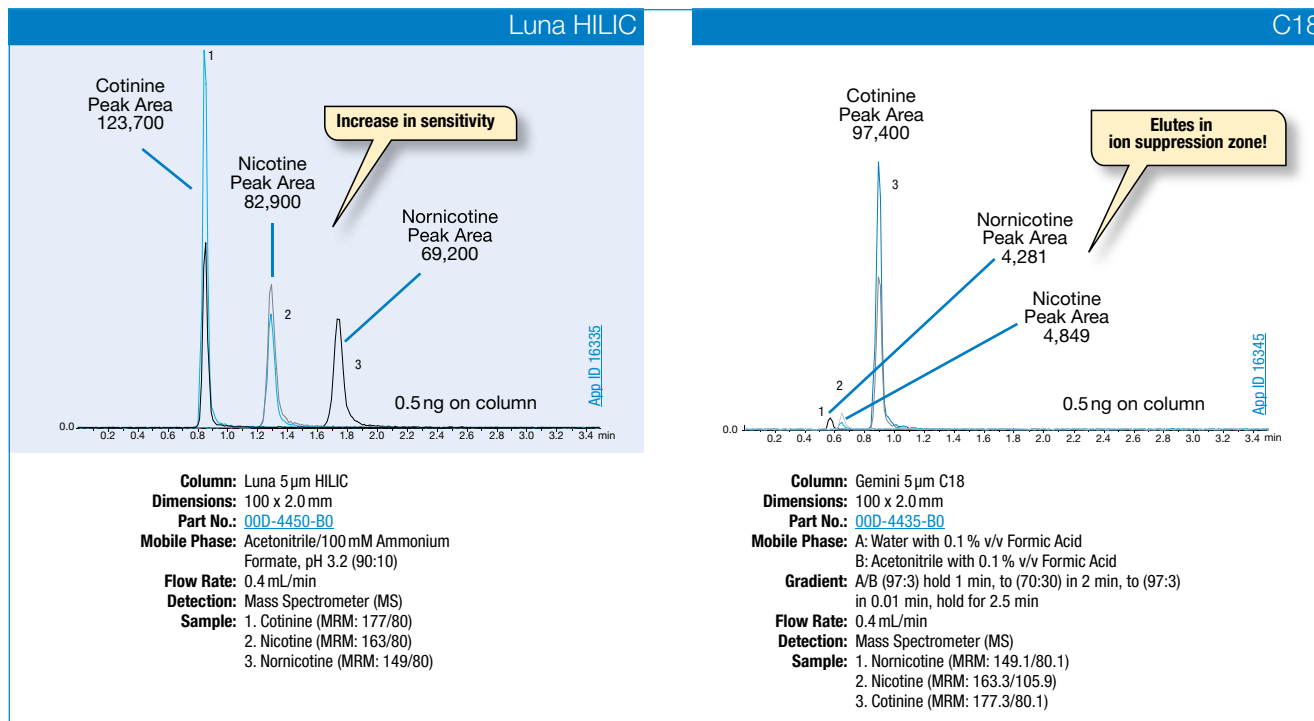

Unique HILIC Selectivity

Not all HILIC columns are alike, Luna HILIC columns deliver on the exacting standards you have come to trust from the Luna product line.

Chromatographic Comparisons of HILIC Columns**

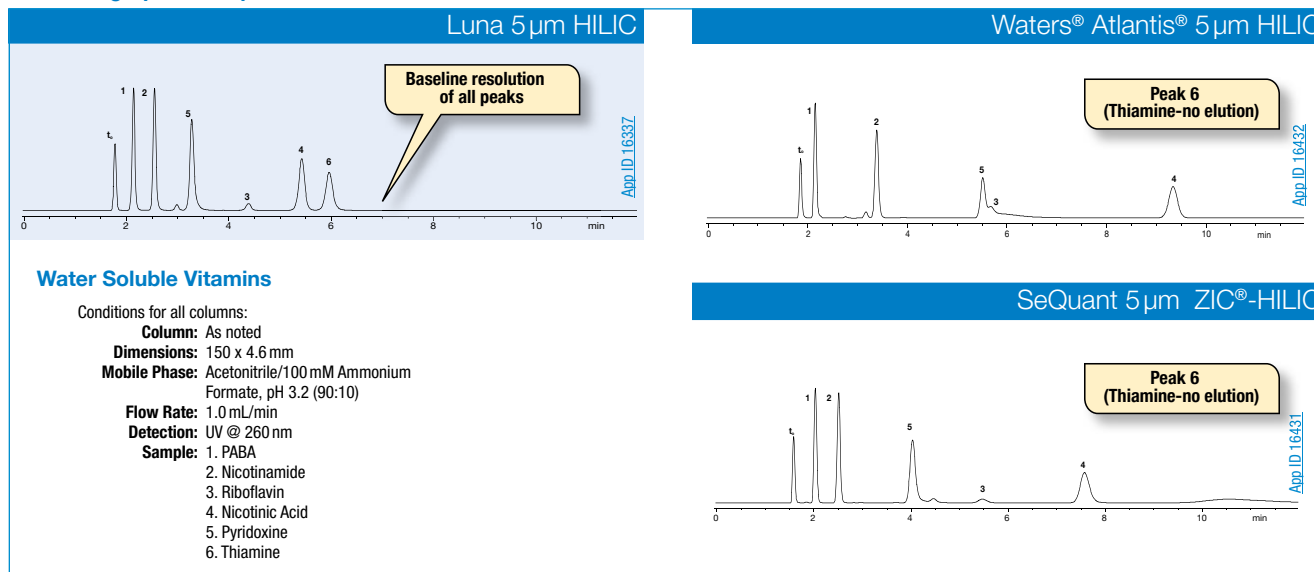

** The comparative data presented here may not be representative for all applications.

Luna PFP(2)


Powerful Selectivity for Reversed Phase Methods

Luna PFP(2) columns provide remarkable selectivity for highly polar compounds, complex natural products, isomers, and other closely related compounds. This is achieved by using a pentafluorophenyl with a propyl linkage which provides multiple retention mechanisms different to other reversed phase media.


- Achieve excellent selectivity using four mechanisms of solute/stationary phase interactions
- Extremely discerning for halogenated, aromatic and conjugated compounds
- Provides orthogonal selectivity even using traditional reversed phase mobile phase systems

Luna PFP(2) selectivity is achieved through 4 mechanisms of interaction

- Hydrogen Bonding
- Dipole-Dipole Interactions
- Aromatic and π - π Interactions
- Hydrophobic




A typical alkyl phase (C18, C8) achieves selectivity through only 1 mechanism of interaction.



Luna PFP(2)

Pentafluorophenyl groups provide very little hydrogen bonding abilities, but the strongly electronegative fluorine groups will provide good charge based selectivity for cationic compounds, while the rigid bonded phase is a good steric selector.


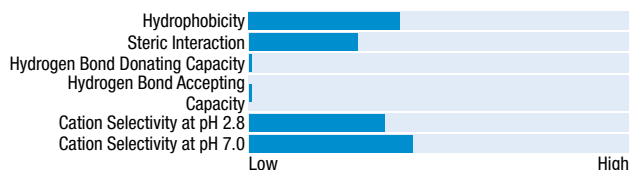


Aromatic Compounds

Aromatic compounds show different retention characteristics on Luna PFP(2) compared to traditional reversed phase columns. The presence of the aromatic benzene ring in Luna PFP(2) increases the relative attraction between the stationary phase and aromatic analytes, leading to increased retention for these types of compounds. Closely related polyphenolic compounds are readily separated with Luna PFP(2) columns.



Catechins

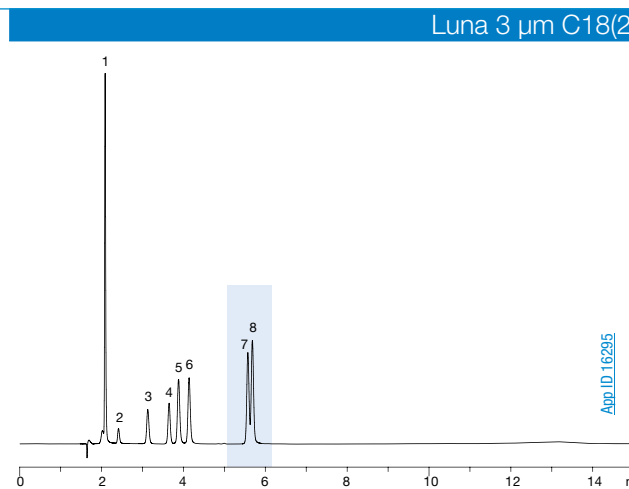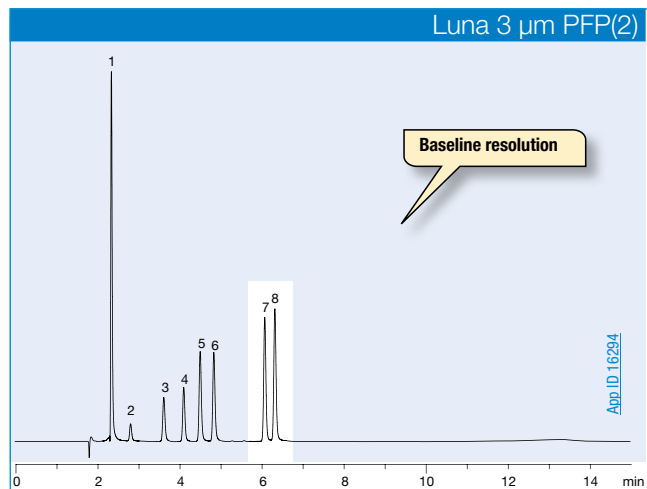

Columns: Luna 3 μ m PFP(2)
Luna 3 μ m C18(2)
Part Nos.: [00F-4447-E0](#)
[00F-4251-E0](#)

Conditions for all columns:

Dimensions: 150 x 4.6 mm
Mobile Phase: A: 0.1 % Formic acid in Water
B: 0.1 % Formic acid in Acetonitrile
Gradient: A/B (80:20) to (55:45) in 10 min
Flow Rate: 1 mL/min
Temperature: 22 °C
Detection: UV @ 280 nm

Sample: 1. Gallic acid
2. Epigallo catechin
3. Catechin
4. Epicatechin
5. Epigallocatechin gallate
6. Gallo catechin gallate
7. Epicatechin gallate
8. Catechin gallate

If Luna analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information

2.5 µm High Speed Technology (HST) Columns (mm)					
Phase	30 x 2.0	50 x 2.0	100 x 2.0	50 x 3.0	100 x 3.0
Luna 2.5 µm C18(2)-HST	00A-4446-BO	00B-4446-BO	00D-4446-BO	00B-4446-YO	00D-4446-YO



For information about HST Columns, contact your Phenomenex technical consultant or local distributor.

3 µm and 5 µm Capillary Columns (mm)					
Phases	50 x 0.30	150 x 0.30	50 x 0.50	150 x 0.50	250 x 0.50
3 µm C8(2)	—	—	00B-4248-AF	00F-4248-AF	—
3 µm C18(2)	00B-4251-AC	00F-4251-AC	00B-4251-AF	00F-4251-AF	—
5 µm C8(2)	—	00F-4249-AC	—	—	—
5 µm C18(2)	00B-4252-AC	00F-4252-AC	—	00F-4252-AF	00G-4252-AF
5 µm Phenyl-Hexyl	00B-4257-AC	—	00B-4257-AF	00F-4257-AF	—

MercuryMS™ LC-MS Cartridges (mm)						Columns (mm)	
3 µm	Phase	10 x 2.0	10 x 4.0	20 x 2.0	20 x 4.0	20 x 2.0	20 x 4.0
Luna	C18(2)	00N-4251-BO-CE	00N-4251-DO-CE	00M-4251-BO-CE	00M-4251-DO-CE	00M-4251-BO	00M-4251-DO
Luna	C8(2)	00N-4248-BO-CE	—	00M-4248-BO-CE	00M-4248-DO-CE	00M-4248-BO	—
5 µm	Phase	10 x 2.0	10 x 4.0	20 x 2.0	20 x 4.0	—	—
Luna	C18(2)	00N-4252-BO-CE	00N-4252-DO-CE	00M-4252-BO-CE	00M-4252-DO-CE	—	—
Luna	C8(2)	00N-4249-BO-CE	—	00M-4249-BO-CE	—	—	—

MercuryMS™ Cartridge Holders

Ordering Information

Direct-Connect Cartridge Holders

Part No.	Description
CHO-7187	10 mm direct-connect holder
CHO-7188	20 mm direct-connect holder

Standard Cartridge Holders

Part No.	Description
CHO-5846	10 mm standard holder
CHO-5845	20 mm standard holder



Direct-Connect Holder



Standard Holder

Ordering Information

3 µm Microbore and Minibore Columns (mm)							SecurityGuard Cartridges (mm)	
Phases	50 x 1.0	150 x 1.0	30 x 2.0	50 x 2.0	100 x 2.0	150 x 2.0	4 x 2.0*	
Silica(2)	—	00F-4162-AO	00A-4162-BO	00B-4162-BO	00D-4162-BO	00F-4162-BO	—	AJO-4347
C8(2)	00B-4248-AO	00F-4248-AO	00A-4248-BO	00B-4248-BO	00D-4248-BO	00F-4248-BO	—	AJO-4289
C18(2)	00B-4251-AO	00F-4251-AO	00A-4251-BO	00B-4251-BO	00D-4251-BO	00F-4251-BO	—	AJO-4286
CN	—	—	00A-4254-BO	00B-4254-BO	00D-4254-BO	00F-4254-BO	—	AJO-4304
Phenyl-Hexyl	00B-4256-AO	—	00A-4256-BO	00B-4256-BO	00D-4256-BO	00F-4256-BO	—	AJO-4350
NH ₂	—	00F-4377-AO	00A-4377-BO	00B-4377-BO	00D-4377-BO	00F-4377-BO	—	AJO-4301
HILIC	—	—	00A-4449-BO	00B-4449-BO	00D-4449-BO	00F-4449-BO	—	AJO-8328
PPP(2)	—	00F-4447-AO	00A-4447-BO	00B-4447-BO	00D-4447-BO	00F-4447-BO	—	AJO-8326

for ID: 2.0-3.0 mm

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJO-4282](#)



Luna[®] One of The World's Leading LC Columns

Ordering Information (continued)

3 µm MidBore™ and Analytical Columns (mm)									SecurityGuard™ Cartridges (mm)	
Phases	30 x 3.0	50 x 3.0	150 x 3.0	30 x 4.6	50 x 4.6	75 x 4.6	100 x 4.6	150 x 4.6	4 x 2.0*	4 x 3.0*
									/10pk	/10pk
Silica(2)	—	00B-4162-Y0	00F-4162-Y0	00A-4162-E0	00B-4162-E0	00C-4162-E0	00D-4162-E0	00F-4162-E0	AJO-4347	AJO-4348
C8(2)	00A-4248-Y0	00B-4248-Y0	00F-4248-Y0	00A-4248-E0	00B-4248-E0	00C-4248-E0	00D-4248-E0	00F-4248-E0	AJO-4289	AJO-4290
C18(2)	00A-4251-Y0	00B-4251-Y0	00F-4251-Y0	00A-4251-E0	00B-4251-E0	00C-4251-E0	00D-4251-E0	00F-4251-E0	AJO-4286	AJO-4287
CN	—	00B-4254-Y0	00F-4254-Y0	00A-4254-E0	00B-4254-E0	00C-4254-E0	00D-4254-E0	00F-4254-E0	AJO-4304	AJO-4305
Phenyl-Hexyl	—	00B-4256-Y0	00F-4256-Y0	00A-4256-E0	00B-4256-E0	00C-4256-E0	00D-4256-E0	00F-4256-E0	AJO-4350	AJO-4351
NH ₂	—	00B-4377-Y0	00F-4377-Y0	—	00B-4377-E0	—	00D-4377-E0	00F-4377-E0	AJO-4301	AJO-4302
HILIC	—	00B-4449-Y0	00F-4449-Y0	—	—	—	00D-4449-E0	00F-4449-E0	AJO-8328	AJO-8329
PPF(2)	—	00B-4447-Y0	00F-4447-Y0	—	00B-4447-E0	—	00D-4447-E0	00F-4447-E0	AJO-8326	AJO-8327

for ID: 2.0-3.0 mm 3.2-8.0 mm

5 µm Microbore and Minibore Columns (mm)								SecurityGuard™ Cartridges (mm)	
Phases	50 x 1.0	150 x 1.0	250 x 1.0	30 x 2.0	50 x 2.0	150 x 2.0	250 x 2.0	4 x 2.0*	
								/10pk	
Silica(2)	—	—	—	00A-4274-B0	00B-4274-B0	00F-4274-B0	00G-4274-B0	AJO-4347	
C5	—	—	—	00A-4043-B0	00B-4043-B0	00F-4043-B0	—	AJO-4292	
C8(2)	—	00F-4249-A0	—	00A-4249-B0	00B-4249-B0	00F-4249-B0	00G-4249-B0	AJO-4289	
C18(2)	00B-4252-A0	00F-4252-A0	00G-4252-A0	00A-4252-B0	00B-4252-B0	00F-4252-B0	00G-4252-B0	AJO-4286	
CN	—	—	—	—	00B-4255-B0	00F-4255-B0	—	AJO-4304	
Phenyl-Hexyl	00B-4257-A0	—	—	00A-4257-B0	00B-4257-B0	00F-4257-B0	00G-4257-B0	AJO-4350	
NH ₂	00B-4378-A0	00F-4378-A0	—	00A-4378-B0	00B-4378-B0	00F-4378-B0	00G-4378-B0	AJO-4301	
PPF(2)	—	—	—	00A-4448-B0	00B-4448-B0	00F-4448-B0	—	AJO-8326	

for ID: 2.0-3.0 mm



5 µm MidBore and Analytical Columns (mm)								SecurityGuard™ Cartridges (mm)	
Phases	30 x 3.0	50 x 3.0	150 x 3.0	250 x 3.0	30 x 4.6	50 x 4.6	75 x 4.6	4 x 2.0*	4 x 3.0*
								/10pk	/10pk
Silica(2)	—	00B-4274-Y0	00F-4274-Y0	—	—	00B-4274-E0	—	AJO-4347	AJO-4348
C5	—	—	00F-4043-Y0	—	—	00B-4043-E0	—	AJO-4292	AJO-4293
C8(2)	00A-4249-Y0	00B-4249-Y0	00F-4249-Y0	00G-4249-Y0	00A-4249-E0	00B-4249-E0	00C-4249-E0	AJO-4289	AJO-4290
C18(2)	00A-4252-Y0	00B-4252-Y0	00F-4252-Y0	00G-4252-Y0	00A-4252-E0	00B-4252-E0	00C-4252-E0	AJO-4286	AJO-4287
CN	—	00B-4255-Y0	00F-4255-Y0	00G-4255-Y0	00A-4255-E0	00B-4255-E0	00C-4255-E0	AJO-4304	AJO-4305
Phenyl-Hexyl	—	00B-4257-Y0	00F-4257-Y0	00G-4257-Y0	00A-4257-E0	00B-4257-E0	—	AJO-4350	AJO-4351
NH ₂	—	00B-4378-Y0	00F-4378-Y0	00G-4378-Y0	00A-4378-E0	00B-4378-E0	—	AJO-4301	AJO-4302
SCX	—	—	00F-4398-Y0	—	—	00B-4398-E0	—	AJO-4307	AJO-4308
HILIC	—	—	00F-4450-Y0	—	—	—	—	AJO-8328	AJO-8329
PPF(2)	—	00B-4448-Y0	00F-4448-Y0	—	—	00B-4448-E0	—	AJO-8326	AJO-8327

for ID: 2.0-3.0 mm 3.2-8.0 mm

5 µm Analytical and Semi-Prep Columns (mm)					SecurityGuard™ Cartridges (mm)	
Phases	100 x 4.6	150 x 4.6	250 x 4.6	250 x 10	4 x 3.0*	10 x 10 [‡]
					/10pk	/3pk
Silica(2)	00D-4274-E0	00F-4274-E0	00G-4274-E0	00G-4274-N0	AJO-4348	AJO-7223
C5	00D-4043-E0	00F-4043-E0	00G-4043-E0	00G-4043-N0	AJO-4293	AJO-7372
C8(2)	00D-4249-E0	00F-4249-E0	00G-4249-E0	00G-4249-N0	AJO-4290	AJO-7222
C18(2)	00D-4252-E0	00F-4252-E0	00G-4252-E0	00G-4252-N0	AJO-4287	AJO-7221
CN	00D-4255-E0	00F-4255-E0	00G-4255-E0	00G-4255-N0	AJO-4305	AJO-7313
Phenyl-Hexyl	00D-4257-E0	00F-4257-E0	00G-4257-E0	00G-4257-N0	AJO-4351	AJO-7314
NH ₂	00D-4378-E0	00F-4378-E0	00G-4378-E0	00G-4378-N0	AJO-4302	AJO-7364
SCX	00D-4398-E0	00F-4398-E0	00G-4398-E0	00G-4398-N0	AJO-4308	AJO-7369
HILIC	00D-4450-E0	00F-4450-E0	00G-4450-E0	00G-4450-N0	AJO-8329	AJO-8902
PPF(2)	00D-4448-E0	00F-4448-E0	00G-4448-E0	00G-4448-N0	AJO-8327	AJO-8376

for ID: 3.2-8.0 mm 9-16 mm

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJO-4282](#)

‡SemiPrep SecurityGuard™ Cartridges require holder, Part No.: [AJO-9281](#)

If Luna analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information (continued)

5 µm Axia™ Packed Preparative Columns (mm)								SecurityGuard™ Cartridges (mm)	
Phases	50 x 21.2	100 x 21.2	150 x 21.2	250 x 21.2	50 x 30	100 x 30	250 x 30	15 x 21.2**	15 x 30 *
								/ea	/ea
Silica(2)	—	00D-4274-PO-AX	00F-4274-PO-AX	00G-4274-PO-AX	—	—	00G-4274-UO-AX	AJO-7229	AJO-8312
C5	—	—	—	00G-4043-PO-AX	—	—	—	—	—
C8(2)	—	—	00F-4249-PO-AX	00G-4249-PO-AX	—	00D-4249-UO-AX	—	AJO-7840	AJO-8302
C18(2)	00B-4252-PO-AX	00D-4252-PO-AX	00F-4252-PO-AX	00G-4252-PO-AX	00B-4252-UO-AX	00D-4252-UO-AX	00G-4252-UO-AX	AJO-7839	AJO-8301
CN	—	—	—	00G-4255-PO-AX	—	—	00G-4255-UO-AX	AJO-8220	AJO-8311
Phenyl-Hexyl	—	—	00F-4257-PO-AX	00G-4257-PO-AX	—	—	00G-4257-UO-AX	AJO-7841	AJO-8303
NH ₂	—	—	00F-4378-PO-AX	00G-4378-PO-AX	—	—	—	AJO-8162	AJO-8309
PFP(2)	—	00D-4448-PO-AX	00F-4448-PO-AX	00G-4448-PO-AX	—	00D-4448-UO-AX	—	AJO-8377	AJO-8378
HILIC	—	00D-4450-PO-AX	00F-4450-PO-AX	00G-4450-PO-AX	—	—	00G-4450-UO-AX	AJO-8829	AJO-8830

for ID: 18-29 mm 30-49 mm

10 µm Axia™ Packed Preparative Columns (mm) (continued)					SecurityGuard Cartridges (mm)		
Phases	50 x 21.2	100 x 21.2	250 x 21.2	250 x 30	250 x 50	15 x 21.2**	15 x 30 *
						/ea	/ea
Silica(2)	—	—	00G-4091-PO-AX	00G-4091-UO-AX	00G-4091-VO-AX	AJO-7229	AJO-8312
C5	—	00D-4092-PO-AX	00G-4092-PO-AX	—	00G-4092-VO-AX	—	—
C8(2)	—	—	00G-4250-PO-AX	—	00G-4250-VO-AX	AJO-7840	AJO-8302
C18(2)	00B-4253-PO-AX	00D-4253-PO-AX	00G-4253-PO-AX	00G-4253-UO-AX	00G-4253-VO-AX	AJO-7839	AJO-8301
CN	—	—	00G-4300-PO-AX	—	—	AJO-8220	AJO-8311
Phenyl-Hexyl	—	—	00G-4285-PO-AX	00G-4285-UO-AX	—	AJO-7841	AJO-8303
NH ₂	—	—	00G-4379-PO-AX	—	—	AJO-8162	AJO-8309

for ID: 18-29 mm 30-49 mm

10 µm Analytical and Semi-Prep Columns (mm)			SecurityGuard Cartridges (mm)	
Phases	250 x 4.6	250 x 10	4 x 3.0*	10 x 10*
			/10 pk	/3 pk
Silica(2)	00G-4091-E0	00G-4091-N0	AJO-4348	AJO-7223
C8(2)	00G-4250-E0	00G-4250-N0	AJO-4290	AJO-7222
C18(2)	00G-4253-E0	00G-4253-N0	AJO-4287	AJO-7221
CN	00G-4300-E0	—	AJO-4305	AJO-7313
Phenyl-Hexyl	00G-4285-E0	00G-4285-N0	AJO-4351	AJO-7314
NH ₂	00G-4379-E0	00G-4379-N0	AJO-4302	AJO-7364
SCX	00G-4401-E0	00G-4401-N0	AJO-4308	AJO-7369

for ID: 3.2-8.0 mm 9-16 mm

15 µm Pilot Scale Columns (mm)	
Phases	250 x 4.6
C18(2)	00G-4273-E0
Phenyl-Hexyl	00G-4286-E0

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJO-4282](#)
 †SemiPrep SecurityGuard Cartridges require holder, Part No.: [AJO-9281](#)
 **PREP SecurityGuard Cartridges require holder, Part No.: [AJO-8223](#)
 ◆PREP SecurityGuard Cartridges require holder, Part No.: [AJO-8277](#)



See our latest developments in High-throughput Purifications starting on page 372
 For more dimensions and phases of Axia packed preparative columns, see p. 382
 For SecurityGuard Cartridge Holders and Cartridges, see p. 326
 For Bulk Media, see p. 383

Method development column kits and method validation column kits are available. Contact Phenomenex for details.



Improve analyte sensitivity and reduce baseline noise with Strata SPE tubes and well plates, see p. 67 for more information

If Luna analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Luna Omega Silica

The Luna Omega 1.6µm, 3µm, and 5µm particles build upon the Luna legacy with an innovative yet rugged UHPLC and HPLC silica particle architecture. The novel manufacturing process implements a proprietary processing technique to gain greater particle inertness, a stronger particle morphology, and more consistent porosity.

Thermal Modified Pore Structure

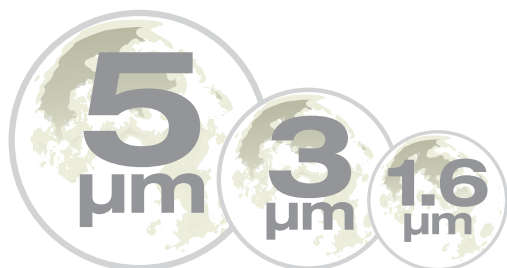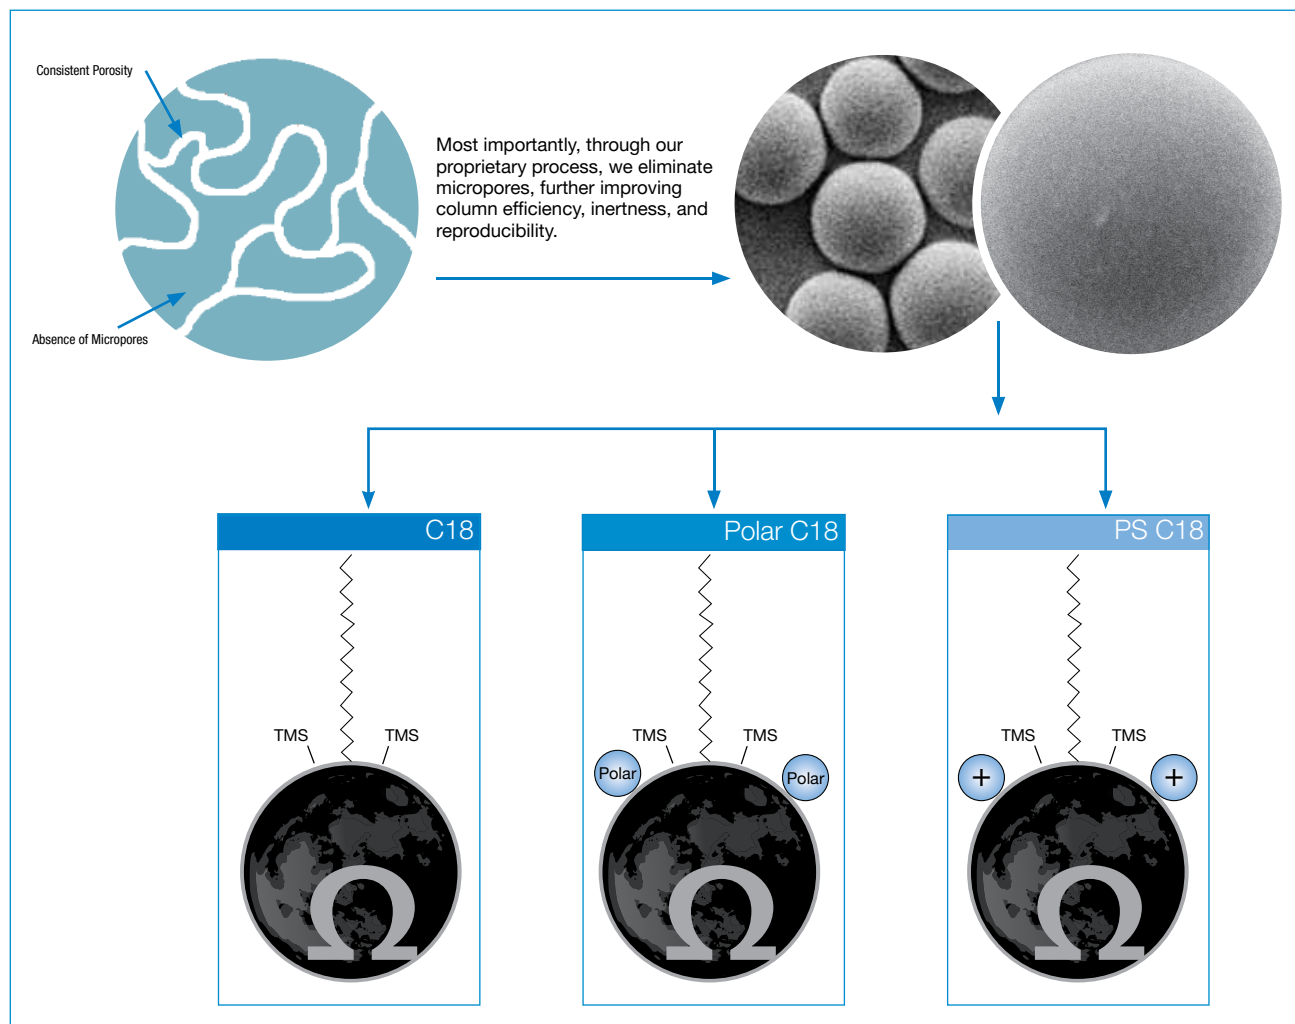


Astounding Performance

The undeniably high efficiency levels found in each Luna Omega UHPLC column provide you with the potential of huge gains in method performance. While traditional silica and hybrid fully porous

particles claim high performance, when compared to Luna Omega 1.6µm, they drastically fall short and prevent UHPLC scientists from reaching their UHPLC potential

UHPLC Efficiency Comparison

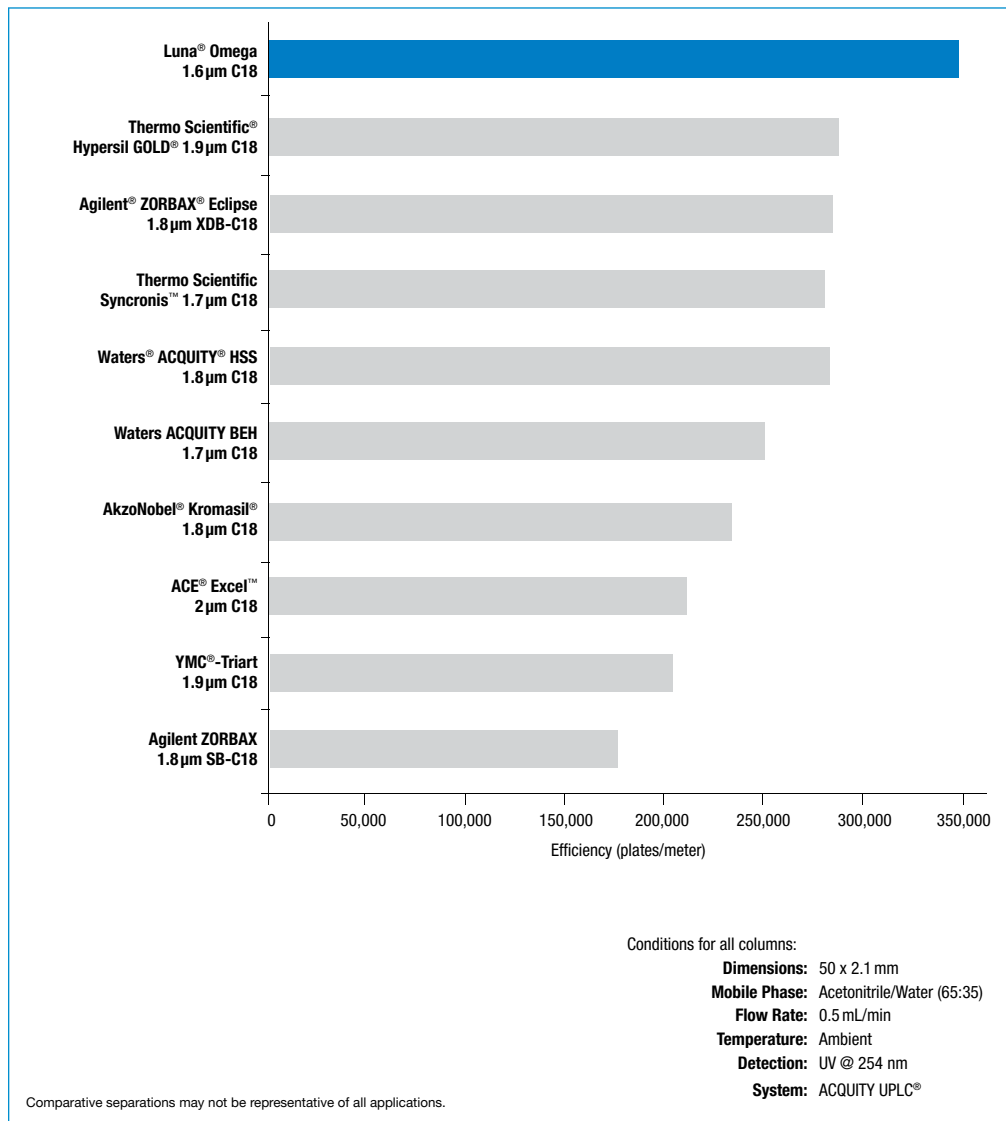


Luna Omega C18

Luna Omega C18 is an excellent first choice for chromatographers who are just starting method development or attempting to improve upon existing chromatographic results with other C18s. With its higher performance potential, excellent retention profile, and greater inertness, the Luna Omega C18 was designed to be the new all-purpose UHPLC solution for industries all over the world.

Materials Characteristics


Phase	Particle Sizes (µm)	Pore Size (Å)	Surface Area (m ² /g)	Carbon Load (%)	pH Stability	Pressure Limit	USP Column Classification
C18	1.6	100	260	11	1.5 - 8.5*	1000 bar	L1

*pH stability under gradient conditions. pH stability is 1.5-10 under isocratic conditions.

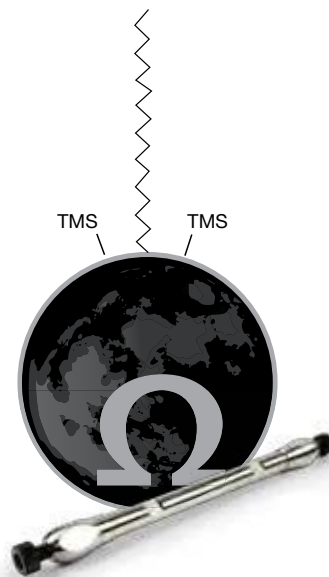

Greater Retention and Better Results

Higher efficiency levels in combination with excellent stationary phase coverage and greater particle inertness, translates to improved separation power for you. Now you can utilize the greater retention of Luna Omega C18 to tackle both easy and difficult separations.

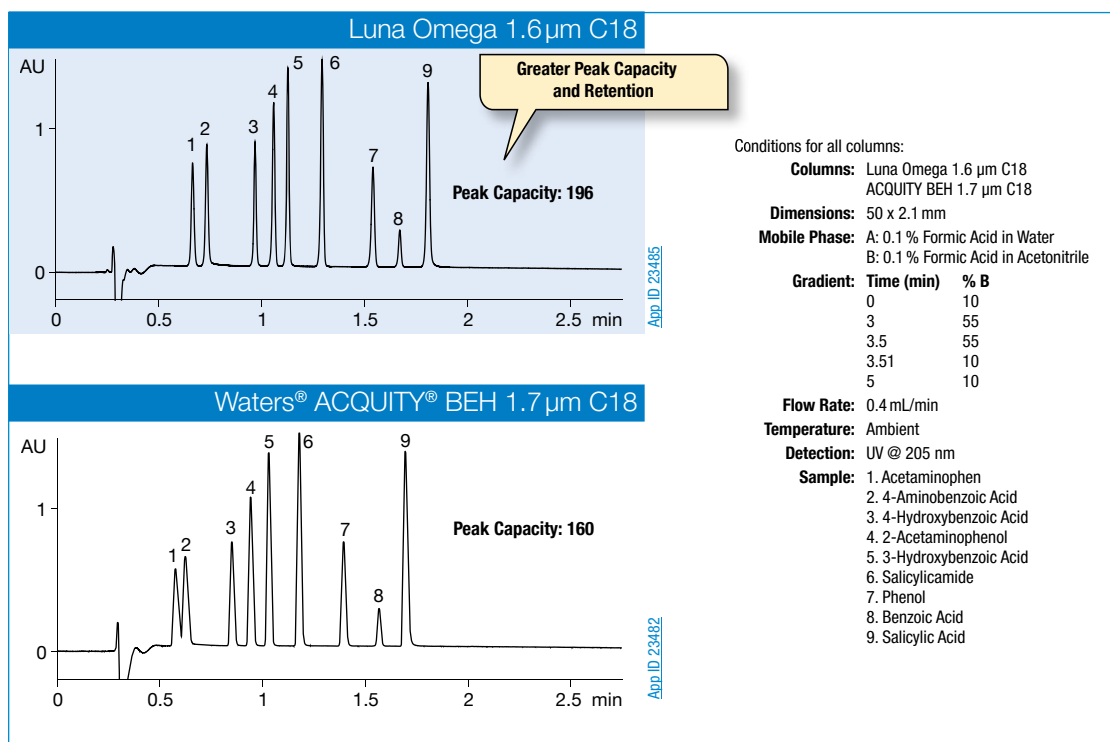


Comparative separations may not be representative of all applications.

Luna Omega C18 (cont'd)


Consistent Batch-to-Batch Reproducibility

Batch-to-batch and column-to-column, Luna Omega media and columns are designed to be consistent and incredibly accurate tools for your analysis. Each batch and column are quality tested to ensure dependability and reproducibility.


Luna Omega C18 – Batch A

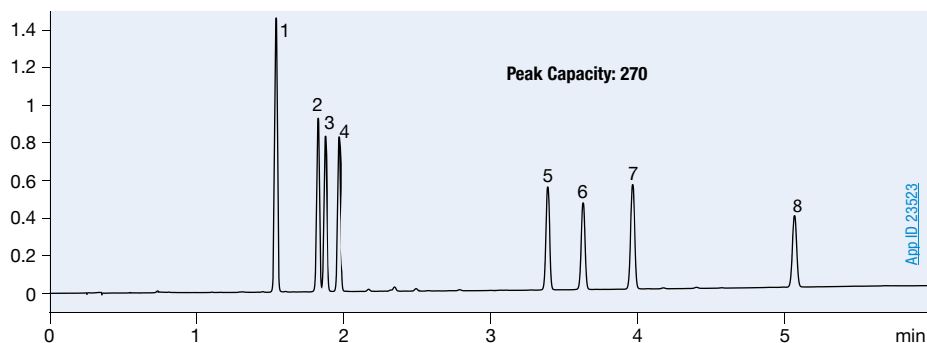

Luna Omega C18 – Batch B

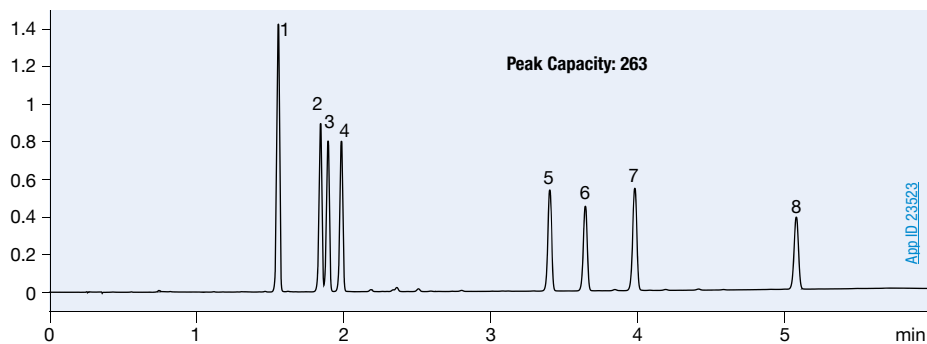

Luna Omega C18 – Batch C

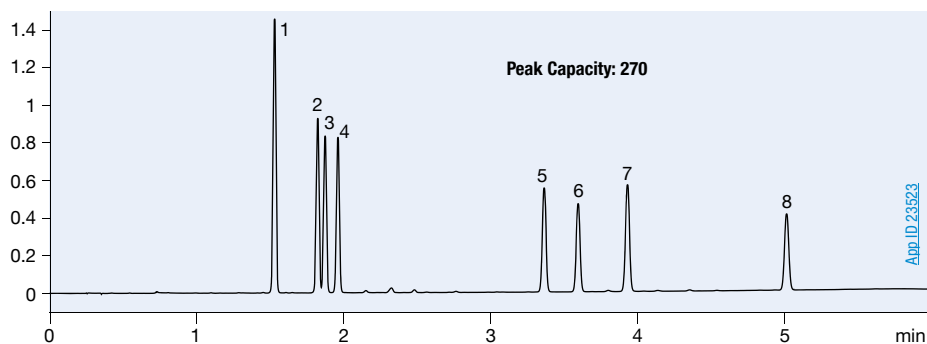

Conditions for all columns:

Columns: Luna Omega 1.6 µm C18

Dimensions: 50 x 2.1 mm

Part No.: [00B-4742-AN](#)

Mobile Phase: A: Water
B: Acetonitrile

Gradient:	Time (min)	% B
	0	20
	6	60
	6.01	20
	8	20

Flow Rate: 0.4 mL/min

Temperature: Ambient

Detection: UV @ 220 nm

Sample: 1. Estriol
2. Prednisolone
3. Hydrocortisone
4. Cortisone
5. Cortisone Acetate
6. 21-Hydroxycortisone
7. 17-Hydroxycortisone
8. Deoxycorticosterone




Luna Omega PS C18

Luna Omega PS C18 is a unique mixed-mode stationary phase that provides incredibly useful polar and non-polar retention. The surface of the PS C18 contains a positive charge which aids in the retention of acidic compounds through ionic interactions, while the C18 ligand promotes general reversed phase retention. This mixed-mode selectivity allows for greater separation between compounds with varying functional groups.

Materials Characteristics

Phase	Particle Sizes (µm)	Pore Size (Å)	Surface Area (m ² /g)	Carbon Load (%)	pH Stability	Pressure Limit	USP Column Classification
PS C18	1.6, 3, 5	100	260	9	1.5 - 8.5*	1000 bar	L1


*pH stability under gradient conditions. pH stability is 1.5-10 under isocratic conditions.

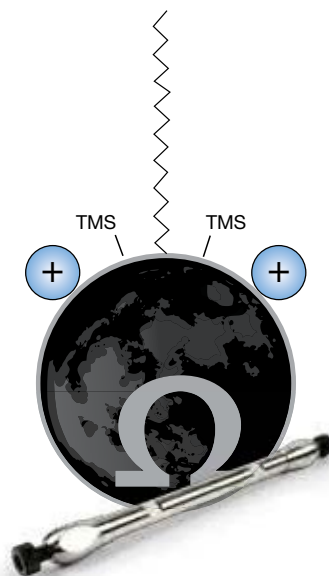


A C18, But More Positive

Luna Omega PS C18 has been fine-tuned and manufactured by Phenomenex to provide a mixed selectivity that is highly useful for method development involving either combinations of polars and non-polars, or just one single compound class with small changes in functional groups.

Luna Omega C18 silica surface

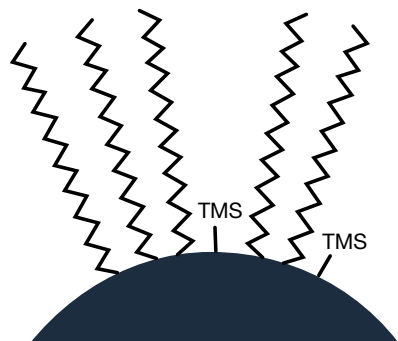

Luna Omega PS C18 silica surface

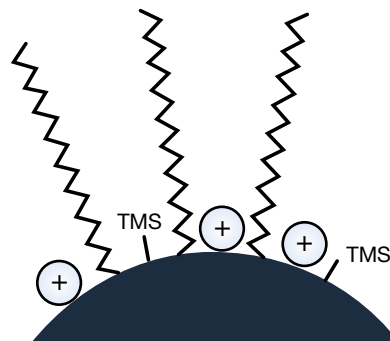


Luna Omega PS C18 (cont'd)


Better Peak Shape for Bases

While traditional alkyl phases are prone to show tailing for basic compounds because of secondary interactions occurring at the silica surface, the surface of the Luna Omega PS C18 was designed with positive charges that serve to repel strong basic species and consistently display sharp peak shape.

Pharmaceutical Compound Mixture

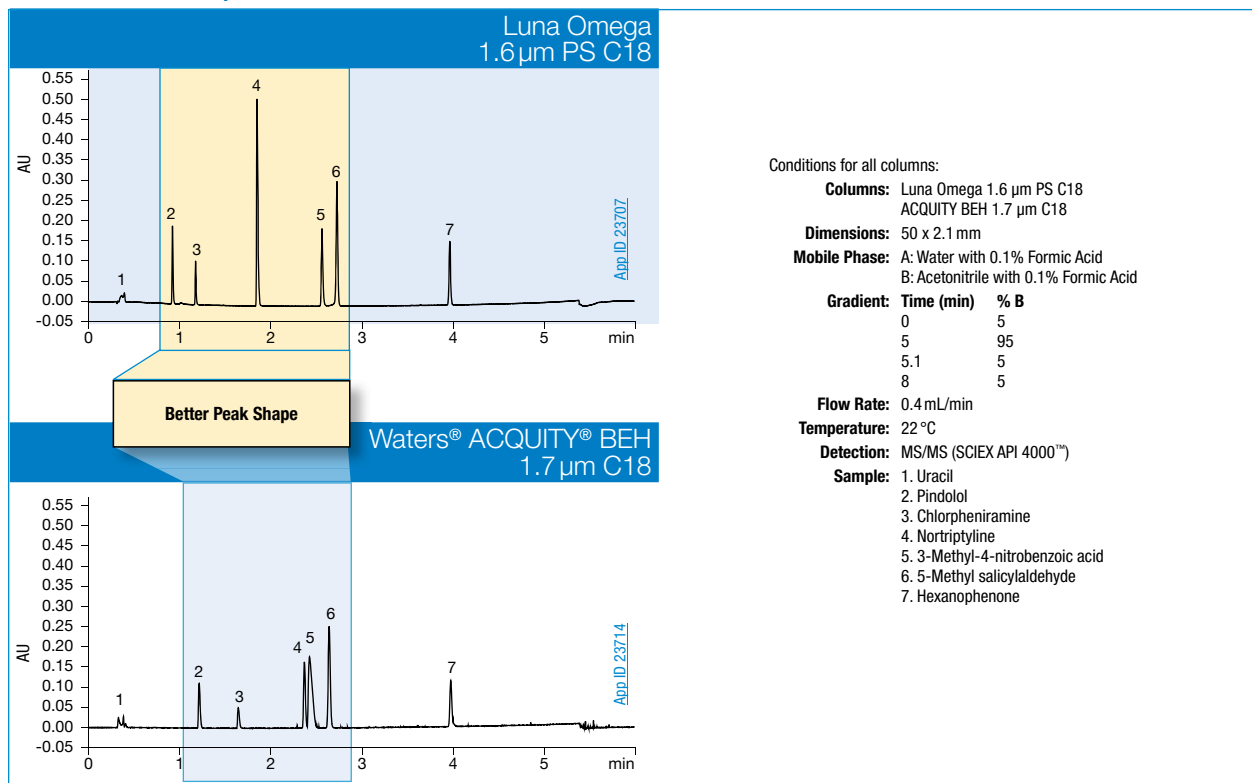

Intact Insulin

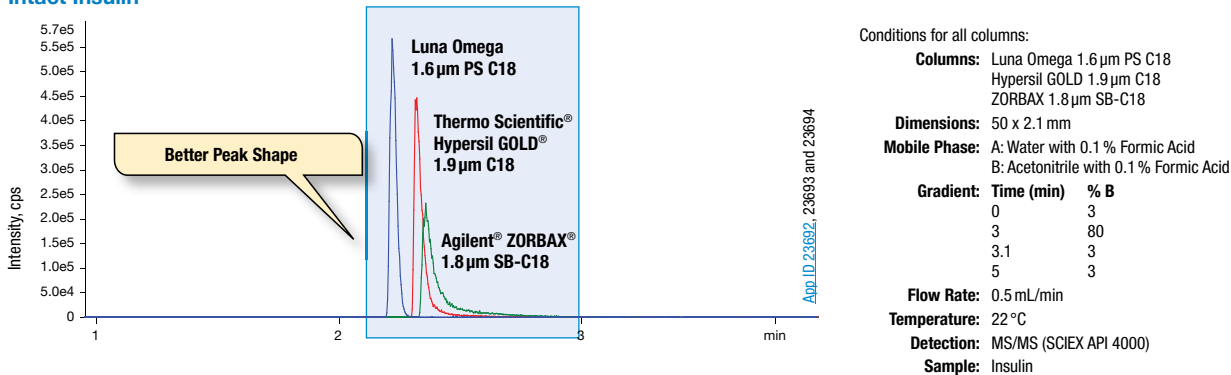

Comparative separations may not be representative of all applications.


Luna Omega Polar C18

Luna Omega Polar C18 is a novel UHPLC stationary phase capable of providing a unique selectivity within a wide elution window and increased retention for both polar and non-polar analytes. The all-purpose C18 ligand provides hydrophobic interactions while a polar modified particle surface provides enhanced polar retention and also aqueous stability. These attributes make the Luna Omega Polar C18 an excellent choice for balanced retention of polar and hydrophobic compounds as well as to solely enhance retention of highly polar compounds.

Materials Characteristics

Phase	Particle Sizes (µm)	Pore Size (Å)	Surface Area (m ² /g)	Carbon Load (%)	pH Stability	Pressure Limit	USP Column Classification
Polar C18	1.6, 3, 5	100	260	9	1.5 - 8.5*	1000 bar	L1


*pH stability under gradient conditions. pH stability is 1.5-10 under isocratic conditions.

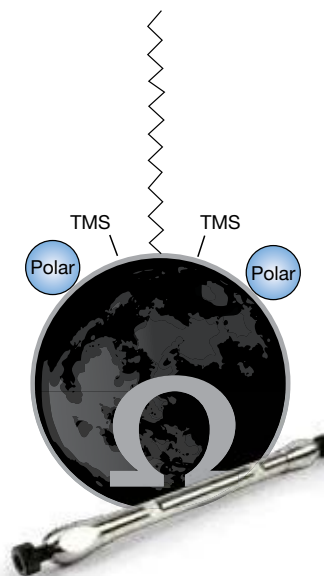


A C18, But Different

Luna Omega Polar C18 is a uniquely modified C18-based chemistry that has been optimized to improve the performance of polar analyses. This new particle surface chemistry makes the Polar C18 applicable to all industries that utilize UHPLC for mixtures of polar and non-polar compounds.

Luna Omega C18 silica surface

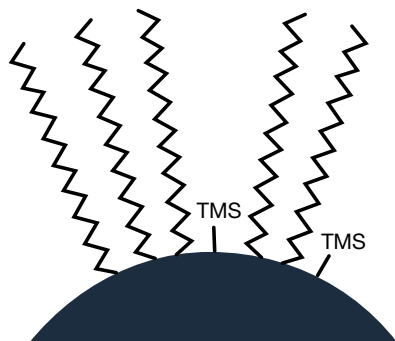

Luna Omega Polar C18 silica surface

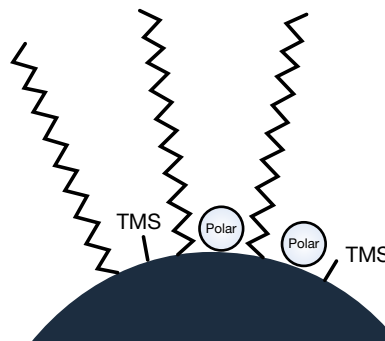


Luna Omega Polar C18 (cont'd)

No Stationary Phase Collapse

Traditional C18 phases are known to collapse under 100% aqueous conditions, causing retention loss of compounds and method development headaches. That is why an advanced proprietary bonding technology was used for the Luna Omega Polar C18 in order to ensure aqueous stability. The graph below displays the excellent stability of Polar C18 in 100% aqueous buffer conditions for over 2 weeks.


Aqueous Stability of Luna Omega Polar C18

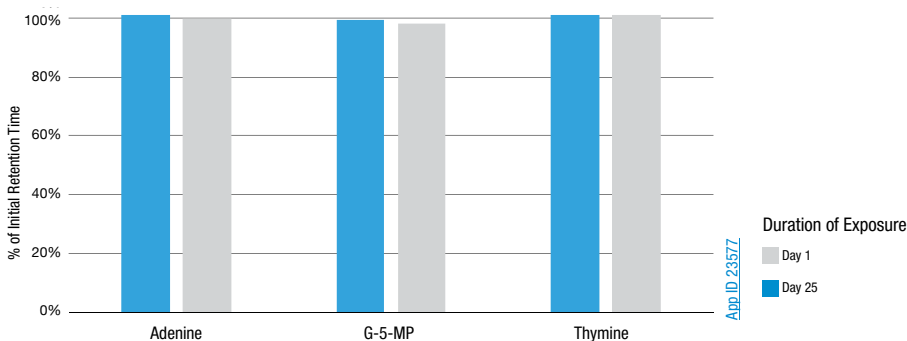

Conditions for all columns:

Columns: Luna Omega 1.6 µm Polar C18	Temperature: 22 °C
Dimension: 50 x 2.1 mm	Detection: UV @ 254 nm
Part No.: 00B-4748-AN	Sample: 1. Adenine
Mobile Phase: 10 mM Ammonium Formate with 0.1 % Formic Acid	2. Guanosine-5-Monophosphate
Flow Rate: 0.4 mL/min	3. Thymine

Nucleosides in 100% Aqueous Conditions

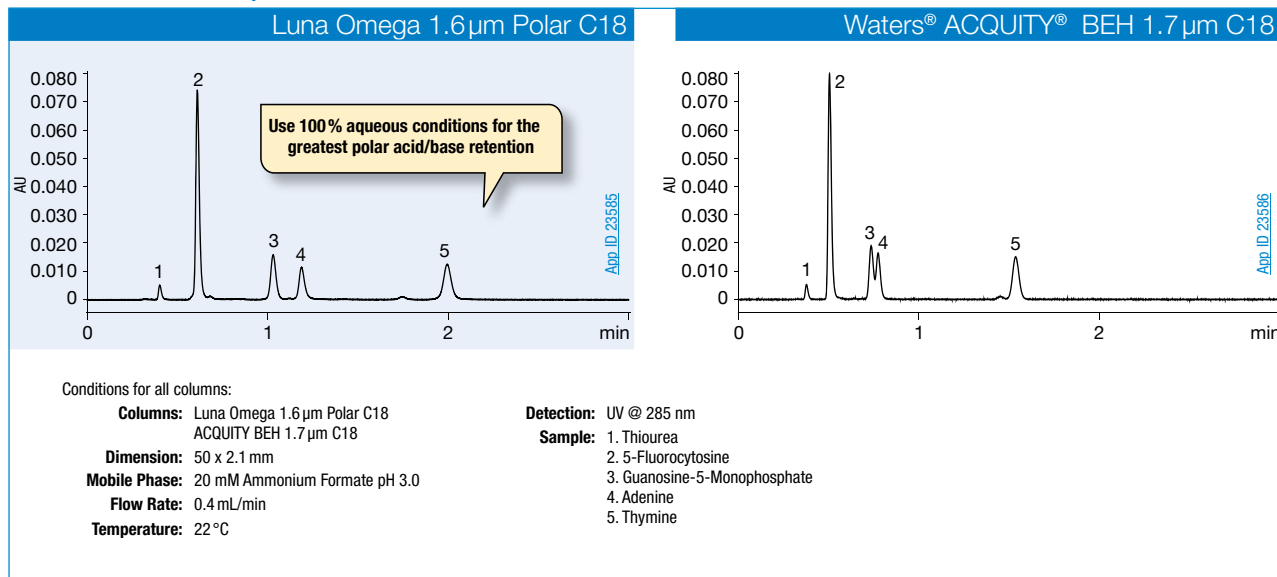

Comparative separations may not be representative of all applications.

If Luna analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information

1.6 µm Microbore Columns (mm)			
Phases	50 x 1.0	100 x 1.0	150 x 1.0
Polar C18	00B-4748-A0	00D-4748-A0	00F-4748-A0
C18	00B-4742-A0	00D-4742-A0	00F-4742-A0

1.6 µm Minibore Columns (mm)					SecurityGuard™ ULTRA Cartridges†
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	3/pk
Polar C18	00A-4748-AN	00B-4748-AN	00D-4748-AN	00F-4748-AN	AJ0-9505
PS C18	00A-4752-AN	00B-4752-AN	00D-4752-AN	00F-4752-AN	AJ0-9508
C18	00A-4742-AN	00B-4742-AN	00D-4742-AN	00F-4742-AN	AJ0-9502

for 2.1 mm ID

3 µm Minibore and MidBore™ Columns (mm)								SecurityGuard Cartridges (mm)
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	50 x 3.0	100 x 3.0	150 x 3.0	4 x 2.0* /10 pk
Polar C18	00A-4760-AN	00B-4760-AN	00D-4760-AN	00F-4760-AN	00B-4760-Y0	00D-4760-Y0	00F-4760-Y0	AJ0-7600
PS C18	00A-4758-AN	00B-4758-AN	00D-4758-AN	00F-4758-AN	00B-4758-Y0	00D-4758-Y0	00F-4758-Y0	AJ0-7605

for ID: 2.0-3.0 mm

3 µm Analytical Columns (mm)					SecurityGuard Cartridges (mm)
Phases	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0* /10 pk
Polar C18	00B-4760-E0	00D-4760-E0	00F-4760-E0	00G-4760-E0	AJ0-7601
PS C18	00B-4758-E0	00D-4758-E0	00F-4758-E0	00G-4758-E0	AJ0-7606

for ID: 3.2-8.0 mm

5 µm Minibore and MidBore™ Columns (mm)								SecurityGuard Cartridges (mm)
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	50 x 3.0	100 x 3.0	150 x 3.0	4 x 2.0* /10 pk
Polar C18	00A-4754-AN	00B-4754-AN	00D-4754-AN	00F-4754-AN	00B-4754-Y0	00D-4754-Y0	00F-4754-Y0	AJ0-7600
PS C18	00A-4753-AN	00B-4753-AN	00D-4753-AN	00F-4753-AN	00B-4753-Y0	00D-4753-Y0	00F-4753-Y0	AJ0-7605

for ID: 2.0 - 3.0 mm

5 µm Analytical Columns (mm)					SecurityGuard Cartridges (mm)
Phases	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0* /10 pk
Polar C18	00B-4754-E0	00D-4754-E0	00F-4754-E0	00G-4754-E0	AJ0-7601
PS C18	00B-4753-E0	00D-4753-E0	00F-4753-E0	00G-4753-E0	AJ0-7606

for ID: 3.2-8.0 mm

5 µm Semi-Preparative Columns (mm)		SecurityGuard Cartridges (mm)
Phases	250 x 10	10 x 10**
		/3 pk
Polar C18	00G-4754-N0	AJ0-9519
PS C18	00G-4753-N0	AJ0-9520

for ID: 9-16 mm

5 µm Axia Packed Preparative Columns (mm)						SecurityGuard Cartridges (mm)	
Phases	150 x 21.2	250 x 21.2	150 x 30	250 x 30	250 x 50	15 x 21.2**	15 x 30.0*
						/ea	/ea
Polar C18	00F-4754-P0-AX	00G-4754-P0-AX	00F-4754-U0-AX	00G-4754-U0-AX	00G-4754-V0-AX	AJ0-7603	AJ0-7604
PS C18	00F-4753-P0-AX	00G-4753-P0-AX	00F-4753-U0-AX	00G-4753-U0-AX	00G-4753-V0-AX	AJ0-7608	AJ0-7609

for ID: 18-29 mm

for ID: 30-49 mm



† SecurityGuard ULTRA Cartridges require holder, Part No.: [AJ0-9000](#)

* SecurityGuard Analytical Cartridges require holder, Part No.: [KJ0-4282](#)

***SemiPREP SecurityGuard Cartridges require holder, Part No.: [AJ0-9281](#)

**PREP SecurityGuard Cartridges require holder, Part No.: [AJ0-8223](#)

* PREP SecurityGuard Cartridges require holder, Part No.: [AJ0-8277](#)

If Lux analytical columns (≤ 4.6 mm ID) do not provide at least an equivalent or better chiral separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Replace CHIRALCEL[®] and CHIRALPAK[®] Columns at a Fraction of the Cost!









Lux coated and immobilized chiral columns are guaranteed to perform similar to or better than the equivalent DAICEL Chiral Technologies column of matching polysaccharide backbone and chiral selector at considerable cost savings. Lux phases can also provide alternative selectivity to other chiral selectors when separation is not achieved or when higher resolution is required.

Technical Specifications

Particle Size	3, 5, 10 ¹ , 20 ¹ μ m
pH Stability	2-9
Stability	Normal phase, polar organic, SFC, and reversed phase conditions
Maximum Pressure	300 bar
Temperature Range	0-50 °C
Shipping Solvent	n-Hexane/2-propanol (9:1, v/v)
Switching Solvent	Methanol/Ethanol (9:1, v/v)

¹Please inquire for availability

Resolve Over 92% of Your Enantiomers with Our Eight Coated and Immobilized Phases!

			
Lux i-Amylose-1 Amylose tris (3,5-dimethylphenylcarbamate)	Lux i-Cellulose-5 Cellulose tris (3,5-dichlorophenylcarbamate)	Lux Amylose-1 Amylose tris (3,5-dimethylphenylcarbamate)	Lux Amylose-2 Amylose tris (5-chloro-2-methylphenylcarbamate)
			
Lux Cellulose-1 Cellulose tris (3,5-dimethylphenylcarbamate)	Lux Cellulose-2 Cellulose tris (3-chloro-4-methylphenylcarbamate)	Lux Cellulose-3 Cellulose tris (4-methylbenzoate)	Lux Cellulose-4 Cellulose tris (4-chloro-3-methylphenylcarbamate)

Easily upgrade from your existing chiral columns to Lux LC/SFC columns!


If you are using one of the DAICEL [®] columns below:	Guaranteed alternative:	Phase description:
CHIRALPAK [®] IA [®] and IA-3	Lux i-Amylose-1	Amylose tris(3,5-dimethylphenylcarbamate)
CHIRALPAK [®] IC [®] and IC-3	Lux i-Cellulose-5	Cellulose tris(3,5-dichlorophenylcarbamate)
CHIRALPAK [®] AD [®] , AD-H [®] , AD-3, AD-RH [®] , and AD-3R	Lux Amylose-1	Amylose tris(3,5-dimethylphenylcarbamate)
CHIRALPAK [®] AY [®] , AY-H [®] , AY-3, AY-RH, and AY-3R	Lux Amylose-2	Amylose tris(5-chloro-2-methylphenylcarbamate)
CHIRALCEL [®] OD [®] , OD-H [®] , OD-3, OD-RH [®] , and OD-3R	Lux Cellulose-1	Cellulose tris(3,5-dimethylphenylcarbamate)
CHIRALCEL [®] OZ, OZ-H [®] , OZ-3, OZ-RH, and OZ-3R	Lux Cellulose-2	Cellulose tris(3-chloro-4-methylphenylcarbamate)
CHIRALCEL [®] OJ [®] , OJ-H [®] , OJ-3, OJ-RH [®] , and OJ-3R	Lux Cellulose-3	Cellulose tris(4-methylbenzoate)
CHIRALCEL [®] OX-H, OX-3, OX-RH, and OX-3R	Lux Cellulose-4	Cellulose tris(4-chloro-3-methylphenylcarbamate)

Lux Immobilized Chiral Selectors

The immobilization and bonding technology used within the Lux i-Cellulose-5 and i-Amylose-1 promotes column stability in strong organic solvents, which affords you the ability to expand your chiral separation success with more solvent systems and separations modes.

Expansive Strong Solvent Stability and Robustness

Strong Solvent Stability

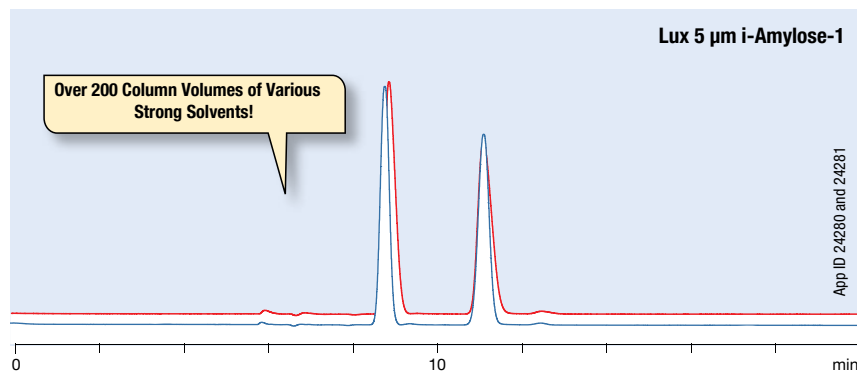

Conditions for all columns:


- Column:** Lux 5 µm i-Amylose-1
- Dimensions:** 250 x 4.6 mm
- Part No.:** [00G-4762-EQ](#)
- Mobile Phase:** 0.1% DEA in Hexane / 0.1% DEA in IPA (90:10)
- Flow Rate:** 1 mL/min
- Detection:** UV @ 260 nm
- Temperature:** 22 °C
- Sample:** Mianserin
- Column Exposed to:**
 1. MtBE
 2. Dichloromethane
 3. Ethyl Acetate
 4. THF
 5. Hexane
 6. Methanol
 7. Ethanol
 8. Isopropanol



Load Samples in Desired Strong Solvents

With the strong solvent stability of the Lux i-Cellulose-5 and i-Amylose-1 comes the ability to keep samples diluted in the strong

organic solvents that are needed for sample solubility or are directly from a reaction mixture.

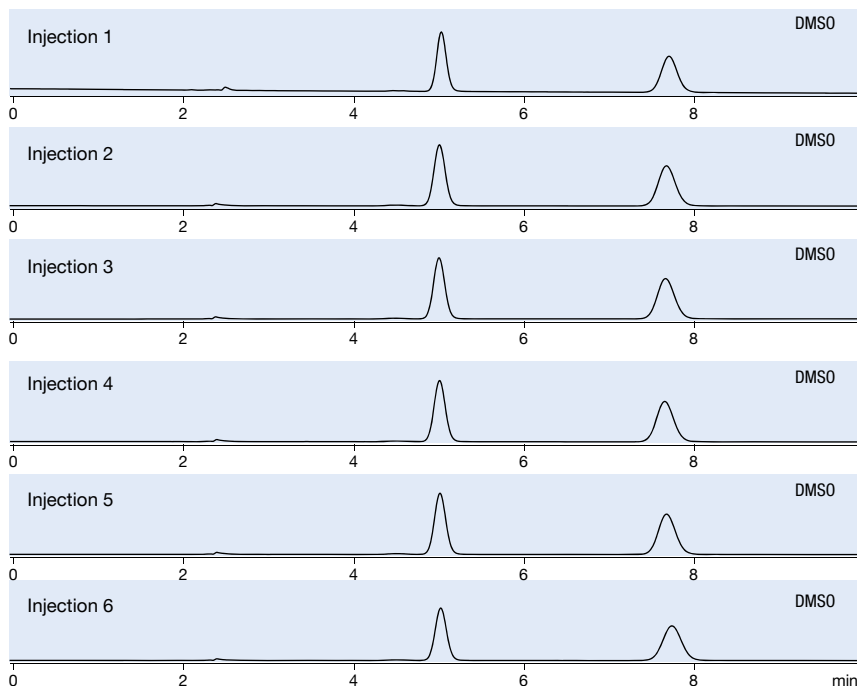

Conditions for all columns:

- Column:** Lux 5 µm i-Cellulose-5
- Dimensions:** 250 x 4.6 mm
- Part No.:** [00G-4756-EQ](#)
- Mobile Phase:** Methanol/DEA (100:0.1)
- Flow Rate:** 1.5 mL/min
- Detection:** UV @ 280 nm
- Temperature:** 27 °C
- Sample:** Laudanosine
- Dilution Solvent:** Dimethyl Sulfoxide (DMSO)

Unlock chiral

compound solubility issues by loading in strong organic solvents for preparative purifications on extremely robust Lux i-Cellulose-5 and i-Amylose-1 AXIA™ packed columns.



Lux Chiral Stationary Phases

The Lux line of coated and immobilized cellulose-based and amylose-based chiral stationary phases includes eight complementary selectivities.




Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.





Lux i-Amylose-1: Immobilized Dimethyl Amylose Chiral Selector

Known to have broad enantio-recognition, this incredibly popular Amylose tris (3,5-dimethylphenylcarbamate) chiral selector provides polar, electrostatic, hydrophobic, van der Waals, and other retention mechanisms.



Amylose tris(3,5-dimethylphenylcarbamate)

Tramadol

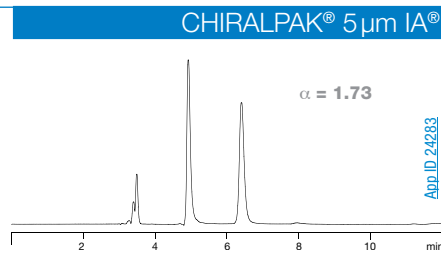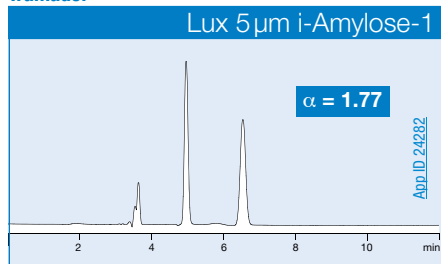

Conditions for both columns:


Dimensions: 250 x 4.6 mm

Mobile Phase: 0.1% DEA in Hexane /
0.1% DEA in IPA (90:10)

Flow Rate: 1 mL/min

Detection: UV @ 270 nm

Temperature: Ambient




Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.





Lux i-Cellulose-5: Immobilized Dichloro Cellulose Chiral Selector

The dichlorophenyl-moiety part of the i-Cellulose-5 selector creates a novel chiral selectivity by way of having two strong electron accepting atoms that draw the electron cloud of the phenyl ring outward.



Cellulose tris(3,5-dichlorophenylcarbamate)

Ornidazole

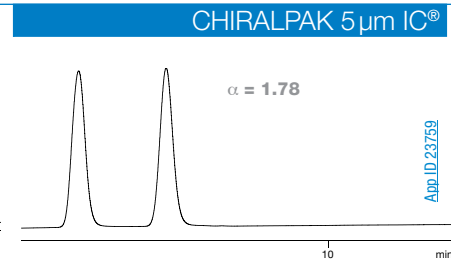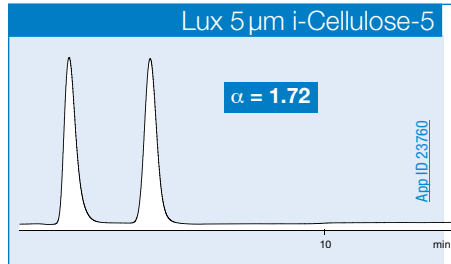

Conditions for both columns:


Dimensions: 250 x 4.6 mm

Mobile Phase: 0.1% Ethylamine in MtBE

Flow Rate: 1 mL/min

Detection: UV @ 254 nm

Temperature: Ambient




Columns used for comparison were manufactured by DANCEL Corporation. Phenomenex is in no way affiliated with DANCEL Corporation. Comparative separations may not be representative of all applications.



Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.


Lux Amylose-1: Dimethyl Amylose Chiral Selector

This universally trusted amylose phenylcarbamate derivative is absolutely essential to any chiral screen. Lux Amylose-1 is a guaranteed alternative to CHIRALPAK[®] AD[®]. Expect equivalent or better performance when using this Lux phase.



Amylose tris(3,5-dimethylphenylcarbamate)


Ketoprofen

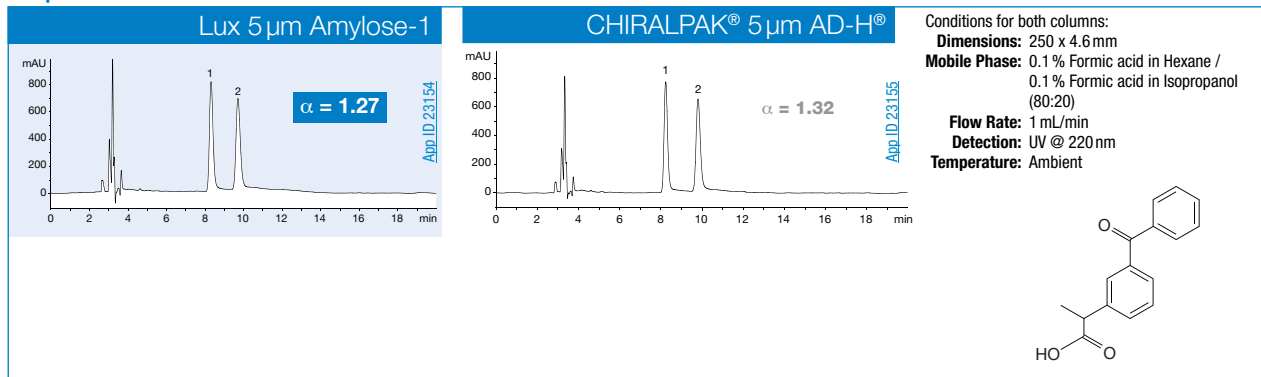

Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.


Lux Amylose-2: Chlorinated Amylose Chiral Selector

This first-to-market chlorinated amylose phenylcarbamate derivative offers complex chiral recognition components that greatly increase the chances of achieving chiral resolution.



Amylose tris(5-chloro-2-methylphenylcarbamate)

Ifenprodil

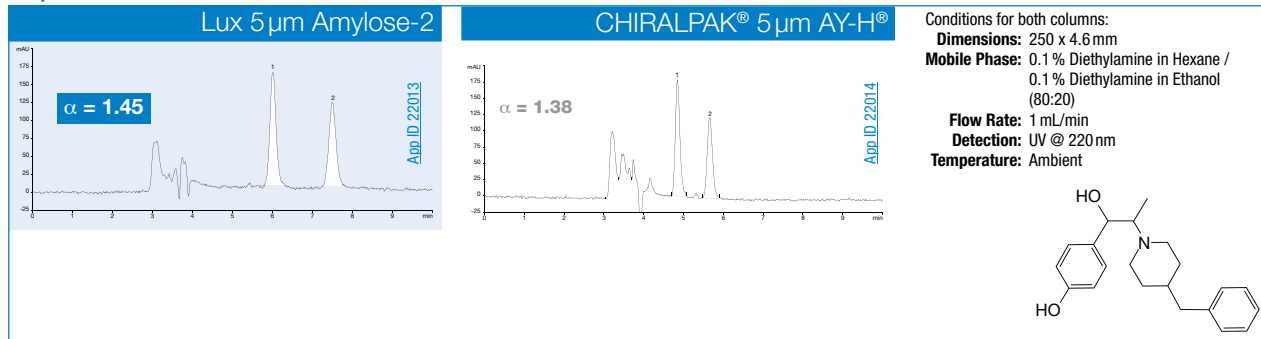


Comparative separations may not be representative of all applications.



Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.


Lux Cellulose-1: Dimethyl Cellulose Chiral Selector

This universally trusted cellulose phenylcarbamate derivative is absolutely essential to any chiral screen. Guaranteed alternative to CHIRALCEL[®] OD-H[®]. Expect equivalent or better performance.



Cellulose tris(3,5-dimethylphenylcarbamate)


Metoprolol

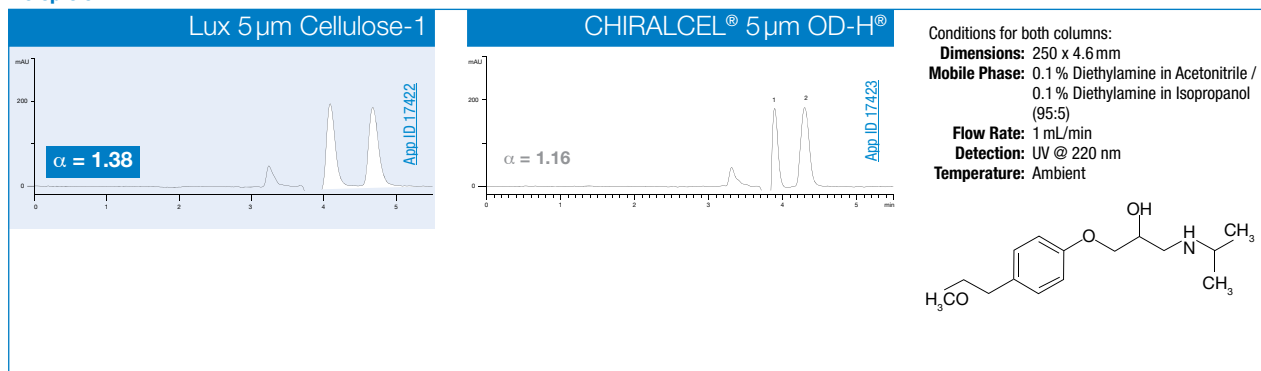

Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.


Lux Cellulose-2: Chlorinated Cellulose Carbamate Phase

This first-to-market halogenated cellulose phenylcarbamate derivative offers unique chiral recognition abilities that complement the rest of the Lux family of columns.



Cellulose tris(3-chloro-4-methylphenylcarbamate)

Alprenolol

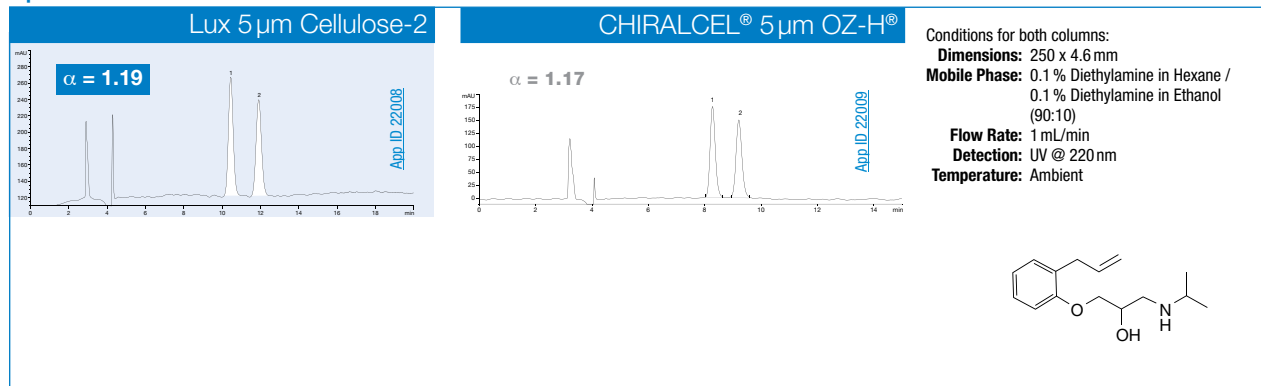


Comparative separations may not be representative of all applications.



Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.



Lux Cellulose-3: Cellulose Ester Phase

This cellulose methylbenzoate derivative offers distinct and complementary chiral recognition abilities.




Cellulose tris(4-methylbenzoate)

Disopyramide

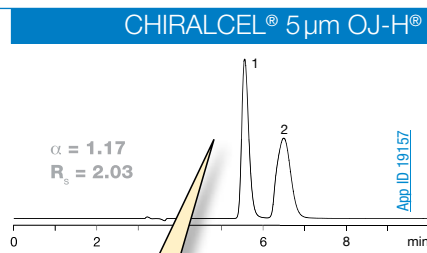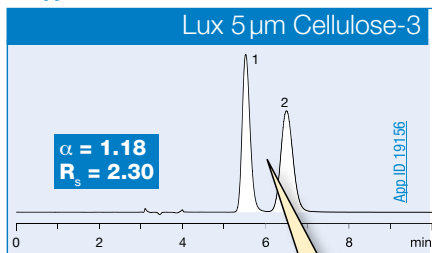

Similar Lux phases can offer equivalent, if not better, performance when compared to CHIRALCEL[®] and CHIRALPAK[®]


Conditions for both columns:
Dimensions: 250 x 4.6 mm
Mobile Phase: 0.1 % Diethylamine in Hexane / 0.1 % Diethylamine in Ethanol (90:10)
Flow Rate: 1 mL/min
Detection: UV @ 220 nm
Temperature: Ambient



Excellent separation at a fraction of the cost of DAICEL/Chiral Technologies.



Lux Cellulose-4: Chlorinated Cellulose Carbamate Phase

This chlorinated cellulose phenylcarbamate offers unique chiral recognition abilities.




Cellulose tris(4-chloro-3-methylphenylcarbamate)

Cyproconazole

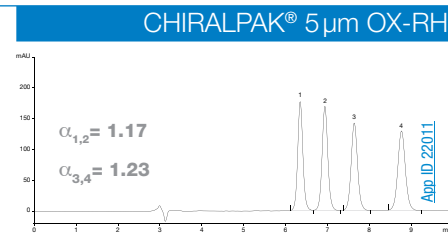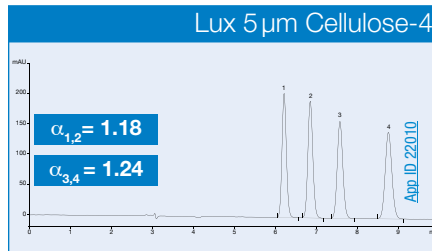

Conditions for both columns:
Dimensions: 250 x 4.6 mm
Mobile Phase: 0.1 % Diethylamine in Acetonitrile / 0.1 % Diethylamine in 20 mM Ammonium bicarbonate (60:40)
Flow Rate: 1 mL/min
Detection: UV @ 220 nm
Temperature: Ambient




Comparative separations may not be representative of all applications.


Achiral SFC Success with Chiral Columns!

While the incredible range of interaction mechanisms (polar, electrostatic, hydrophobic, van der Waals, and others) present in each Lux material are fundamental for ensuring baseline separation of chiral compounds, these same interaction mechanisms can also be used as an excellent screening tool for achiral work. Here we

present an achiral screening of natural cannabinoids using 7 Lux selectivities under one SFC mobile phase. The initial resolution and separation provided by the Lux Cellulose-2 was then further optimized to provide even greater resolution.

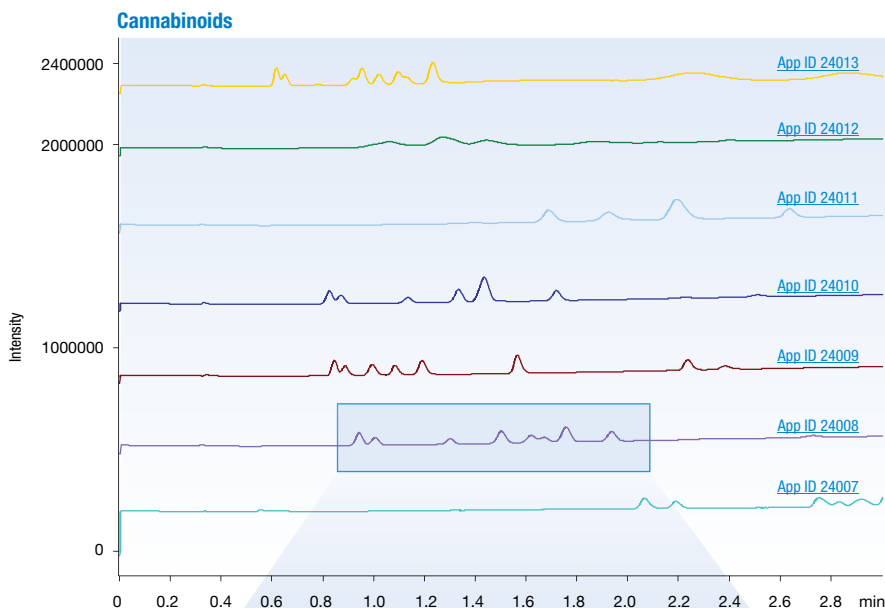

Expanded and optimized method separates achiral and chiral species!

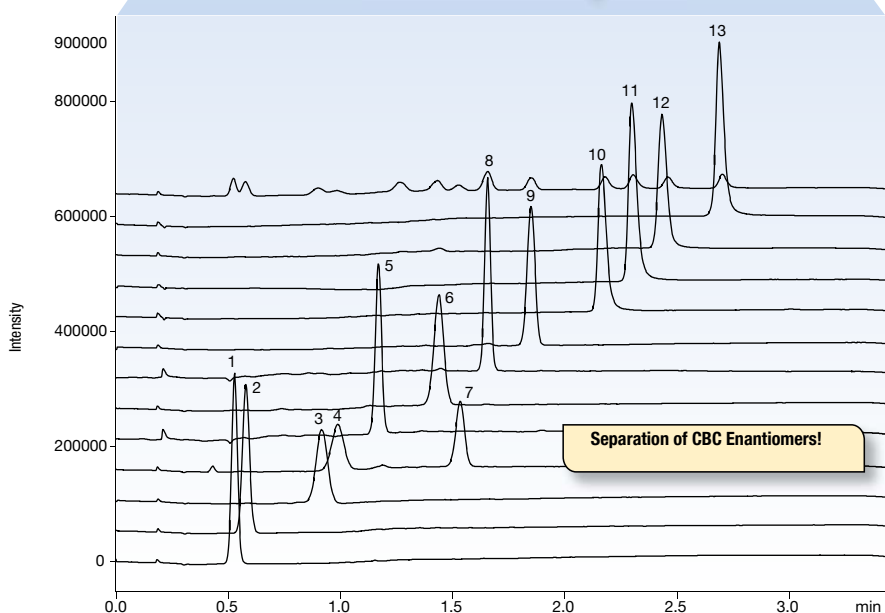

Conditions for all columns:

- Columns:** Lux 3 µm i-Cellulose-5
Lux 3 µm Amylose-2
Lux 3 µm Amylose-1
Lux 3 µm Cellulose-4
Lux 3 µm Cellulose-3
Lux 3 µm Cellulose-2
Lux 3 µm Cellulose-1
- Dimensions:** 150 x 3.0 mm
- Mobile Phase:** A: Carbon Dioxide
B: Methanol
- Gradient:**

Time (min)	% B
0	5
2.5	25
3	25
- Flow Rate:** 3 mL/min
- Detection:** UV @ 220 nm
- Temperature:** 40 °C
- Sample:** Cannabinoid mix of 8

- Column:** Lux 3 µm Cellulose-2
- Dimensions:** 150 x 3.0 mm
- Part No.:** [00F-4456-Y0](#)
- Mobile Phase:** A: Carbon Dioxide
B: Methanol
- Gradient:**

Time (min)	% B
0	4
3	25
3.5	25
- Flow Rate:** 5 mL/min
- Detection:** UV @ 220 nm
- Temperature:** 40 °C
- Sample:** Cannabinoid mix of 12

- | | |
|-----------------------|-----------|
| 1. CBDV | 8. THCV |
| 2. CBN | 9. CBG |
| 3. Delta-8-THC | 10. CBDA |
| 4. CBC (Enantiomer 1) | 11. CBDVA |
| 5. CBD | 12. THCA |
| 6. Delta-9-THC | 13. CBGA |
| 7. CBC (Enantiomer 2) | |



Axia™ Chiral Columns Out Perform Other Prep Columns


Axia specialized preparative hardware shows higher performance than traditionally packed standard hardware preparative columns. This revolutionary packing technology paired with Lux polysaccharide-based chiral stationary phases provide purification results like no other chiral column can provide.

To better understand how much Axia technology improves column performance over traditionally slurry packed preparative columns we scaled-up a 5 μm Lux Cellulose-1 chiral media analytical column and packed the same media into two different 150 x 21.2 mm ID


columns. One column was packed using Axia technology and the other prep column was packed using the traditional slurry packing process.

The Axia packing technology had a substantial increase in column efficiency resulting in increased resolution over traditionally packed preparative columns. With increased resolution you are able to increase your sample load enabling you to purify more target compound(s) per purification run. This equates to better throughput and economics.


Warfarin Chiral Purification in Normal Phase Mode

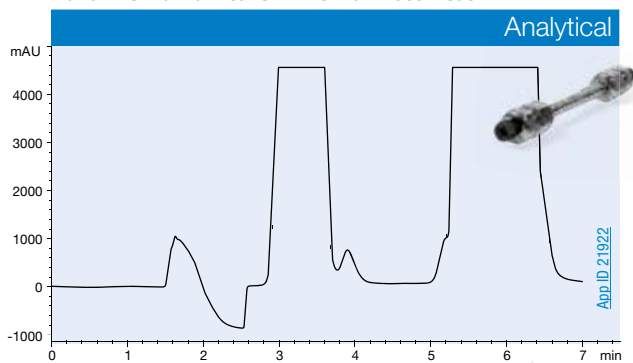


Column: Lux 5 μm Cellulose-1
Dimensions: 150 x 4.6 mm
Mobile Phase: Hexane/Ethanol (75:25)
Flow Rate: 1 mL/min
Temperature: Ambient
Inj. Volume: 100 μL



Standard Packing and Hardware

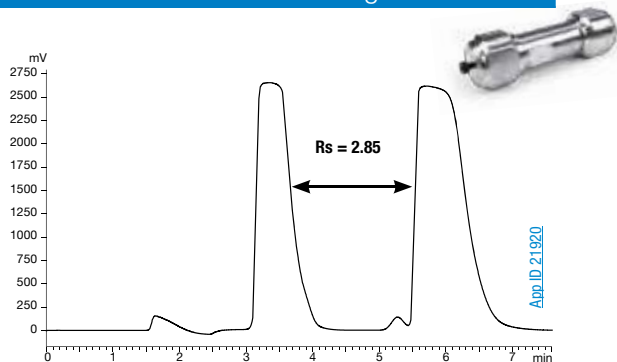

Axia Technology and Hardware

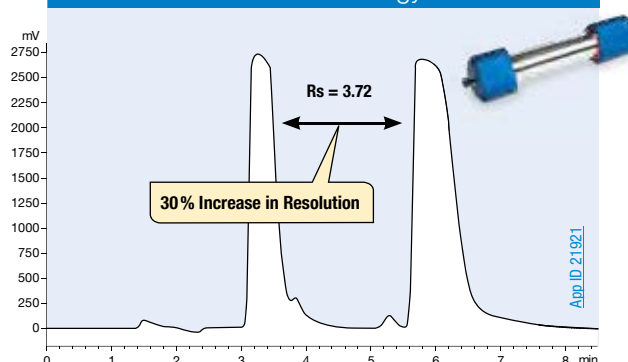

Conditions for both columns:
Media: Lux 5 μm Cellulose-1
Dimensions: 150 x 21.2 mm
Mobile Phase: Hexane / Ethanol (75:25)

Flow Rate: 20 mL/min
Temperature: Ambient
Inj. Volume: 2 mL

42% Increase in Efficiency

Column (mm)	Analytical 150 x 4.6	Standard 150 x 21.2	Axia 150 x 21.2
Mass Loaded (mg)	2	40	40
Resolution*	1.5	2.85	3.72
Plates (N)	117	535	760

“We have used Phenomenex Axia prep-HPLC columns for several years and they consistently provide excellent separation and reproducibility for a variety of different compounds.”

Jeremy R. Wolf
 ABC Laboratories, USA

* Resolution calculated with peak width at baseline and center retention time due to the overloaded peaks being off-scale

The opinions stated herein are solely those of the speaker and not necessarily those of any company or organization.



LUX[®] Chiral LC & SFC Columns

Ordering Information

3µm Minibore, MidBore™, and Analytical Columns (mm)									SecurityGuard™ Cartridges (mm)	
Phases	50 x 2.0	150 x 2.0	100 x 3.0	150 x 3.0	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 2.0*	4 x 3.0*
									/10pk	/10pk
i-Amylose-1	00B-4761-B0	00F-4761-B0	00D-4761-Y0	00F-4761-Y0	00B-4761-E0	00D-4761-E0	00F-4761-E0	00G-4761-E0	AJO-8640	AJO-8641
i-Cellulose-5	00B-4755-B0	00F-4755-B0	00D-4755-Y0	00F-4755-Y0	00B-4755-E0	00D-4755-E0	00F-4755-E0	00G-4755-E0	AJO-8631	AJO-8632
Cellulose-1	00B-4458-B0	00F-4458-B0	00D-4458-Y0	00F-4458-Y0	00B-4458-E0	00D-4458-E0	00F-4458-E0	00G-4458-E0	AJO-8402	AJO-8403
Cellulose-2	00B-4456-B0	00F-4456-B0	00D-4456-Y0	00F-4456-Y0	00B-4456-E0	00D-4456-E0	00F-4456-E0	00G-4456-E0	AJO-8398	AJO-8366
Cellulose-3	00B-4492-B0	00F-4492-B0	00D-4492-Y0	00F-4492-Y0	00B-4492-E0	00D-4492-E0	00F-4492-E0	00G-4492-E0	AJO-8621	AJO-8622
Cellulose-4	00B-4490-B0	00F-4490-B0	00D-4490-Y0	00F-4490-Y0	00B-4490-E0	00D-4490-E0	00F-4490-E0	00G-4490-E0	AJO-8626	AJO-8627
Amylose-1	00B-4729-B0	00F-4729-B0	00D-4729-Y0	00F-4729-Y0	00B-4729-E0	00D-4729-E0	00F-4729-E0	00G-4729-E0	AJO-9337	AJO-9336
Amylose-2	00B-4471-B0	00F-4471-B0	00D-4471-Y0	00F-4471-Y0	00B-4471-E0	00D-4471-E0	00F-4471-E0	00G-4471-E0	AJO-8471	AJO-8470

for ID: 2.0–3.0 mm 3.2–8.0 mm

5µm Minibore and Analytical Columns (mm)						SecurityGuard™ Cartridges (mm)	
Phases	50 x 2.0	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 2.0*	4 x 3.0*
						/10pk	/10pk
i-Amylose-1	—	00B-4762-E0	00D-4762-E0	00F-4762-E0	00G-4762-E0	AJO-8640	AJO-8641
i-Cellulose-5	—	00B-4756-E0	00D-4756-E0	00F-4756-E0	00G-4756-E0	AJO-8631	AJO-8632
Cellulose-1	00B-4459-B0	00B-4459-E0	00D-4459-E0	00F-4459-E0	00G-4459-E0	AJO-8402	AJO-8403
Cellulose-2	00B-4457-B0	00B-4457-E0	00D-4457-E0	00F-4457-E0	00G-4457-E0	AJO-8398	AJO-8366
Cellulose-3	00B-4493-B0	00B-4493-E0	00D-4493-E0	00F-4493-E0	00G-4493-E0	AJO-8621	AJO-8622
Cellulose-4	00B-4491-B0	00B-4491-E0	00D-4491-E0	00F-4491-E0	00G-4491-E0	AJO-8626	AJO-8627
Amylose-1	00B-4732-B0	00B-4732-E0	00D-4732-E0	00F-4732-E0	00G-4732-E0	AJO-9337	AJO-9336
Amylose-2	00B-4472-B0	00B-4472-E0	00D-4472-E0	00F-4472-E0	00G-4472-E0	AJO-8471	AJO-8470

for ID: 2.0–3.0 mm 3.2–8.0 mm

5µm Semi-Prep Columns (mm)			SecurityGuard™ Cartridges (mm)
Phases	150 x 10.0	250 x 10.0	10 x 10.0 [†]
			/3pk
i-Amylose-1	—	00G-4762-N0	AJO-8642
i-Cellulose-5	—	00G-4756-N0	AJO-8633
Cellulose-1 [†]	00F-4459-N0	00G-4459-N0	AJO-8404
Cellulose-2 [†]	00F-4457-N0	00G-4457-N0	AJO-8399
Cellulose-3	—	00G-4493-N0	AJO-8623
Cellulose-4	—	00G-4491-N0	AJO-8628
Amylose-1	—	00G-4732-N0	AJO-9344
Amylose-2	00F-4472-N0	—	AJO-8472

for ID: 9–16 mm

[†]Inquire for Lux 10µm Cellulose-1 and Cellulose-2 columns.

5µm Axia™ Packed Preparative Columns (mm)					SecurityGuard™ Cartridges (mm)	
Phases	150 x 21.2	250 x 21.2	250 x 30	250 x 50	15 x 21.2**	15 x 30.0*
					/ea	/ea
i-Amylose-1	00F-4762-P0-AX	00G-4762-P0-AX	00G-4762-U0-AX	00G-4762-V0-AX	AJO-8643	AJO-8644
i-Cellulose-5	00F-4756-P0-AX	00G-4756-P0-AX	00G-4756-U0-AX	00G-4756-V0-AX	AJO-8634	AJO-8635
Cellulose-1 [†]	00F-4459-P0-AX	00G-4459-P0-AX	00G-4459-U0-AX	00G-4459-V0-AX	AJO-8405	AJO-8406
Cellulose-2 [†]	00F-4457-P0-AX	00G-4457-P0-AX	00G-4457-U0-AX	00G-4457-V0-AX	AJO-8400	AJO-8401
Cellulose-3	00F-4493-P0-AX	00G-4493-P0-AX	00G-4493-U0-AX	00G-4493-V0-AX	AJO-8624	AJO-8625
Cellulose-4	00F-4491-P0-AX	00G-4491-P0-AX	00G-4491-U0-AX	00G-4491-V0-AX	AJO-8629	AJO-8630
Amylose-1	00F-4732-P0-AX	00G-4732-P0-AX	00G-4732-U0-AX	00G-4732-V0-AX	AJO-9338	AJO-9339

for ID: 18–29 mm 30–49 mm

*SecurityGuard Analytical Cartridges require holder, Part No.: [KJO-4282](#)
[†]SemiPrep SecurityGuard™ Cartridges require holder, Part No.: [AJO-9281](#)

**HPLC PREP SecurityGuard Cartridges require holder, Part No.: [AJO-8223](#)
 SFC PREP SecurityGuard Cartridges require holder, Part No.: [AJO-8617](#)

*HPLC PREP SecurityGuard Cartridges require holder, Part No.: [AJO-8277](#)
 SFC PREP SecurityGuard Cartridges require holder, Part No.: [AJO-8618](#)

Bulk Media		
Phases	100 g	1 kg
10 µm		
Cellulose-1	04G-4501	04K-4501
Cellulose-2	04G-4502	04K-4502
Cellulose-3	04G-4624	04K-4624
Cellulose-4	04G-4625	04K-4625
20 µm		
Cellulose-1	04G-4473	04K-4473
Cellulose-2	04G-4464	04K-4464
Cellulose-3	04G-4504	04K-4504
Cellulose-4	04G-4503	04K-4503

Please inquire for 20µm Lux Amylose-2 media.



guarantee

If Lux analytical columns (≤ 4.6 mm ID) do not provide at least an equivalent or better chiral separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Column Performance Check Standard

Part No.	Description	Unit
AL0-8412	Chiral Test Mix No. 5 (Lux)	ea



Lux Chiral Method Screening Kits are available. Please contact your Phenomenex representative for more information.








Rapid and Accurate Chiral Separation of Methamphetamine and Amphetamine Enantiomers from Urine

Lux 3 µm AMP is a unique LC media that is specifically developed and tested for the chiral analysis of amphetamine and substituted amphetamines, including methamphetamine. Once presence of amphetamine or methamphetamine has been determined, enantiomeric confirmation can then easily be achieved.

Not Affected by Common Interferences

Another excellent benefit of the Lux 3 µm AMP is that its separation of amphetamine and methamphetamine enantiomers isn't affected by common therapeutics and ingredients such as those seen below. In addition, the separation power of the Lux AMP column can also help with resolution between enantiomers of substituted amphetamines.

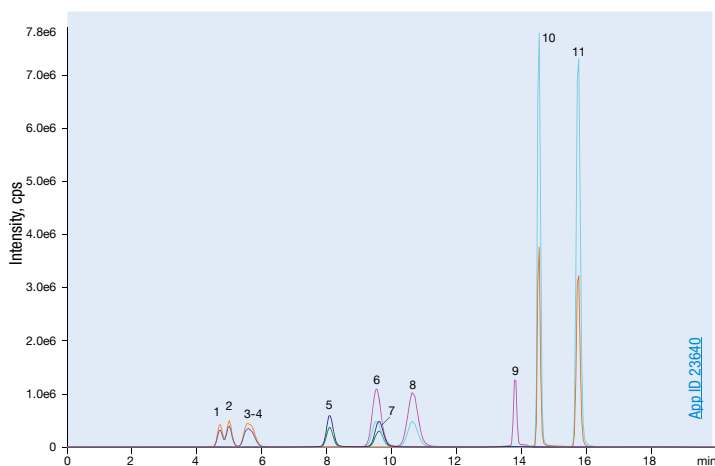

Column: Lux 3 µm AMP
Dimension: 150 x 3.0 mm
Part No.: 00F-4751-Y0
Mobile Phase: A: 5 mM Ammonium Bicarbonate, adjusted to pH 11 with Ammonium Hydroxide
 B: Methanol

Gradient	Time (min)	% B
	0	60
	10	60
	11	95
	16	95
	16.3	60

Flow Rate: 0.42 mL/min
Temperature: Ambient
Detection: MS/MS (SCIEX 4500 QTRAP[®])

- 1S,2R(+)-Ephedrine
2. R,R(-)-Pseudoephedrine
3. S,S(+)-Pseudoephedrine
4. 1R,2S(-)-Ephedrine
5. R(-)-Amphetamine
6. R(-)-Methamphetamine
7. S(+)-Amphetamine
8. S(+)-Methamphetamine
9. Phentermine
10. MDMA
11. MDMA

Compounds included in this interference study but not illustrated chromatographically:

- acetaminophen
- aspirin
- (±)-chlorpheniramine
- caffeine
- diphenhydramine
- dextromethorphan
- ibuprofen
- (±)-MDA
- (±)-MDEA
- phenylephrine
- norephedrine

1-Minute β-Glucuronidase Removal

Within 1 minute, with no necessary method development, your samples will be ready for analysis.

Learn more at:
www.phenomenex.com/beta-gone
 or visit p. 54




If Lux analytical columns (≤ 4.6 mm ID) do not provide at least an equivalent or better chiral separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.


Exceptional Reliability

Lux 3 μm AMP media and columns are designed to be consistent and incredibly accurate tools for amphetamine and methamphetamine analysis. Each batch is specifically tested by LC-MS for the analysis of amphetamine and methamphetamine, and columns are quality tested to ensure dependability and reproducibility.


Amphetamine Enantiomers

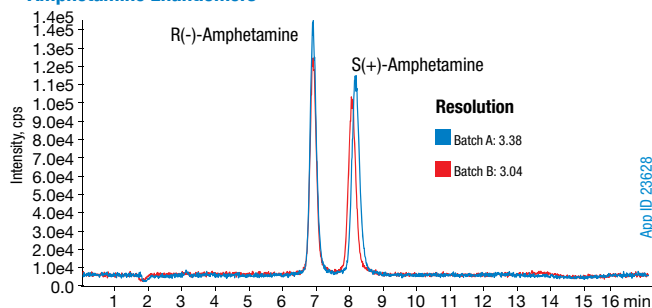

Methamphetamine Enantiomers

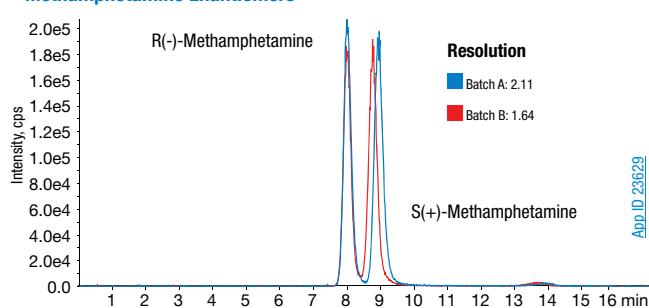

Ephedrine and Pseudoephedrine

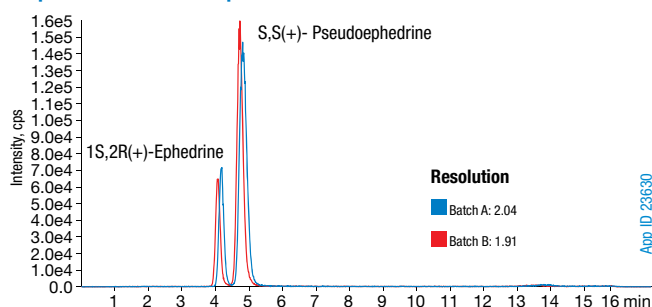


Column: Lux 3 μm AMP
Dimension: 150 x 3.0 mm
Part No.: 00F-4751-Y0
Mobile Phase: A: 5 mM Ammonium Bicarbonate, adjusted to pH 11 with Ammonium Hydroxide
 B: Methanol
Gradient:

Time (min)	% B
0	60
10	60
11	95
13	95
13.1	60

Temperature: 22 °C
Sample: 1. Ephedrine
 2. Pseudoephedrine
 3. R(-)-Amphetamine
 4. S(+)-Amphetamine
 5. R(-)-Methamphetamine
 6. S(+)-Methamphetamine
Flow Rate: 0.42 mL/min



Excellent Lifetime

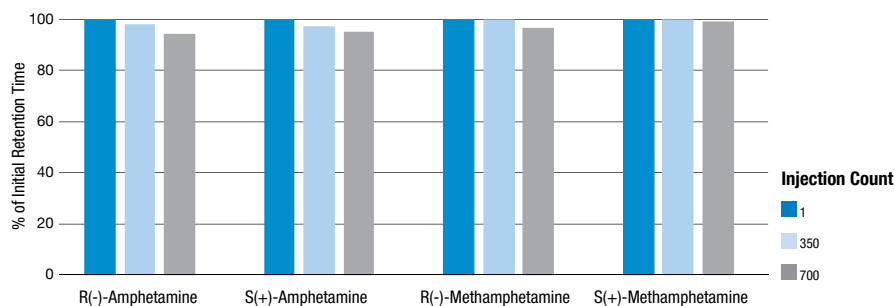

Ordering Information

Phase	3 μm Analytical Columns (mm)		SecurityGuard™ Cartridges (mm)	
	150 x 3.0	150 x 4.6	4 x 2.0*	4 x 3.0*
AMP	00F-4751-Y0	00F-4751-E0	10/pk AJ0-8475	10/pk AJ0-8476
	for ID:		2.0 - 3.0 mm	3.2 - 8.0 mm

SecurityGuard Cartridges require holder, Part No.: [KJ0-4282](#)

MERCK KGaA, Darmstadt, Germany, Products

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit:
www.phenomenex.com/lichrosorb and www.phenomenex.com/lichrospher

Nucleosil®

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit:
www.phenomenex.com/nucleosil

If Onyx analytical columns do not provide at least an equivalent separation as compared to a competing column of the same monolithic characteristics, similar phase, and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Finish First with Monolithic Silica HPLC Columns

Onyx is a silica monolithic HPLC column designed for high speed analysis. The monolithic nature allows for "dilute-and-shoot" applications saving scientists valuable sample preparation time.

- Reduce run times by more than 50 %
- "Dilute-and-Shoot" dirty biological samples
- Analytical, capillary, and semi-prep dimensions



Material Characteristics

Packing Material	Macropore Size (µm)	Mesopore Size (Å)	Pore Volume (mL/g)	Surface Area (m²/g)	Carbon Load %	Calculated Bonded Phase Coverage (µmole/m²)	End Capping
Onyx C8	2	130	1.0	300	11	3.8	Yes
Onyx C18	2	130	1.0	300	18	3.6	Yes
Onyx C18*	1.5	130	1.0	300	18	3.6	Yes
Onyx HD-C18	1	130	1.0	300	18	3.6	Yes

Maximum Pressure: 200 Bar; pH Range: 2.0-7.5

*50 x 2.0 mm ID only; enhanced 1.5 µm macropore size for higher efficiencies

High Resolution Monolithic Columns — Onyx HD-C18

- 50% higher performance compared to our standard Onyx columns
- Backpressure 2 times lower than particle packed columns
- 30% longer column lifetime compared to some particle packed columns

Monolithic Technology vs. Particle-Based Technology

Onyx

- **Monolithic porous silica rod**
- **Significantly shorter run times**
Cut methods by more than half
- **Low backpressures**
Less stress on system and column
- **High flow rates**
Due to high porosity
- **No inlet bed settling**
Increased reliability, reproducibility, and lifetime



Particle-Based Columns


- **Individual silica particles**
- **High flow resistance**
Limits ability to shorten run times
- **Increased backpressure**
Limits life of pumps, seals, and column
- **Reduced throughput**
Long run times
- **Bed splitting possible**
Shortens column life & lessens reproducibility



Dramatically Increase Throughput and Reduce Analysis Time

Onyx columns can be used in a variety of reversed phase methods - anytime you want the advantage of speed and throughput, put Onyx to the test!

Increased Resolution of Steroids with Onyx HD-C18

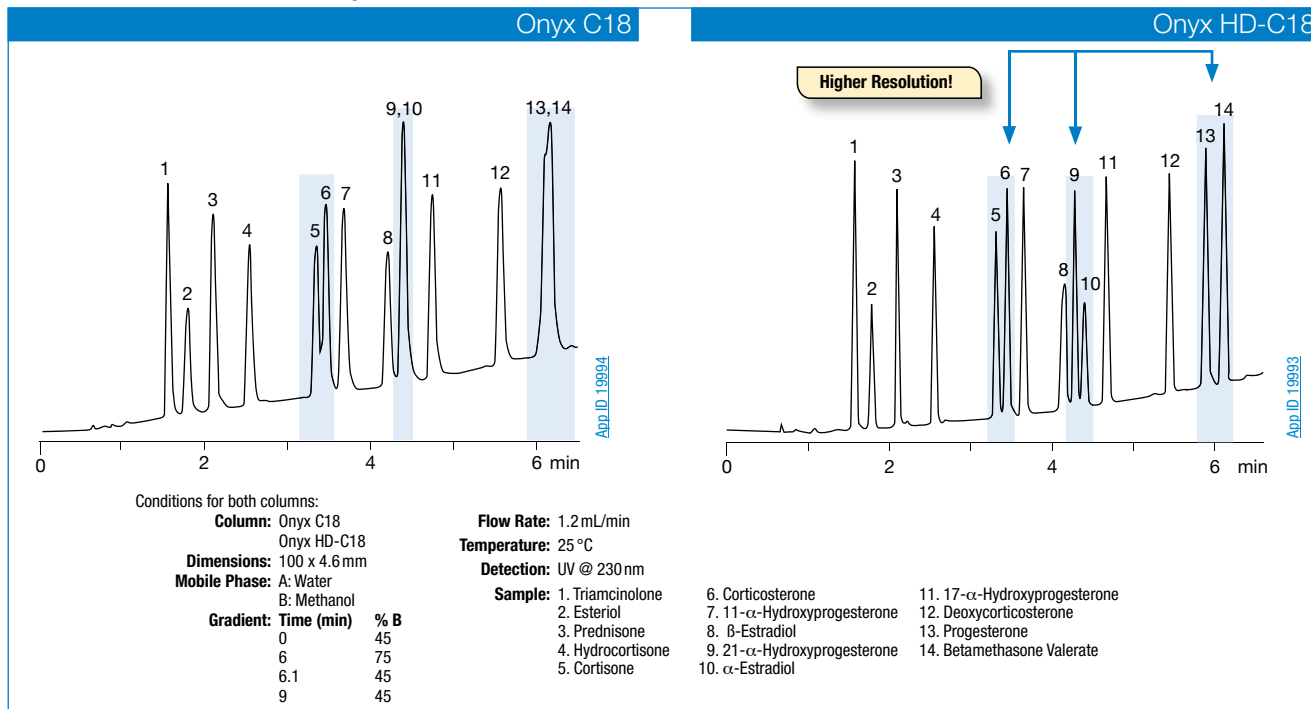


Extremely Low Backpressure

The very high porosity of Onyx columns result in very low backpressures, even at high flow rates. Onyx silica monolithic columns rarely exceed 100 bar, even at 9 mL/min, while particle-based columns reach backpressure limits at much lower flow rates.

- Typically 60% less backpressure than particle-based columns
- Couple columns together to produce extremely high plate counts to separate critical pairs
- Minimal worry of system shutdowns from high backpressure


Backpressure vs. Flow Rate

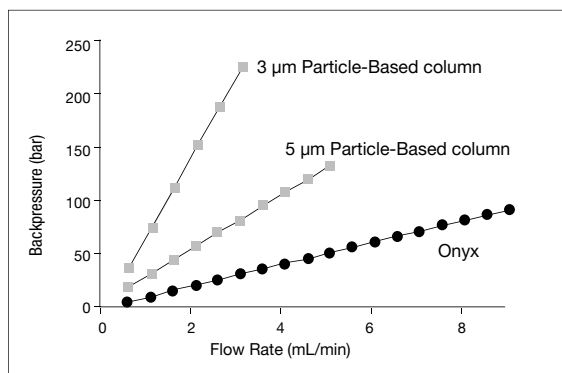

- Option to run from 1 mL/min up to 9 mL/min
- Reduce re-equilibration time from sample to sample
- Shorten total separation time once target compound has eluted with flow gradient options

High Efficiencies

Onyx 2.0mm ID columns have a reduced macropore of 1.5 μ m, providing excellent efficiencies.

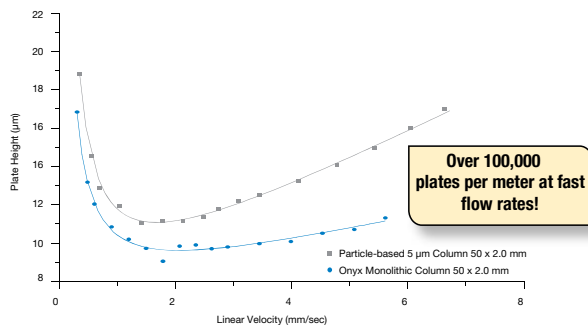

Conditions same for both separations:

- Columns:** Particle-based 5 μ m Column 50 x 2.0 mm ID
Onyx Monolithic Column 50 x 2.0 mm ID
- Mobile Phase:** Acetonitrile/Water (65:35)
- Flow Rate:** As noted
- Detection:** UV @ 254 nm
- Temperature:** 30 °C
- Samples:** 1. Uracil
2. Acetophenone
3. Benzene
4. Toluene
5. Naphthalene

Over 100,000 plates per meter at fast flow rates!

If Onyx analytical columns do not provide at least an equivalent separation as compared to a competing column of the same monolithic characteristics, similar phase, and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

10 mm ID Onyx Semi-Prep Column

- Flow rates from 5 – 35 mL/min
- Loading capacities approaching what is typically observed on 21.2mm ID columns for some samples
- Pore structure rapidly disrupts DMSO injection slug resulting in better mixing & improved binding of analyte to sorbent
- Long lifetimes when analyzing “dirty” samples due to monolithic nature

Excellent Reproducibility

Several parameters, such as peak asymmetry and retention factors, were used to test the reproducibility of Onyx silica monolithic columns and ensure that every batch meets the quality control standards of chromatographers worldwide.



Refer to technical note, [TN-1025](#), for more information pertaining to Onyx reproducibility. Call your Phenomenex representative.

Ordering Information

Part No.	Description	Size (mm)
Capillary Columns		
CHO-7646	Onyx Monolithic C18	150 x 0.1
Analytical Columns		
CHO-8373	Onyx Monolithic C18	50 x 2.0
CHO-8464	Onyx Monolithic C18	25 x 3.0
CHO-8158	Onyx Monolithic C18	100 x 3.0
CHO-7643	Onyx Monolithic C18	100 x 4.6
CHO-7644	Onyx Monolithic C18	50 x 4.6
CHO-7645	Onyx Monolithic C18	25 x 4.6
CHO-8611	Onyx Monolithic HD-C18	100 x 4.6
CHO-7647	Onyx Monolithic C8	100 x 4.6
SemiPrep Columns		
CHO-7878	Onyx Monolithic C18	100 x 10.0
Guard Cartridge System		
KJO-8465	Onyx Monolithic C18 Guard Cartridge Kit (3/pk cartridges + holder)	5 x 3.0
CHO-8466	Onyx Monolithic C18 Guard Cartridges (3/pk)	5 x 3.0
CHO-7649	Onyx Monolithic C18 Guard Cartridges (3/pk)	5 x 4.6
KJO-7652	Onyx Monolithic C18 Guard Cartridge Kit (3/pk cartridges + holder + wrench)	10 x 4.6
CHO-7650	Onyx Monolithic C18 Guard Cartridges (3/pk)	10 x 4.6
Column Coupler		
AQQ-7654	Onyx Column Coupler, 0.020 in. ID	



For Onyx Reversed Phase Column
Check Standard, see p. 414



Product based on monolithic technology under
license from Merck KGaA, Darmstadt, Germany

If Phenogel analytical GPC columns do not provide at least an equivalent separation as compared to a competing GPC column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Organic Size Exclusion/Gel Permeation for Polymer Analysis

- 5 and 10 µm particle sizes
- Narrow bore (4.6 mm ID) solvent-saver to preparative columns available
- Alternative to Agilent® (Polymer Labs) PLgel™, Waters® Styragel® and Ultrastaygel™, and other columns (see p. 313)
- Highly cross-linked for mechanical and chemical stability
- Temperature stable to 140°C

Phenogel is available in seven different pore sizes, ranging from 50 Å to 10⁶ Å†, and a linear bed configuration. Pore size distribution and pore volume are closely controlled parameters in the manufacturing process accounting for the high resolution, tight linear calibration curves, and excellent column-to-column reproducibility.


Sample Elution

Each standard dimension Phenogel column (300 x 7.8 mm) has an internal volume of 15 mL that is distributed as follows:

- 3 mL is occupied by the solid portions of the gel particles (20% of total column volume)
- 6 mL is the pore volume of the packing material (40% of total column volume)
- 6 mL is the interstitial volume or volume between the gel particles (40% of total column volume)

Thus, about 6 mL of solvent must elute through each column before even the largest molecules can emerge, while the smallest molecules emerge with the total column volume of 12 mL. This constant distribution of volume makes it possible to predict the amount of solvent and time necessary to complete any analysis.

SEM Photos of Phenogel Polymer Beads

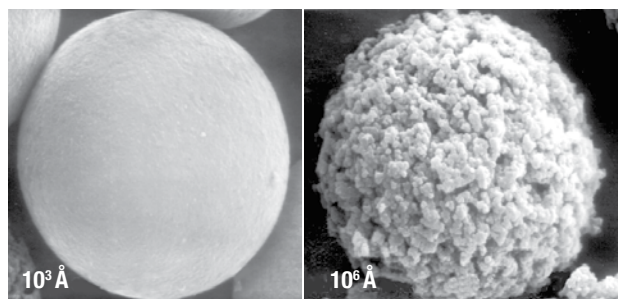

Technical Specifications

Material:	SDVB
Particle Size:	5, 10 µm
Porosities:	50 Å to 10 ⁶ Å†, and mixed beds
Maximum Pressure:	1500 psi
Maximum Temperature:	140 °C
Minimum Efficiency*:	5 µm: 45,000 p/m** 10 µm: 35,000 p/m**
Typical Flow Rates:	4.6 mm ID: 0.35 mL/min 7.8 mm ID: 1.0 mL/min 21.2 mm ID: 7.0 mL/min


* Tested in THF ** For 300 x 7.8 mm ID columns

† See note on p. 434 regarding pore sizes and exclusion limits

Column Selection by Molecular Weight

Sample Type	Molecular Weight	Phenogel Column
Small Organics	100 - 3 K	50 Å
	500 - 6 K	100 Å
	1 K - 15 K	500 Å
Resins	1 K - 75 K	10 ³ Å
	5K - 500 K	10 ⁴ Å
	10 K - 1,000 K	10 ⁵ Å
High MW Polymers	60 K - 10,000 K	10 ⁶ Å
	100 - 10,000 K	Linear(2)

Column Molecular Weight Calibration Curves

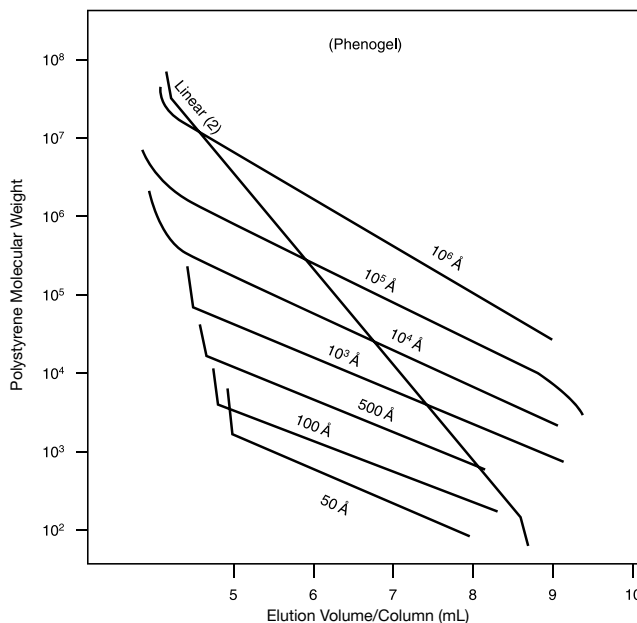

Solvent and Temperature Compatibility

- Phenogel columns are packed in tetrahydrofuran (THF)
- Columns can also be shipped in solvents such as DMF and chloroform to help minimize equilibration time

Solvent Compatibility Table

Mobile Phase Solvent	Phenogel Pore Size:							Linear & Mixed	Suggested Operating Temp.
	50 (Å)	100	500	10 ³	10 ⁴	10 ⁵	10 ⁶		
Acetone	Y	Y	Y	Y	Y	Y	Y	Y	
Benzene	Y	Y	Y	Y	Y	Y	Y	Y	
Carbon Tetrachloride	Y	Y	Y	Y	Y	Y	Y	Y	
Chloroform	Y	Y	Y	Y	Y	Y	Y	Y	
30% HFIP/Chloroform	Y	Y	Y	Y	Y	Y	Y	Y	
Diethyl Ether	Y	Y	Y	Y	Y	Y	Y	Y	
Dimethylacetamide (DMAC)	Y*	Y	Y	Y	Y	Y	Y	Y	60 °C
Dimethylformamide (DMF)	Y*	Y	Y	Y	Y	Y	Y	Y	60 °C
Dioxane	Y	Y	Y	Y	Y	Y	Y	Y	
DMSO	Y*	Y	Y	Y	Y	Y	Y	Y	60 °C
Ethyl Acetate	Y	Y	Y	Y	Y	Y	Y	Y	
Hexafluoroisopropanol (HFIP)	Y	Y	Y	Y	Y	Y	Y	Y	
Hexane	Y	Y	Y	Y	Y	Y	Y	Y	
M-Cresol	Y*	Y	Y	Y	Y	Y	Y	Y	100 °C
Methyl Ethyl Ketone	Y	Y	Y	Y	Y	Y	Y	Y	
Methylene Chloride	Y	Y	Y	Y	Y	Y	Y	Y	
O-Chlorophenol	Y*	Y	Y	Y	Y	Y	Y	Y	100 °C
O-Dichlorobenzene	Y*	Y	Y	Y	Y	Y	Y	Y	135 °C
Quinolin	Y*	Y	Y	Y	Y	Y	Y	Y	60 °C
Tetrahydrofuran	Y	Y	Y	Y	Y	Y	Y	Y	
Toluene	Y	Y	Y	Y	Y	Y	Y	Y	
Trichlorobenzene	Y*	Y	Y	Y	Y	Y	Y	Y	135 °C
Water	N	N	N	N	N	N	N	N	
Xylene	Y	Y	Y	Y	Y	Y	Y	Y	

*Not recommended on 5 μm 50 Å columns.

N = Not Compatible
Y = Compatible




Solvent Switching Considerations

Although Phenogel columns are rugged and can withstand strong solvent changes, care should be exercised when switching from high-swell solvents (A) to low-swell solvents (B, C, and D). Improper solvent switches can result in a void. Best results are attained when an intermediate-swell solvent is used and column lifetime is improved. Contact Phenomenex regarding solvents not listed below.

Column life can be maximized by dedicating certain columns to certain solvents. This will also minimize solvent switches. If care is not taken, a void may occur.

- Reduce flow rate to 0.2 mL/min
- Backpressure must NEVER exceed 1500 psi
- Always check solvent miscibility in a beaker or follow the solvent miscibility table on page 432 before proceeding with ANY solvent switch.
- Compare the swell characteristics of solvent 1 (old solvent) to solvent 2 (new solvent) and use the following guidelines:
 - If solvent 1 and solvent 2 belong to the same swell category (see table below), check the solvent miscibility and proceed with the switch.
 - If solvent 1 and solvent 2 belong to successive swell categories as indicated by the arrows in the table below, check the miscibility and proceed with the switch.
 - If solvent 1 and solvent 2 DO NOT belong to the same OR successive swell categories, switch to an intermediate solvent FIRST, as indicated by the arrows in the table.

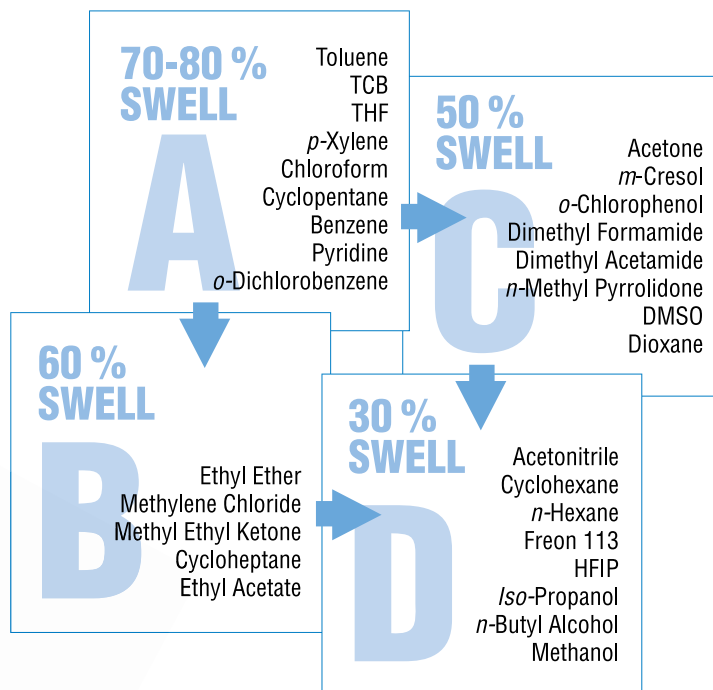


Pharmaceutical Excipients Analysis

Gel permeation chromatography using Phenogel columns is an excellent method for measuring the molecular weight distribution and lot-to-lot consistency of fillers and dispersants.


Polyethylene Glycol 330

Column: Phenogel 5 μ m 50 Å, 100 Å, 500 Å
Dimensions: 300 x 7.8 mm
Guard Cartridge: [AJ0-9292](#)
Guard Holder: [KJ0-4282](#)
Solvent: THF
Flow Rate: 1.0 mL/min
Detection: Differential Refractometer
Injection Volume: 100 μ L 0.25% w/v
Temperature: Ambient
Vial: [AR0-9925-13](#)
Filter: [AF0-1102-52](#)
Sample: 1. dp7 546 MW 5. dp3 194 MW
 2. dp6 458 MW 6. dp2 106 MW
 3. dp5 370 MW 7. dp1 62 MW
 4. dp4 282 MW

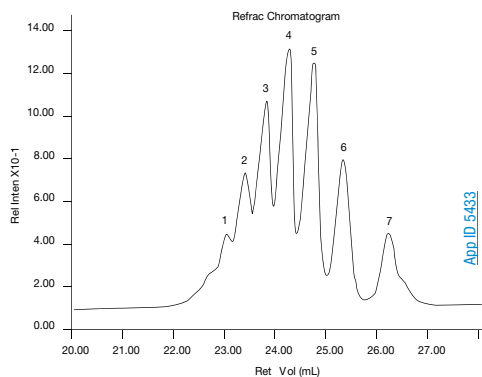


Polyethylene Glycol 106

Column: Phenogel 5 μ m 50 Å, 100 Å, 500 Å
Dimensions: 300 x 7.8 mm
Guard Cartridge: [AJ0-9292](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: THF
Flow Rate: 1 mL/min
Detection: Refractive Index (RI)
Temperature: 40 °C
Vial: [AR0-9925-13](#)
Filter: [AF0-1102-52](#)
Sample: 1. PEG 106
 2. API peak A (unknown)
 3. API peak B (unknown)

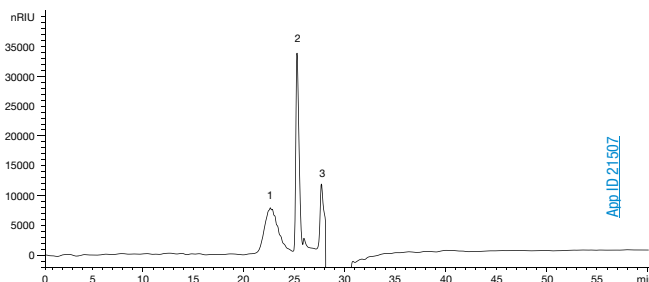

Polyvinylpyrrolidone

Column: Phenogel 5 μ m Linear(2) x2
Dimensions: 300 x 7.8 mm
Part No: [00H-3259-K0](#)
Guard Cartridge: [AJ0-9292](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 10 mM Lithium bromide in DMF
Flow Rate: 2 mL/min
Detection: Refractive Index (RI)
Column Temp: 40 °C
Vial: [AR0-9925-13](#)
Filter: [AF0-1102-52](#)
Sample: 1. Polyvinylpyrrolidone (PVP)

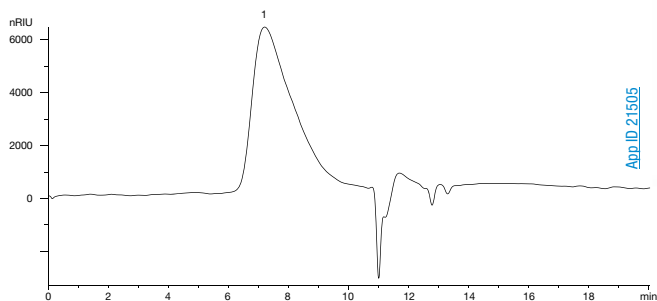


Phenogel™ Organic GPC/SEC Columns

50-106 Å Columns

- High resolution at low cost
- Customize your analysis by coupling different pore-size columns
- Wide range of solvent compatibility

Polymethyl Methacrylates (Wide MW Range)


Column: Phenogel 5 µm 10⁵ Å, 10⁴ Å, 10³ Å, 500 Å
Dimensions: 300 x 7.8 mm
Solvent: THF
Flow Rate: 1.0 mL/min
Detection: Differential Refractometer
Injection Volume: 100 µL 0.25% w/v
Sample:
 1. 700,000 MW
 2. 107,000 MW
 3. 27,000 MW

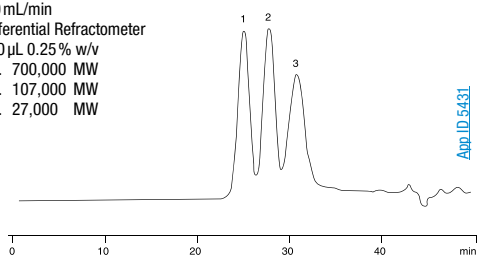

App ID: 5431

Closely Related Hydrocarbons


Column: Phenogel 5 µm 50 Å, 100 Å, 500 Å
Dimensions: 300 x 7.8 mm
Solvent: THF
Flow Rate: 1.0 mL/min
Detection: Differential Refractometer
Injection Volume: 100 µL 0.25% w/v
Temperature: Ambient
Sample:
 1. C40 562 MW 4. C20 282 MW
 2. C32 450 MW 5. C16 226 MW
 3. C24 338 MW 6. C13 184 MW

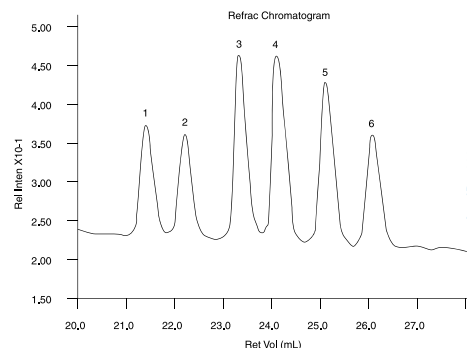

App ID: 5432

Polyethylene Oxide (PEO)


Column: Phenogel 10 µm 10⁵, 10⁴, 10³ Å
Dimensions: 300 x 7.8 mm
Mobile Phase: DMF (0.1 M LiBr)
Flow Rate: 1.0 mL/min
Detection: Differential Refractometer
Injection Volume: 100 µL 0.125% w/v
Temperature: 50 °C
Sample: 400,000 MW

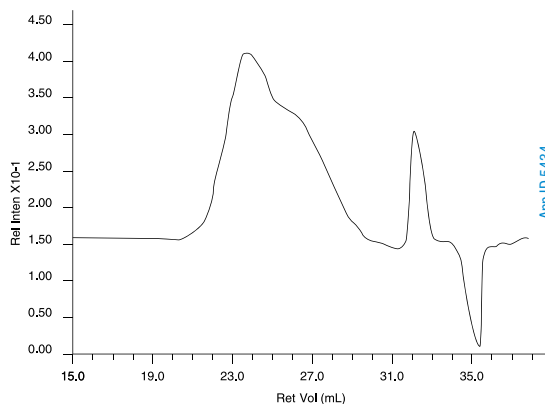

App ID: 5434

Polystyrenes (Wide MW Range)


Column: Phenogel 10 µm 10⁵, 10⁴, 10³ Å
Dimensions: 300 x 7.8 mm
Mobile Phase: THF
Flow Rate: 1.0 mL/min
Detection: Differential Refractometer
Injection Volume: 100 µL 0.125% w/v
Temperature: Ambient
Sample:
 1. 1,560,000 MW 5. 6,100 MW
 2. 260,000 MW 6. 845 MW
 3. 94,000 MW 7. 146 MW
 4. 30,000 MW

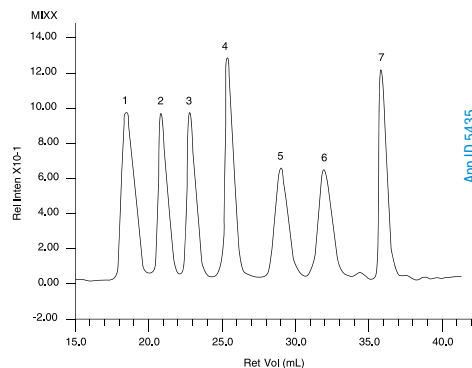

App ID: 5435

Poly-(α-Methyl Styrene) (Wide MW Range)


Column: Phenogel 5 µm 10⁵, 10⁴, 10³, 500 Å
Dimensions: 300 x 7.8 mm
Solvent: THF
Flow Rate: 1.0 mL/min
Detection: Differential Refractometer
Injection Volume: 100 µL 0.25% w/v
Sample:
 1. 680,000 MW
 2. 90,000 MW
 3. 30,000 MW
 4. 6,000 MW

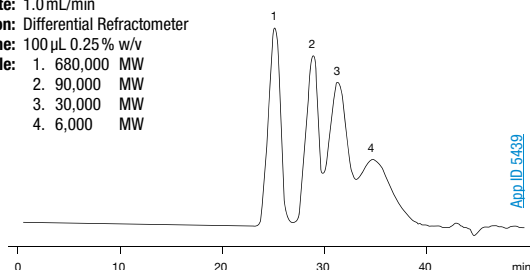

App ID: 5439

Polybutadienes (Wide MW Range)

Column: Phenogel 5 µm 10⁵, 10⁴, 10³, 500 Å
Dimensions: 300 x 7.8 mm
Solvent: THF
Flow Rate: 1.0 mL/min
Detection: Differential Refractometer
Injection Volume: 100 µL 0.25% w/v
Sample:
 1. 420,000 MW
 2. 24,000 MW
 3. 2,500 MW
 4. 500 MW

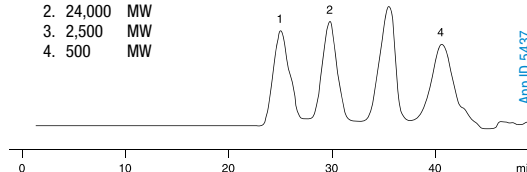


App ID: 5437

Linear Columns


- Linear calibration to 10 million daltons
- Long column lifetime
- Excellent mechanical stability
- Excellent for analyzing a wide range of molecular weights

Mixed Polystyrene Standard

Column: Phenogel 5 µm Linear(2)
Dimensions: 300 x 7.8 mm
Part No.: [00H-3259-K0](#)
Guard Cartridge: [AJ0-9292](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: THF
Flow Rate: 1.0 mL/min
Detection: RI
Injection Volume: 50 µL
Temperature: 35 °C
Vial: [ARO-9925-13](#)
Filter: [AF0-1102-52](#)
Sample: Polystyrene standards injected
 1. 2,860,000 MW
 2. 277,000 MW
 3. 9,350 MW

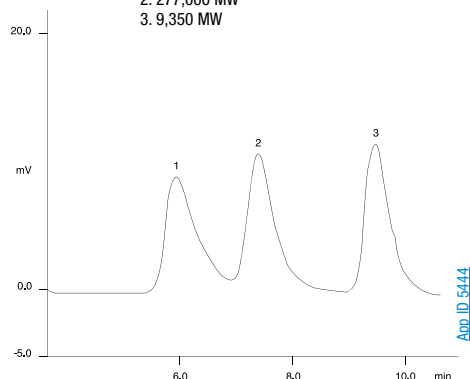

Calibration Curve: Linear (2) - Phenogel 5 µm 300 x 7.8 mm

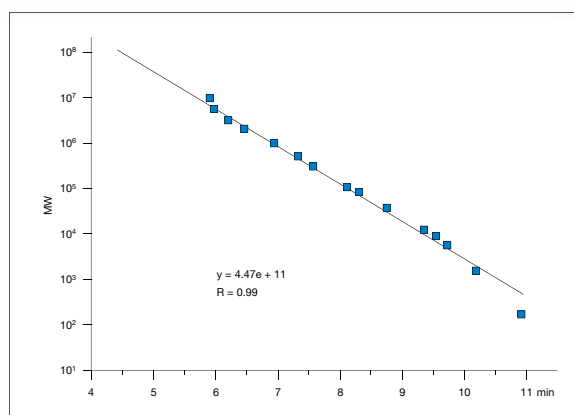

Narrow Bore Columns

An Improved Dimension in GPC Analysis


- Decrease solvent consumption
- Retain same elution profile
- Reduce solvent disposal costs

Phenogel-NB (Narrow Bore) columns are optimized to reduce solvent consumption. The Phenogel-NB columns have a 4.6 mm column ID and run at 0.35 mL/min, reducing solvent consumption and disposal costs up to 65 %!

Loading

With narrow bore GPC/SEC columns, the volume in which the sample elutes is significantly decreased, thus increasing the effective concentration of the sample. In GPC, this leads to overloading effects and proportionally lower sample loadings must be used.

Cut Waste!

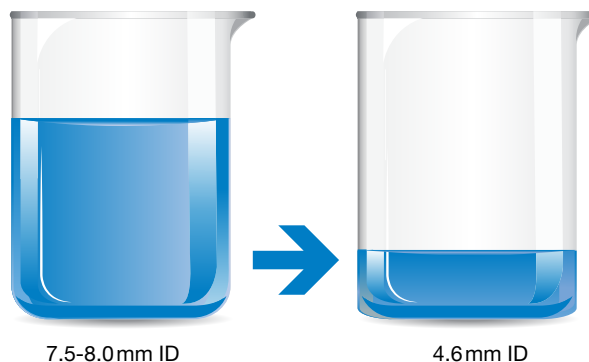

DISCOVER HOW MUCH YOU WILL SAVE when switching to Phenogel Narrow Bore columns!

Try our NEW solvent savings calculator web tool at

www.phenomenex.com/GPCSavings

Phenogel™ Organic GPC/SEC Columns

guarantee

If Phenogel analytical GPC columns do not provide at least an equivalent separation as compared to a competing GPC column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information

5 µm Analytical Columns (mm)		Shipping Solvent			SecurityGuard™ Cartridges (mm)
		THF	Chloroform	DMF	
		300 x 7.8	300 x 7.8	300 x 7.8	4 x 3.0*
Pore Size	MW Range				/3pk
50 Å	100-3 K	00H-0441-KO	00H-0441-KO-CL	00H-0441-KO-DF	AJ0-9292
100 Å	500-6 K	00H-0442-KO	00H-0442-KO-CL	00H-0442-KO-DF	AJ0-9292
500 Å	1 K-15 K	00H-0443-KO	00H-0443-KO-CL	00H-0443-KO-DF	AJ0-9292
10³ Å	1 K-75 K	00H-0444-KO	00H-0444-KO-CL	00H-0444-KO-DF	AJ0-9292
10⁴ Å	5 K-500 K	00H-0445-KO	00H-0445-KO-CL	00H-0445-KO-DF	AJ0-9292
10⁵ Å	10 K-1,000 K	00H-0446-KO	00H-0446-KO-CL	00H-0446-KO-DF	AJ0-9292
10⁶ Å	60 K-10,000 K	00H-0447-KO	00H-0447-KO-CL	00H-0447-KO-DF	AJ0-9292
		300 x 7.8	300 x 7.8	300 x 7.8	4 x 3.0*
Mixed Beds					/3pk
Linear(2)	100-10,000 K	00H-3259-KO	00H-3259-KO-CL	00H-3259-KO-DF	AJ0-9292

for 3.2–8.0 mm ID

5 µm Narrow Bore (NB) Columns (mm)		SecurityGuard™ Cartridges (mm)	
		300 x 4.6	4 x 3.0*
Pore Size	MW Range		/3pk
50 Å	100-3 K	00H-0441-E0	AJ0-9292
100 Å	500-6 K	00H-0442-E0	AJ0-9292
500 Å	1 K-15 K	00H-0443-E0	AJ0-9292
10³ Å	1 K-75 K	00H-0444-E0	AJ0-9292
10⁴ Å	5 K-500 K	00H-0445-E0	AJ0-9292
10⁵ Å	10 K-1,000 K	00H-0446-E0	AJ0-9292
10⁶ Å	60 K-10,000 K	00H-0447-E0	AJ0-9292
		300 x 4.6	4 x 3.0*
Mixed Beds		/3pk	
Linear(2)	100-10,000 K	00H-3259-E0	AJ0-9292

for 3.2–8.0 mm ID

10 µm Analytical Columns (mm)		SecurityGuard™ Cartridges (mm)	
		300 x 7.8	4 x 3.0*
Pore Size	MW Range		/3pk
50 Å	100-3 K	00H-0641-KO	AJ0-9292
100 Å	500-6 K	00H-0642-KO	AJ0-9292
500 Å	1 K-15 K	00H-0643-KO	AJ0-9292
10³ Å	1 K-75 K	00H-0644-KO	AJ0-9292
10⁴ Å	5 K-500 K	00H-0645-KO	AJ0-9292
10⁵ Å	10 K-1,000 K	00H-0646-KO	AJ0-9292
10⁶ Å	60 K-10,000 K	00H-0647-KO	AJ0-9292
		300 x 7.8	4 x 3.0*
Mixed Beds		/3pk	
Linear(2)	100-10,000 K	00H-3260-KO	AJ0-9292

for 3.2–8.0 mm ID

5 µm Preparative Columns (mm)		Guards	
		300 x 21.2	50 x 21.2
Pore Size	MW Range		
100 Å	500-6 K	00H-0442-P0	03B-0642-P0

10 µm Preparative Columns (mm)		Guards	
		300 x 21.2	50 x 21.2
Pore Size	MW Range		
100 Å	500-6 K	00H-0642-P0	03B-0642-P0

Guard Cartridge Holder

Part No.	Description
KJ0-4282	Reusable Holder (SecurityGuard Kit)

Column Union

Part No.	Description	Unit
AQ0-8507	Zero Dead Union, SS, with 10-32 fittings	ea

Note: Additional union ([AQ0-8507](#)) may be necessary for SecurityGuard to fit in column oven with less than 30 cm length capacity.



Phenogel columns are routinely shipped in THF. However, columns are also available in commonly used solvents, Chloroform and DMF, for an additional charge for these shipping solvents. Please specify shipping solvent when ordering.

Phenogel Columns are a Recommended Alternative to:

Manufacturer	Columns
Agilent® (Polymer Labs)	PLgel™
Jordi Labs	Jordi Gel™ DVB Jordi Gel DVB Fluorinated Jordi Gel DVB Glucose
Polymer Standards Service (PSS)	SDV® GRAM PolarSil PFG POLEFIN®
Shodex®	GPC K-800 Series GPC KF-800 Series GPC KD-800 Series
Tosoh Bioscience®	TSKgel® SuperMultiporeHZ TSKgel SuperHZ TSKgel Hxl TSKgel SuperH TSKgel Hhr
Waters®	Styragel® Ultrastrygel™ ACQUITY® APC™

*SecurityGuard Analytical Cartridges require holder, Part No.: [KJ0-4282](#)



For Column Heater, see p. 408



SecurityGuard cartridges for Non-Aqueous Polymer GPC columns are not compatible with HFIP solvent.



PhenoSphere™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/phenosphere

PhenoSphere™ - *NEXT*™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/phenospherenext

PLgel™ and PLRP-S

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/plgel and www.phenomenex.com/plrps

If PolymerX analytical columns do not provide at least equivalent separation as compared to your PSDVB column of similar particle size and dimension, return the column with comparative data within 45 days for a FULL REFUND.

Reversed Phase Polymer HPLC Columns

- Excellent alternative to other polystyrene divinylbenzene (PSDVB) columns
- High chemical strength and stability
- pH stable from 0-14
- No bonded phase = zero phase bleed
- Great long-lived solution for separating quaternary amines

PolymerX RP-1 is a porous (100 Å) polystyrene divinylbenzene media which has hydrophobic retention similar to a C18-bonded silica. Because the media is a polymer instead of silica, it is tolerant to pH extremes (0-14) and a good solution for high pH applications where silica-based media fail. PolymerX also delivers good lifetime for analytes like quaternary amines which strongly interact with bonded silica particles.

Material Characteristics


Packing Material	Particle Shape/Size (µm)	Pore Size (Å)	pH Stability
RP-1 (PSDVB)	Spherical 3, 5, 7, 10	100	0 - 14

Typical Results and Operating Parameters of RP Silica and Polymer Columns

Parameter	C18 silica	RP-polymer
Acidic silanols	present	absent
pH stability	2-9	0-14
Recovery*	~50-80 %	>95 %
Capacity*	1 mg	10-25 mg
Pressure limit	3500 psi	2500 psi
Temperature limit	60 °C	80 °C
Column lifetime		longer

*pertains to dimethyltritylated (DMT) synthetic oligomer purification on a 150 x 4.1 mm column

Chromatographic Comparison** of Polymer Columns

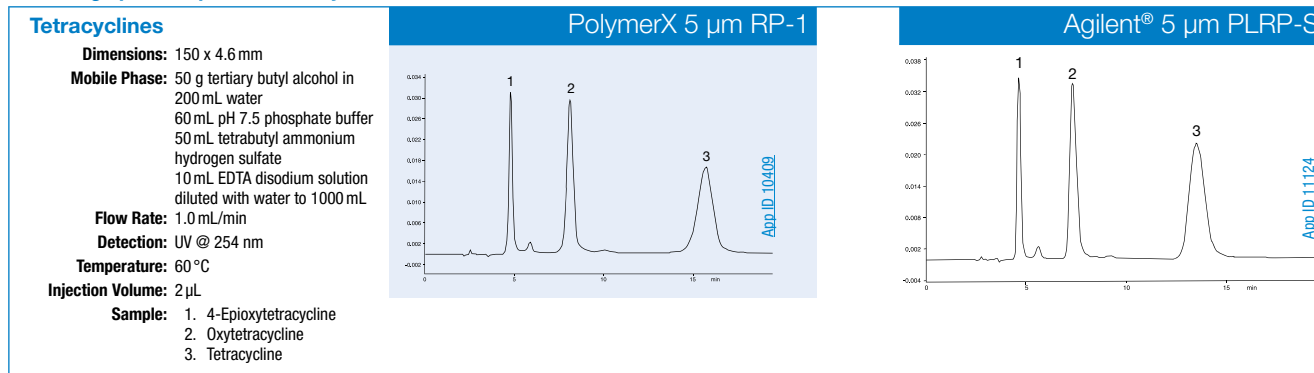

**Comparative separations may not be representative of all applications.

Erythromycins

Column: PolymerX 7 µm RP-1

Dimensions: 250 x 4.6 mm

Part No.: [00G-4327-E0](#)

Guard Cartridge: [AJ0-5809](#)

Guard Holder: [KJ0-4282](#)

Mobile Phase: A: 1.75 g dibasic potassium phosphate in 50 mL water, adjust to pH 9.0. Add 165 mL of tertiary butyl alcohol and 30 mL acetonitrile. Add water to a final volume of 1 L
B: Acetonitrile A/B (50:50)

Flow Rate: 0.8 mL/min

Detection: UV @ 215 nm


Temperature: 75 °C

Injection Volume: 20 µL

Vial: [ARO-9925-13](#)

Filter: [AF0-8103-52](#)

Sample: 1. Unknown
2. Erythromycin related compound N
3. Erythromycin C
4. Erythromycin A
5. Erythromycin B

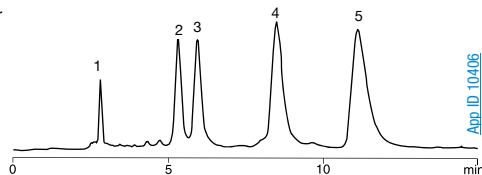

polymerX™

HPLC/UHPLC | POLYMERX

Ordering Information

	PolymerX RP-1 Columns (mm)							
	50 x 4.0	150 x 2.0	150 x 4.1	150 x 4.6	250 x 4.1	250 x 4.6	250 x 10.0	250 x 21.2
3 µm	00B-4338-D0	—	00F-4338-Z0	—	—	—	—	—
5 µm	—	00F-4326-B0	00F-4326-Z0	00F-4326-E0	00G-4326-Z0	00G-4326-E0	—	—
7 µm	—	—	—	—	—	00G-4327-E0	—	—
10 µm	—	—	—	—	00G-4328-Z0	00G-4328-E0	00G-4328-N0	00G-4328-P0

RP-1 SecurityGuard™ Cartridges (mm)		
4 x 3.0*	10 x 10 [‡]	15 x 21.2**
/10pk	/3pk	/ea
AJ0-5809	AJ0-7368	AJ0-8358
for ID: 3.2-8.0 mm	9-16 mm	18-29 mm



Bulk media available upon request.



For PolymerX Column Performance Check Standards, see p. 414

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)

†SemiPrep SecurityGuard Cartridges require holder, Part No.: [AJ0-7220](#)

**Prep SecurityGuard Cartridges require holder, Part No.: [AJ0-8223](#)


Aqueous GFC Columns for the Separation of Polymers, Proteins and Peptides

- Highly hydrophilic synthetic polymer phase
- Suitable for water-soluble polymers
- Very low nonspecific interaction with the separation matrix
- Extremely cost-effective
- High efficiencies
- Good mechanical strength

The PolySep material undergoes rigorous quality control tests, from the initial stages of testing of the starting monomers to the final product. There are at least 25 steps of quality assurance during the entire procedure. The packed column then undergoes at least five additional tests, including a batch test for the manufactured materials. Each column is then tested for column efficiency and peak symmetry and ships with a QC chromatogram. This ensures long-lasting columns with very high efficiencies.

Dextran

Column: PolySep-GFC-P4000
 Dimensions: 300 x 7.8 mm
 Part No.: 00H-3144-K0
 Mobile Phase: Water
 Flow Rate: 0.8 mL/min
 Detection: RI
 Sample: 20 µL injected

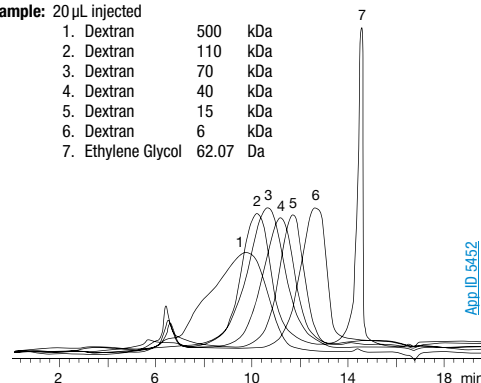

PolySep-GFC-P Technical Data and Specifications

Phase:	1000	2000	3000	4000	5000	6000	Linear
Exclusion Limits in Daltons:							
PEG	2 x 10 ⁵	9 x 10 ⁵	5 x 10 ⁴	2 x 10 ⁵	2 x 10 ⁶	1 x 10 ⁷	1 x 10 ⁷
Pullulans	3.5 x 10 ⁵	1 x 10 ⁴	1 x 10 ⁵	3.5 x 10 ⁵	4 x 10 ⁶	2 x 10 ⁷	2 x 10 ⁷
Separation Range (Da)	20 - 3K	100 - 10K	250 - 75K	3K - 400K	50K - 2M	100K - 15M	1K - 10M
Typical Efficiency Plates/meter	22,000	50,000	32,000	32,000	32,000	32,000	32,000
Maximum Organic Modifier:							
Methanol	20%	95%	70%	70%	70%	70%	70%
Acetonitrile	20%	70%	70%	70%	70%	70%	70%
pH Range	3.0 to 12.0						
Maximum Flow Rate	Depends on backpressure, do not exceed 1000 psi						
Column Hardware	Stainless steel or PEEK (Biocompatible hardware available upon request)						
Temperature	4 to 60 °C						
Maximum Salt	Maximum allowed 0.5 M with a flow rate not to exceed 0.5 mL/min						
Storage	For overnight, pump water at 0.2 mL/min, for longer storage use 0.05% NaNO ₃ in water or 10% methanol in water						
General	A guard column is recommended to improve column life						

Ordering Information

PolySep-GFC-P Columns (mm)		
	Analytical	Guards
Phases	300 x 7.8	35 x 7.8
1000	CHO-9226	CHO-9225
2000	CHO-9227	CHO-9225
3000	CHO-9228	CHO-9225
4000	CHO-9229	CHO-9225
5000	CHO-9230	CHO-9225
6000	CHO-9231	CHO-9225
Linear	CHO-9232	CHO-9225

Aqueous SEC 2 Column Check Standard

(For PolySep GFC-P and other aqueous-soluble analysis columns)

Part No.: AL0-3043

Unit quantity: 2 mL
 Contains: Ethylene Glycol
 Diluent: Water

Test Conditions

Mobile Phase: Water
 Flow Rate: 0.8 mL/min
 Injection Volume: 15 µL
 Detection: RI



For additional GFC Columns, see p. 350



For HPLC Column Heater (25-90 °C), see p. 408

If Prodigy analytical columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Guaranteed Alternative to Inertsil®

- Highly reproducible
- Long column life
- Mimics performance of GL Sciences, Inc. Inertsil®

Ordering Information

3 µm ODS-3 Columns (mm)							SecurityGuard™ Cartridges (mm)	
Phases	100 x 2.0	150 x 2.0	100 x 4.0	30 x 4.6	100 x 4.6	150 x 4.6	4 x 2.0*	4 x 3.0*
ODS-3 100 Å	00D-4222-B0	00F-4222-B0	00D-4222-D0	00A-4222-E0	00D-4222-E0	00F-4222-E0	/10pk AJ0-4286	/10pk AJ0-4287

for ID: 2.0-3.0 mm 3.2-8.0 mm

3 µm and 5 µm ODS-3V Columns (mm)		
Phases	Part No.	Size (mm)
3 µm ODS-3V	00D-4243-E0	100 x 4.6
3 µm ODS-3V	00F-4243-E0	150 x 4.6
5 µm ODS-3V	00F-4241-E0	150 x 4.6
5 µm ODS-3V	00G-4241-E0	250 x 4.6

5 µm Minibore Columns (mm)				SecurityGuard™ Cartridges (mm)	
Phases	50 x 2.0	150 x 2.0	250 x 2.0	4 x 2.0*	
C8 150 Å	00B-3301-B0	00F-3301-B0	—	/10pk AJ0-4289	
ODS-2 150 Å	—	00F-3300-B0	—	AJ0-4286	
ODS-3 100 Å	00B-4097-B0	00F-4097-B0	00G-4097-B0	AJ0-4286	

for ID: 2.0-3.0 mm

5 µm MidBore™ Columns (mm)					SecurityGuard™ Cartridges (mm)	
Phases	150 x 3.0	250 x 3.0	150 x 3.2	250 x 3.2	4 x 2.0*	4 x 3.0*
C8 150 Å	00F-3301-Y0	00G-3301-Y0	—	—	/10pk AJ0-4289	AJ0-4290
ODS-2 150 Å	—	00G-3300-Y0	00F-3300-R0	00G-3300-R0	AJ0-4286	AJ0-4287
ODS-3 100 Å	00F-4097-Y0	00G-4097-Y0	00F-4097-R0	00G-4097-R0	AJ0-4286	AJ0-4287

for ID: 2.0-3.0 mm 3.2-8.0 mm

5 µm and 10 µm Analytical Columns (mm)						SecurityGuard™ Cartridges (mm)	
Phases	30 x 4.6	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0*	/10pk
5 µm C8 150 Å	00A-3301-E0	00B-3301-E0	00D-3301-E0	00F-3301-E0	00G-3301-E0	AJ0-4290	AJ0-4287
5 µm ODS-2 150 Å	00A-3300-E0	00B-3300-E0	00D-3300-E0	00F-3300-E0	00G-3300-E0	AJ0-4287	AJ0-4287
5 µm Silica 100 Å	—	—	—	—	00G-4098-E0	AJ0-4348	AJ0-4287
5 µm ODS-3 100 Å	00A-4097-E0	00B-4097-E0	00D-4097-E0	00F-4097-E0	00G-4097-E0	AJ0-4287	AJ0-4287
5 µm Phenyl-3 (PH-3) 100 Å	—	—	—	00F-4298-E0	00G-4298-E0	AJ0-4351	AJ0-4287
10 µm Silica-3 100 Å	—	—	—	—	00G-4245-E0	AJ0-4348	AJ0-4287
10 µm ODS-3 100 Å	—	—	—	—	00G-4244-E0	AJ0-4287	AJ0-4287

for ID: 3.2-8.0 mm

5 µm and 10 µm SemiPreparative Columns (mm)		SecurityGuard™ Cartridges (mm)	
Phases	250 x 10	10 x 10 ²	
5 µm ODS-3 100 Å	00G-4097-N0	/3pk AJ0-7221	
10 µm ODS-3 100 Å	00G-4244-N0	AJ0-7221	

for ID: 9-16 mm

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)
 †SemiPrep SecurityGuard™ Cartridges require holder, Part No.: [AJ0-7220](#)

For SecurityGuard Cartridge Holders and Cartridges, see p. 326

If Rezex columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, phase and dimensions, return the column with the comparative data within 45 days for a FULL REFUND.

Carbohydrate and Organic Acid Analysis

- Excellent resolution and column-to-column reproducibility
- Easy, accurate quantitation from sharper peak shapes
- Longer column lifetimes and faster run time capability from lower backpressures
- Baseline separation of critical sample components due to higher efficiencies

Rezex HPLC columns achieve reproducible, accurate separations based on multiple modes of interaction. Available in 4% and 8% cross-linked sulfonated styrene-divinylbenzene (SDVB) and multiple ionic forms (calcium, sodium, hydrogen, potassium, lead, and silver) for a wide range of selectivities. USP L17, L19, L22, L34, and L58 packings available.

REZEX™
Carbohydrate and Organic Acid LC

Use Rezex for carbohydrate, oligosaccharide, and organic acid separations:

- Drug formulation and excipient analysis
- Food and beverage quality control testing
- Fermentation reaction monitoring and recovery testing for biofuels



Recommended alternative to Bio-Rad® Aminex®, Supelco® SUPELCOGEL™, and Waters® Sugar-Pak™ (see p. 323)






Bioethanol Fermentation Monitoring

- Easy quantitation of ethanol fermentation broth components
- Monitor starches, sugars, organic acids, and ethanol in one run
- Reliable lactic acid and acetic acid monitoring
- Increase throughput by reducing run times 50% with 150 mm column length


Monitoring the key reaction components throughout the fermentation process is crucial for maximizing ethanol recovery. Rezex ROA is uniquely suited for the separation and analysis of simple and complex sugars, organic acids, and ethanol within a fermentation broth sample. With results easily obtained through an isocratic run, Rezex ROA is instrumental in helping you to accurately determine what critical steps need to be taken to ensure the maximum yield is achieved during your fermentation run.

Rezex ROA has the ability to achieve excellent baseline separation between Dp3 and Dp4+, which have proven to be a challenge within the bioethanol industry. It is this great baseline separation that affords scientists the opportunity to utilize a shorter column dimension. By using the 150 x 7.8 mm Rezex ROA column, you are able to decrease the run time by 50% when compared to the average run time on a 300 x 7.8 mm column.

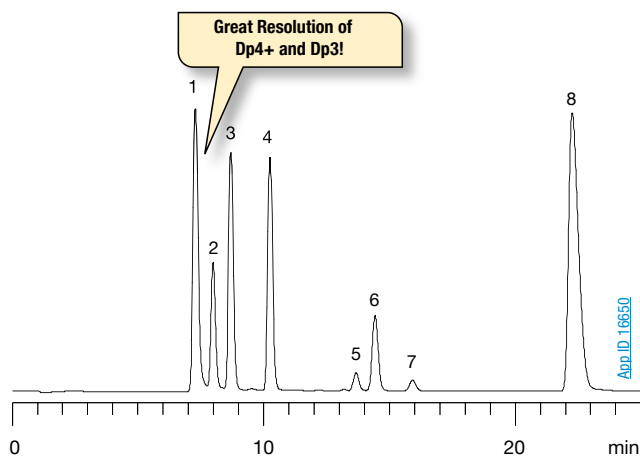

Column: Rezex ROA-Organic Acid
Dimensions: 300 x 7.8 mm
Part No.: [00H-0138-K0](#)
Guard Cartridge: [AJ0-4490](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 0.005 N Sulfuric Acid
Flow Rate: 0.6 mL/min
Detection: RI @ 40 °C
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 60 °C
System: Shimadzu® Prominence® LC-20A System
Sample:

1. Dp4+	5. Lactic Acid
2. Dp3	6. Glycerol
3. Maltose	7. Acetic Acid
4. Glucose	8. Ethanol

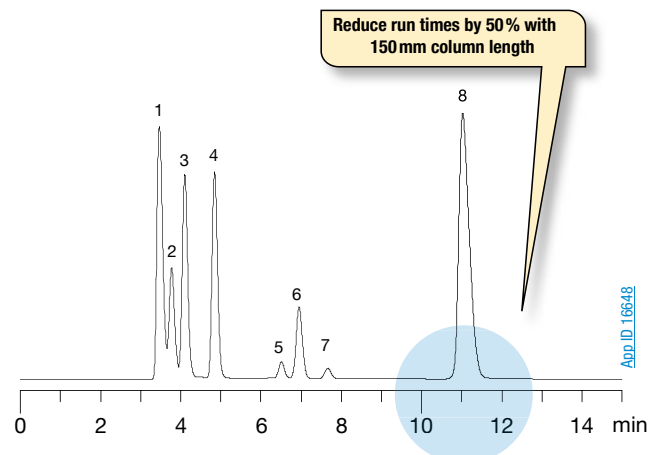

Column: Rezex ROA-Organic Acid
Dimensions: 150 x 7.8 mm
Part No.: [00F-0138-K0](#)
Guard Cartridge: [AJ0-4490](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 0.005 N Sulfuric Acid
Flow Rate: 0.6 mL/min
Detection: RI @ 40 °C
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 60 °C
System: Shimadzu Prominence LC-20A System
Sample:

1. Dp4+	5. Lactic Acid
2. Dp3	6. Glycerol
3. Maltose	7. Acetic Acid
4. Glucose	8. Ethanol

Shorten GC Fuel Quality Testing
 Zebtron® ZB-Bioethanol GC column can shorten your quality test down to 5 minutes! (See pp. 122-123).

Extend Column Lifetime
 Protect the Rezex column from the intrusion of the metal ions by using Phenex™ Syringe Filters and SecurityGuard™. The filters and SecurityGuard guard cartridge system work by trapping metal ions, such as calcium, magnesium, and iron, which can damage the column and cause it to lose or change separation efficiency. (See pp. 10 and 326).

Rezex™ Organic Acid and Carbohydrate Columns

Rezex™ vs. Bio-Rad® Aminex®

Phenomenex guarantees satisfaction when using Rezex HPLC columns. As illustrated below, Rezex offers advantages that enhance chromatographic results, increase throughput, and simplify quantitation.

Easier, Accurate Quantitation

Due to improved peak shape

Saccharides

Conditions for both columns:

Column: Rezex RCM-Monosaccharide
Aminex HPX-87C

Dimensions: 300 x 7.8 mm

Mobile Phase: Water


Flow Rate: 0.6 mL/min

Detection: ELSD

Temperature: 80 °C

Sample: 1. Melezitose 4. Mannose
2. Maltose 5. Fructose
3. Glucose 6. Ribitol

Superior Peak Shape

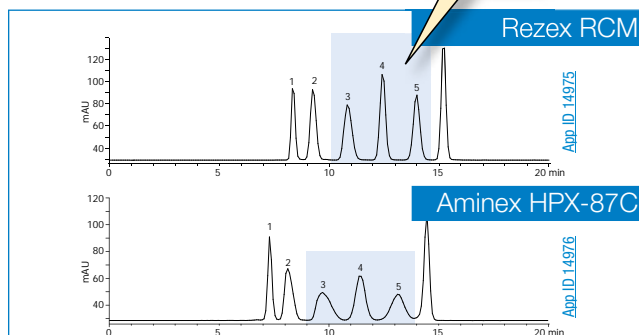

Comparative separations may not be representative of all applications.

Baseline Separation of Critical Sample Components

Due to improved resolution

Sugars

Conditions for both columns:

Column: Rezex RCM-Monosaccharide
Aminex HPX-87C

Dimensions: 300 x 7.8 mm

Mobile Phase: Water


Flow Rate: 0.6 mL/min

Detection: ELSD

Temperature: 80 °C

Sample: 1. Sucrose 4. Fructose
2. Glucose 5. Sorbitol
3. Galactose

Baseline Resolution

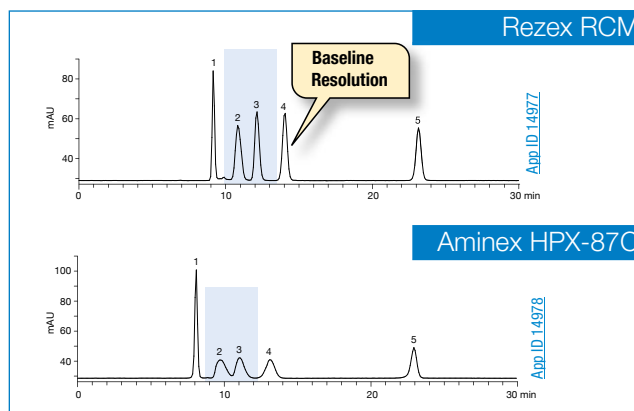

Applications

Food Softeners

Column: Rezex RCM-Monosaccharide

Dimensions: 300 x 7.8 mm

Part No.: [00H-0130-K0](#)


Mobile Phase: Water

Flow Rate: 0.5 mL/min

Detection: RI

Temperature: 60 °C

Sample: 1. Glycerol
2. Methoxypolyethylene Glycol
3. Triethylene Glycol
4. Sorbitol
5. Urea

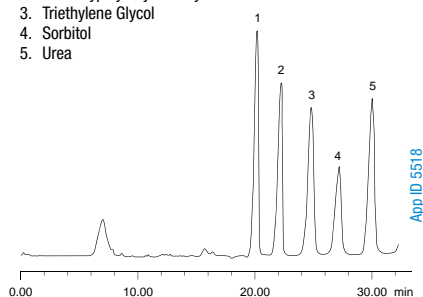

Amino Sugars

Column: Rezex ROA-Organic Acid

Dimensions: 300 x 7.8 mm

Part No.: [00H-0138-K0](#)


Mobile Phase: 1% Phosphoric Acid

Flow Rate: 0.6 mL/min

Detection: RI

Temperature: Ambient


Sample: 1. Glucose
2. N-Acetylglucosamine
3. N-Acetylgalactosamine

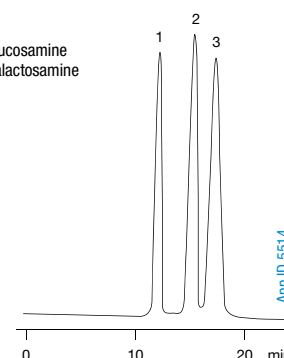

Rezex™ Organic Acid and Carbohydrate Columns


Organic Acids

Column: Rezex ROA-Organic Acid
Dimensions: 300 x 7.8 mm
Part No.: [00H-0138-KO](#)
Guard Cartridge: [AJ0-4490](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 0.005 N Sulfuric Acid
Flow Rate: 0.5 mL/min
Detection: UV @ 210 nm
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 55 °C
Sample: 1. Oxalic
 2. Citric
 3. Tartaric
 4. Succinic
 5. Formic
 6. Acetic

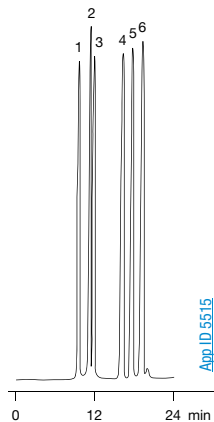


Saccharides

Column: Rezex RCM-Monosaccharide
Dimensions: 300 x 7.8 mm
Part No.: [00H-0130-KO](#)
Guard Cartridge: [AJ0-4493](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: Water
Flow Rate: 0.6 mL/min
Detection: RI
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 85 °C
Sample: 1. Melezitose
 2. Maltose
 3. Glucose
 4. Mannose
 5. Fructose
 6. Ribitol

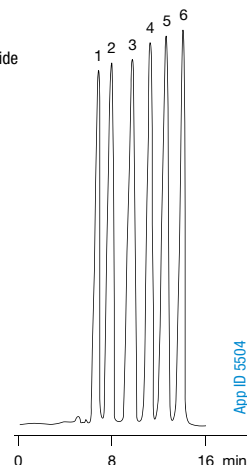


Apple Juice

Column: Rezex RCM-Monosaccharide
Dimensions: 300 x 7.8 mm
Part No.: [00H-0130-KO](#)
Guard Cartridge: [AJ0-4493](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: Water
Flow Rate: 0.6 mL/min
Detection: RI
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 75 °C
Sample: 1. Sucrose
 2. Glucose
 3. Fructose

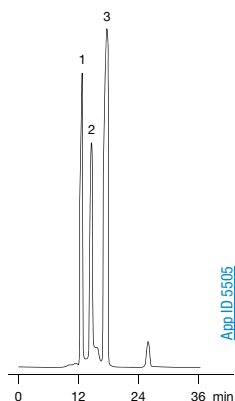


Mannitol and Sorbitol

Column: Rezex RPM-Monosaccharide
Dimensions: 100 x 7.8 mm
Part No.: [00D-0135-KO](#)
Guard Cartridge: [AJ0-4492](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: Water
Flow Rate: 0.6 mL/min
Detection: ELSD
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 80 °C
Sample: 1. Mannitol
 2. Sorbitol

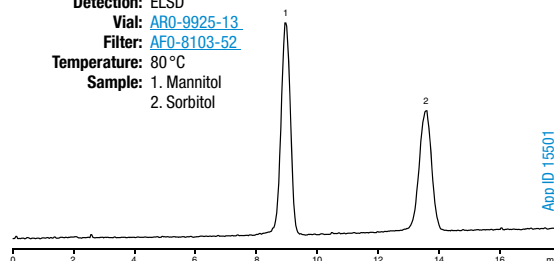

Oligosaccharides


Column: Rezex RSO-Oligosaccharide
Dimensions: 200 x 10 mm
Part No.: [00P-0133-NO](#)
Mobile Phase: Water
Flow Rate: 0.3 mL/min
Detection: RI
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 75 °C
Sample: Malto-Oligosaccharides as shown

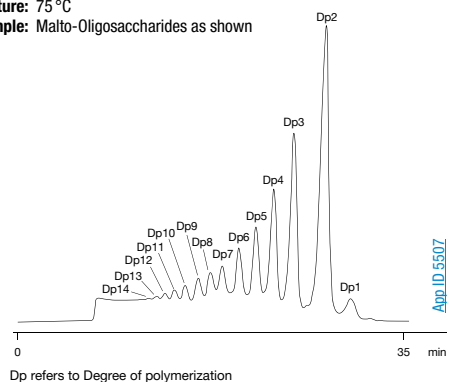

Saccharides

Column: Rezex RPM-Monosaccharide
Dimensions: 300 x 7.8 mm
Part No.: [00H-0135-KO](#)
Guard Cartridge: [AJ0-4492](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: Water
Flow Rate: 0.6 mL/min
Detection: RI
Vial: [ARO-9925-13](#)
Filter: [AF0-8103-52](#)
Temperature: 75 °C

Sample: 1. Stachyose
 2. Maltose
 3. Glucose
 4. Xylose
 5. Galactose
 6. Fructose
 7. Meso-Erythritol
 8. Mannitol
 9. Salicin
 10. Xylitol
 11. Sorbitol

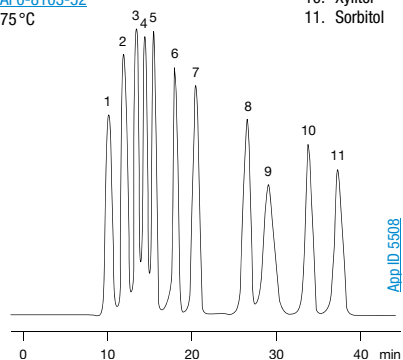


Rezex™ Organic Acid and Carbohydrate Columns

Specifications and Operating Recommendations


	RCM-Monosaccharide	RSO-Oligosaccharide	RNO-Oligosaccharide	RNM-Carbohydrate	RAM-Carbohydrate
Part Number	00H-0130-K0	00P-0133-N0	00P-0137-N0	00H-0136-K0	00H-0131-K0
Ionic Form	Calcium	Silver	Sodium	Sodium	Silver
Standard Dimensions	300 x 7.8 mm	200 x 10 mm	200 x 10 mm	300 x 7.8 mm	300 x 7.8 mm
Matrix	Sulfonated Styrene-divinylbenzene				
Cross Linking	8%	4%	4%	8%	8%
Particle Size	8 µm	12 µm	12 µm	8 µm	8 µm
Min. Efficiency (p/m) based on last peak	35,000	N/A	N/A	30,000	35,000
Typical Pressure (psi @ Testing Flow Rate)	260	115	130	170	285
Max. Pressure (psi @ Max Flow Rate)	1,000	300	300	1,000	1,000
Max. Flow Rate (mL/min)	1.0 (see pressure)	0.3	0.3	1.0	1.0
Max. Temperature (°C)	85	85	85	85	85
Typical Mobile Phase	Water	Water	Water	Water	Water
pH Range	Neutral	Neutral	Neutral	Neutral	Neutral
Guard Column Part No.	03B-0130-K0	03R-0133-N0	03R-0137-N0	03B-0136-K0	03B-0131-K0

Cleaning, Regeneration and Storage

	Organic Modifiers (Max)		5% Methanol, IPA, EtOH		
Inorganic Modifiers	5% CaSO ₄ , Ca(NO ₃) ₂ , CaCl ₂	5% Silver Nitrate	5% Sodium Salts	5% Sodium Salts	2% Silver Nitrate
Avoid 	Acids, Bases, Non-Calcium Salts/ Metal Ions, >30% Acetonitrile	Acids, Bases, Non-Silver Salts/ Metal Ions, >30% Acetonitrile	Acids, Bases, Non-Sodium Salts/ Metal Ions, >30% Acetonitrile	Acids, Bases, Non-Sodium Salts/ Metal Ions, >30% Acetonitrile	Acids, Bases, Non-Silver Salts/ Metal Ions, >30% Acetonitrile
Cleaning Solvent	100% Water	100% Water	100% Water	100% Water	100% Water
Flow Rate (mL/min)	0.4	0.1	0.1	0.4	0.4
Temperature (°C)	85	85	85	85	85
Duration (hrs)	12	12	12	12	12
Regeneration Solvent	0.1 M Ca(NO ₃) ₂	0.1 M AgNO ₃	0.1 M NaNO ₃	0.1 M NaNO ₃	0.1 M AgNO ₃
Flow Rate (mL/min)	0.2	0.1	0.2	0.2	0.2
Temperature (°C)	85	85	85	85	85
Duration (hrs)	4-16	4-16	4-16	4-16	4-16
Ship/Storage Solvent	Water	Water	Water	Water	Water

	RPM-Monosaccharide	RHM-Monosaccharide	ROA-Organic Acid	RFQ-Fast Acid	RCU-Sugar Alcohols
Part Number	00H-0135-K0	00H-0132-K0	00H-0138-K0	00D-0223-K0	00G-0130-D0
Ionic Form	Lead	Hydrogen	Hydrogen	Hydrogen	Calcium
Standard Dimensions	300 x 7.8 mm	300 x 7.8 mm	300 x 7.8 mm	100 x 7.8 mm	250 x 4.0 mm
Matrix	Sulfonated Styrene-divinylbenzene				
Cross Linking	8%	8%	8%	8%	8%
Particle Size	8 µm	8 µm	8 µm	8 µm	8 µm
Min. Efficiency (p/m) based on last peak	35,000	35,000	50,000 (Acetic Acid)	30,000	12,000
Typical Pressure (psi @ Testing Flow Rate)	190	275	580	365	90
Max. Pressure (psi @ Max Flow Rate)	1,000	1,000	1,000	1,000	1,000
Max. Flow Rate (mL/min)	1.0	1.0	1.0	1.0	0.5
Max. Temperature (°C)	85	85	85	85	85
Typical Mobile Phase	Water	Water	0.005 N H ₂ SO ₄	0.005 N H ₂ SO ₄	Water
pH Range	Neutral	1-8	1-8	1-8	Neutral
Guard Column Part No.	03B-0135-K0	03B-0132-K0	03B-0138-K0	03B-0223-K0	03A-0130-D0

Cleaning, Regeneration and Storage

	Organic Modifiers (Max)		5% Methanol, IPA, EtOH		
Inorganic Modifiers	5% Lead Nitrate	5% HNO ₃ , H ₃ PO ₄	5% HNO ₃ , H ₃ PO ₄	5% HNO ₃ , H ₃ PO ₄	5% CaSO ₄ , Ca(NO ₃) ₂ , CaCl ₂
Avoid 	Acids, Bases, Non-Lead Salts/ Metal Ions, >30% Acetonitrile	Acids, Bases, Salts/ Metal Ions, >30% Acetonitrile	Acids, Bases, Salts, Metal Ions, pH > 3, >30% Acetonitrile	Acids, Bases, Salts, Metal Ions, pH > 3, >30% Acetonitrile	Acids, Bases, Non-Calcium Salts, or Metal Ions, >30% Acetonitrile
Cleaning Solvent	100% Water	100% Water	100% Water	100% Water	100% Water
Flow Rate (mL/min)	0.4	0.4	0.4	0.4	0.1
Temperature (°C)	85	85	85	85	85
Duration (hrs)	12	12	12	12	12
Regeneration Solvent	0.1 M Pb(NO ₃) ₂	0.025 M H ₂ SO ₄	0.025 M H ₂ SO ₄	0.025 M H ₂ SO ₄	0.1 M Ca(NO ₃) ₂
Flow Rate (mL/min)	0.2	0.2	0.2	0.2	0.1
Temperature (°C)	85	85	85	85	85
Duration (hrs)	4-16	4-16	4-16	4-16	4-16
Ship/Storage Solvent	Water	Water	0.005 N H ₂ SO ₄	0.005 N H ₂ SO ₄	Water

If Rezex columns do not provide at least an equivalent separation as compared to a competing column of the same particle size, phase and dimensions, return the column with the comparative data within 45 days for a FULL REFUND.

Retention Times for Some Carbohydrates and Sugar Alcohols

Counter Ion	Analyte	RAM Ag ⁺	RCM Ca ⁺²	RNM Na ⁻	RHM H ⁻	RPM Pb ⁺²
Adonitol (Ribitol)		11.54	14.93	11.10	11.11	20.15
D-Altrose		11.95	12.71	11.45	10.21	15.82
D-(-)-Arabinose		13.01	13.56	12.65	11.24	16.47
D-(+)-Cellobiose		8.86	8.60	8.49	8.02	11.00
D-(+)-Digitoxose		11.90	13.82	11.39	12.59	15.32
Dulcitol		11.64	21.61	11.10	10.71	33.25
Meso-Erythritol		12.31	15.49	11.78	12.14	19.82
D-(-)-Fructose		12.05	13.65	11.76	10.31	17.71
L-(-)-Fucose		12.75	13.19	12.30	11.65	16.19
D-(+)-Galactose		11.87	11.73	11.47	10.19	14.94
Gentiobiose		8.70	8.40	8.40	7.87	10.53
D-(+)-Glucose		11.04	10.37	10.71	9.62	12.92
Inositol		12.59	13.35	12.14	9.98	18.87
Isomaltose		9.11	8.74	8.76	8.02	11.28
Lactose		9.27	9.03	8.78	8.32	11.89
Lactulose		9.75	10.32	9.23	8.57	13.95
D- Lyxose		12.41	14.06	11.98	10.68	16.66
D- Maltose		9.16	8.81	8.75	8.18	11.59
Maltotriose		8.27	8.10	7.94	7.51	11.02
Maltulose		9.25	9.47	8.82	8.27	12.40
D- Mannitol		11.36	17.82	10.80	10.59	24.90
D-(+)-Mannose		12.04	12.04	11.54	10.16	16.39
Melibiose		9.26	9.04	8.82	8.14	11.97
D-(+)-Melezitose		8.00	7.93	7.66	7.54*	9.94
D-(+)-Raffinose		8.10	8.16	7.76	7.88*	10.28
L-(+)-Rhamnose		11.50	12.18	11.00	10.90	14.47
D-(-)-Ribose		14.59	23.38	14.34	11.42	33.48
Salicin		18.51	18.58	17.36	14.98	26.81
D-Sorbitol		11.91	22.45	11.39	10.83	35.97
Stachyose		7.60	7.59	7.30	7.27	9.72
Sucrose		9.03	8.71	8.65	9.24*	11.00
Trehalose		8.91	8.72	8.49	8.32	11.01
Xylitol		12.69	22.01	12.16	11.78	32.38
D-(+)-Xylose		12.06	11.62	11.68	10.24	13.84

* Partial hydrolysis results.

Conditions:

Dimensions: 300 x 7.8 mm
Mobile Phase: Water (degassed)
Flow Rate: 0.6 mL/min
Temperature: 80 °C
Detection: RI @ 40 °C

Column Cross Reference Chart

Phenomenex Rezex™	Bio-Rad® Aminex®	Supelco® SUPELCOGEL™	Waters® Sugar-Pak™	Transgenomic® CARBOSEP™	Sepax® Carbomix®
RCM-Monosaccharide	HPX-87C 125-0095	Supelcogel Ca	Sugar-Pak 1	CARBOSep CHO-820	Carbomix Ca
RHM-Monosaccharide	HPX-87H 125-0140	Supelcogel C-610H & H	N/A	ICSep ION-300	Carbomix H
RPM-Monosaccharide	HPX-87P 125-0098	Supelcogel Pb	N/A	CARBOSep COREGEL-87P	Carbomix Pb
RNM-Carbohydrate	HPX-87N 125-0143	N/A	N/A	N/A	Carbomix Na
RSO-Oligosaccharide	HPX-42A 125-0097	Supelcogel Ag1 & Ag2	N/A	N/A	N/A
ROA-Organic Acid	HPX-87H 125-0140	Supelcogel C-610H & H	N/A	N/A	N/A
RFQ-Fast Acid	Fast Acid 125-0100	N/A	N/A	N/A	N/A
RKP-Potassium	HPX-87K 125-0142	Supelcogel K	N/A	CARBOSep COREGEL-87K	Carbomix K
RCU-USP Sugar Alcohols	Sugar Alcohols 125-0094	N/A	N/A	N/A	N/A

Ordering Information

Columns					Guards		SecurityGuard™ Cartridges (mm)
Description	Part No.	Cross Linkage	Ionic Form	Size (mm)	Part No.	Size (mm)	4 x 3.0* /10pk
RCM-Monosaccharide	00F-0130-KO	8%	Calcium	150 x 7.8	03B-0130-KO	50 x 7.8	AJ0-4493
RCM-Monosaccharide	00H-0130-KO	8%	Calcium	300 x 7.8	03B-0130-KO	50 x 7.8	AJ0-4493
RHM-Monosaccharide	00H-0132-KO	8%	Hydrogen	300 x 7.8	03B-0132-KO	50 x 7.8	AJ0-4490
RAM-Carbohydrate	00H-0131-KO	8%	Silver	300 x 7.8	—	—	AJ0-4491
RSO-Oligosaccharide	00P-0133-NO	4%	Silver	200 x 10.0	03R-0133-NO	60 x 10.0	—
RNO-Oligosaccharide	00P-0137-NO	4%	Sodium	200 x 10.0	03R-0137-NO	60 x 10.0	—
RPM-Monosaccharide	00H-0135-KO	8%	Lead	300 x 7.8	03B-0135-KO	50 x 7.8	AJ0-4492
RPM-Monosaccharide	00D-0135-KO	8%	Lead	100 x 7.8	03B-0135-KO	50 x 7.8	AJ0-4492
RNM-Carbohydrate	00H-0136-KO	8%	Sodium	300 x 7.8	03B-0136-KO	50 x 7.8	—
ROA-Organic Acid	00F-0138-EO	8%	Hydrogen	150 x 4.6	—	—	AJ0-4490
ROA-Organic Acid	00G-0138-EO	8%	Hydrogen	250 x 4.6	—	—	AJ0-4490
ROA-Organic Acid	00F-0138-KO	8%	Hydrogen	150 x 7.8	03B-0138-KO	50 x 7.8	AJ0-4490
ROA-Organic Acid	00H-0138-KO	8%	Hydrogen	300 x 7.8	03B-0138-KO	50 x 7.8	AJ0-4490
RKP-Potassium	00H-3252-KO	8%	Potassium	300 x 7.8	—	—	—
RFQ-Fast Acid	00D-0223-KO	8%	Hydrogen	100 x 7.8	03B-0223-KO	50 x 7.8	AJ0-4490
RCU-USP Sugar Alcohols	00G-0130-DO	8%	Calcium	250 x 4.0	03A-0130-DO	30 x 4.0	AJ0-4493

for ID: 3.2-8.0 mm

*SecurityGuard Analytical Cartridges require universal holder Part No.: [KJ0-4282](#)



For Column Heater, see p. 408



For our full line of Column Performance Check Standards, see pp. 414-415

Increase Lab Safety with HPLC/UHPLC Solvent Protection SecurityCAPS

The SecurityCAP mobile phase and solvent waste safety caps prevent dangerous vapors and gases from leaving HPLC/UHPLC solvent reservoirs. Over time, these chemicals can have a negative impact on the health of all employees and visitors in the lab. When lab safety and dependable results are a priority, you need SecurityCAPs!

Mobile Phase Safety Filter and Cap

- Increases Health and Worker Safety**
 Solvent vapors and gasses are restricted to their containers
- Protects HPLC/UHPLC Results**
 Eliminates dust and other air contaminants from testing results
- Confidence During Quality and Safety Audits**
 Eliminate aluminum foil or Parafilm® covering solvent bottles



The SecurityCAP™ mobile phase safety filters have an integrated one-way valve and filter membrane that captures dust, particulates, and other airborne contaminants. This prevents unwanted items from entering the solvent container which can cause irreproducible HPLC/UHPLC results, solvent contamination, bacterial growth and ghost peaks, all of which could negatively impact both your chromatography and HPLC/UHPLC system.

HPLC/UHPLC Solvent Top/Cap Comparison

SecurityCAP offers several advantages over insufficient non-sealed tops/caps which can lead to both hazardous lab conditions and poor chromatography results. When it comes to lab safety, saving money on expensive solvents and ensuring solvent protection, there is no comparison to SecurityCAP.

	Open Top	Aluminum foil wrapped bottle top	Cap with two 10mm holes in the plastic	SecurityCAP™
Protects staff and visitors from volatile organic compounds released into lab	No	No	No	Yes
Ensures confidence during quality and safety audits	No	No	No	Yes
Protects solvents from both atmospheric gases and particulates	No	No	No	Yes
Saves money by preventing solvent evaporation	No	No	No	Yes
Prevents chemical spills/ splashes	No	No	No	Yes
Time monitor device for protection	No	No	No	Yes
100% Sealable	No	No	No	Yes
Easy to use	Yes	No	Yes	Yes
Improves lab safety	No	No	No	Yes

Waste Exhaust Filter and Cap

- Safer Laboratory Work Environment**
 Harmful chemical vapors are safely collected and air quality is protected
- Large Capacity Waste Safety Filter**
 High surface area (560 m²/g) multi-compound adsorbent
- Easy to Use**
 No more twisting tubes during bottle exchange




SecurityCAP solvent waste caps and exhaust filters ensure lab air quality. Feel confident that volatile vapors from solvent waste containers are being captured safely, beyond fume cupboards or hoods.

Prevent Unwanted Changes in Mobile Phase pH

As every chromatographer knows, the pH of the mobile phase can have dramatic effects on selectivity, capacity factor (retention factor), peak shape, resolution, and reproducibility of your HPLC/UHPLC analysis. Because slight variations in pH can have a dramatic impact on the separation, careful mobile phase preparation and protection are essential. When compared to other mobile phase solvent tops, SecurityCAP offers the superior solution to ensure the mobile phase pH will stay constant during use. This ensures reliable solvent conditions for results you can trust!



A 1L solution of 4mM ammonium bicarbonate buffer at pH 11 was made for each bottle and left in a hood for 7 days. The pH was checked before and after the experiment and the percent difference was calculated.

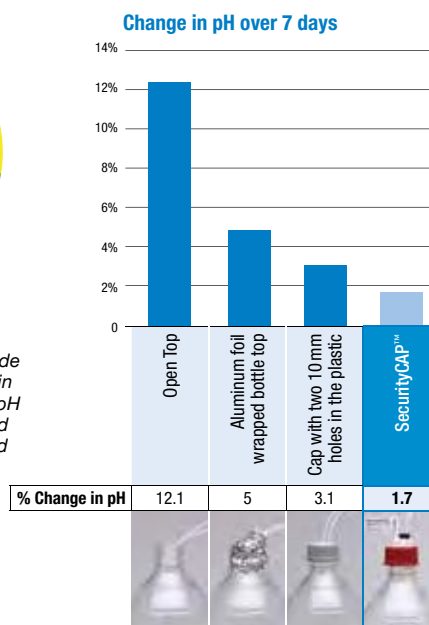

SecurityCAP™ LC Solvent Safety Products

guarantee

If SecurityCAP Safety Products do not perform as well or better than your current solvent safety products of similar type, dimensions, and material, return the product with comparative data within 45 days for a FULL REFUND



Mobile Phase (Eluent) Safety Starter Kits

Ordering Information

SecurityCAP™ Mobile Phase Starter Kits

Part No.	Description
AC2-1245	2-port GL45 Cap and 6-month Safety Filter
AC2-4245	2-port GL45 Caps (x4) and 6-month Safety Filter (x4)
AC2-4240	2-port Merck S40 Caps (x4) and 6-month Safety Filter (x4)
AC2-1345	3-port GL45 Cap and 6-month Safety Filter
AC2-4345	3-port GL45 Caps (x4) and 6-month Safety Filter (x4)
AC2-1445	4-port GL45 Cap and 6-month Safety Filter
AC2-4445	4-port GL45 Cap (x1) and 2-port Cap (3x) and 6-month Safety Filter (x4)
AC2-1545	5-port GL45 Cap and 6-month Safety Filter
AC2-1561	5-port S60/S61 Cap and 6-month Safety Filter



Waste Safety Starter Kits

Ordering Information

SecurityCAP Waste Starter Kits

Part No.	Description	Unit
AC1-1245	2-port GL/DIN45 Cap and 6-month Exhaust Filter + Barbed connector	ea
AC1-1545	5-port GL/DIN45 Cap and 6-month Exhaust Filter	ea
AC1-1551	5-port DIN51 Cap and 6-month Exhaust Filter	ea
AC1-1561	5-port S61 Cap and 6-month Exhaust Filter	ea



Replacement Filters

Ordering Information

SecurityCAP Mobile Phase Safety Filter

Part No.	Description	Unit
AC2-0161	6-month Capacity, 1/4 in.-28 Threads	ea
AC2-0961	6-month Capacity, 1/4 in.-28 Threads	10/pk

SecurityCAP Waste Safety Filters

Part No.	Description	Unit
AC1-0161	6-month Exhaust Filter for SecurityCAP, 1/4 in.-28 Threads	ea
AC1-0361	6-month Exhaust Filter for SecurityCAP, 1/4 in.-28 Threads	3/pk
AC1-0162	6-month Exhaust Filter for Wide-port Caps, GL14 Threads	ea
AC1-0362	6-month Exhaust Filter for Wide-port Caps, GL14 Threads	3/pk

SecurityCAP Waste Safety Filter Compatibility Table

Supplier	Phenomenex SecurityCAP Filters	
	ea	3/pk
SCAT® Safety Waste Caps	AC1-0162	AC1-0362
AIT® SmartCaps™	AC1-0162	AC1-0362
Agilent® InfinityLab Stay Safe Caps	AC1-0162	AC1-0362
VICI® Waste Caps	AC1-0161	AC1-0361
Canary-Safe™ Safety Caps	AC1-0162	AC1-0362
DURAN® DG Safety Caps	AC1-0162	AC1-0362



Fittings and Accessories

Ordering Information

SecurityCAP Fittings

Part No.	Description	Unit
AC3-1101	for 1/16 in. or 2.0 mm ID Tubing, 1/4 in.-28 Threads (POM), blue	ea
AC3-1201	for 2.3-2.6 mm ID Tubing, 1/4 in.-28 Threads (POM), white	ea
AC3-2101	for 1/8 in. ID Tubing, 1/4 in.-28 Threads (POM), black	ea

SecurityCAP Connectors

Part No.	Description	Unit
AC3-1001	Barbed connector, for 5-8 mm ID Tubing (PTFE), white	ea
AC3-1301	Y-connector for 6-8 mm ID Tubing (POM), white	ea

SecurityCAP Adapter

Part No.	Description	Unit
AC2-1138	Cap Thread Adapter, PTFE, GPI/GL 38 Female to GL45 Male	ea

SecurityCAP Sealing Plug

Part No.	Description	Unit
AC3-2001	1/4 in.-28 Threads (POM), white	ea

i POM = polyoxymethylene
PTFE = polytetrafluoroethylene (Teflon)

2014

Laboratory
EQUIPMENTReaders' Choice
WINNER

SecurityGuard™ Standard HPLC and SFC Column Protection

U.S. Patent No. 6, 162, 362

Column Protection for UHPLC, HPLC, SFC to PREP


Your Results and Your Column are Too Important Not to Protect

- Protect HPLC and UHPLC columns and extend lifetime
- Virtually no change in chromatography
- Available in analytical, semi-prep, and preparative sizes
- Simple to use

Did you know a common cause of high backpressure, split peaks, broad peaks, baseline noise, baseline drift and loss of resolution is contaminants? The fact is all mobile phases contain some chemical contaminants or microparticulates, from the sample, solvent, or wear on the polymeric seals of the pump or injector. These contaminants can clog frits, irreversibly bind to columns, degrade performance, and even damage the flow cell. An easy solution, SecurityGuard™ is a universal column protection system designed to effectively (and inexpensively), protect your valuable columns, from the damaging effects of chemical contaminants, without altering your chromatographic results.

guarantee

If the SecurityGuard Cartridge System does not provide at least an equivalent performance as compared to a competing guard cartridge system, return the product with the comparative data within 45 days for a FULL REFUND.

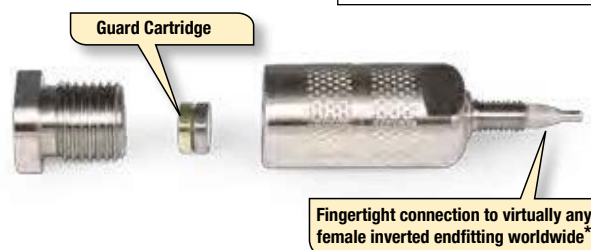

See SecurityGuard Standard in action video:


www.phenomenex.com/SecurityGuardInstallation

A Universal Guard Cartridge System

How SecurityGuard Standard Works*

The SecurityGuard Standard analytical cartridge holder (patented) directly finger-tightens into virtually any manufacturer's non core-shell and $\geq 3 \mu\text{m}$ particle columns. Contaminants are retained by

an inexpensive, 4 mm, disposable cartridge instead of fouling your expensive analytical column.

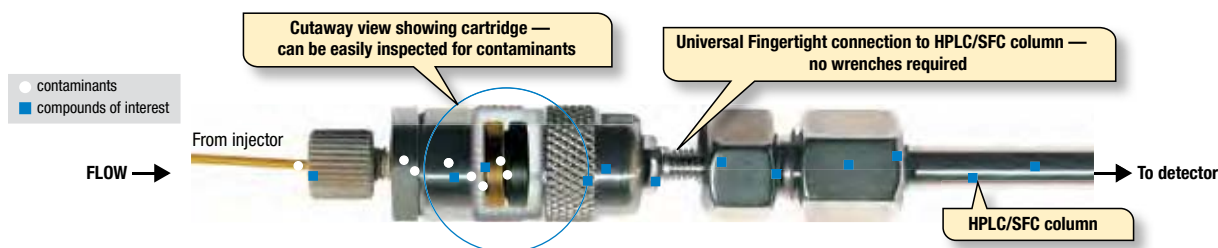


Increases HPLC Column Lifetime, Guaranteed!

Simply replace SecurityGuard cartridges instead of your expensive HPLC/SFC columns. In this graph, once the expired SecurityGuard Standard cartridge was replaced, the pressure immediately dropped and the column performance was restored allowing for extended column use.



The SecurityGuard Standard holder and cartridges are pressure rated to 5000 psi (345 bar).

For all core-shell and / or $< 3 \mu\text{m}$ particle columns, and all applications at higher pressures, use SecurityGuard ULTRA, see p.331. For available Semi-Preparative and PREP sizes, see pp. 328-330. For preparative SFC applications, use holder [AJ0-8617](#) for 15x21.2 mm cartridges or [AJ0-8618](#) for 15x30 mm cartridges. For Kinetex and Aeris Core-Shell SecurityGuard SemiPrep and PREP cartridges, see p. 330.

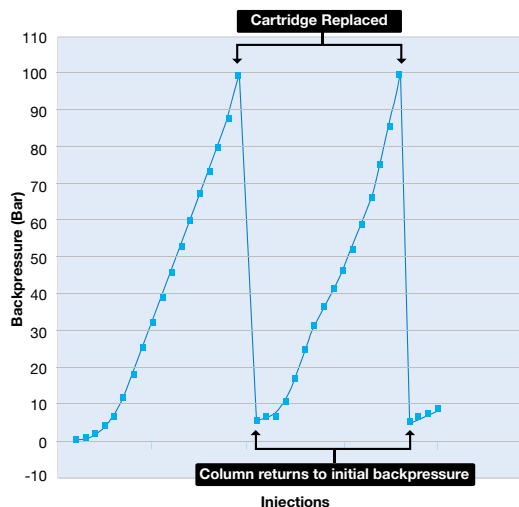

*Feature applies to traditional analytical-sized guard system only, and does not apply to SemiPrep or PREP guard cartridges.

Accelerated lifetime test using endogenous biomolecule matrix on a reversed phase C18 column, 5 μm , 50 x 4.6 mm with SecurityGuard Standard C18 cartridges. Backpressure values represent additional backpressure contributed by SecurityGuard.


U.S. Patent No. 6, 162, 362

See Your “Dirt” Feature

The “see your dirt” feature lets you know exactly when it’s time to replace your cartridge.

Visually inspect the surface of the cartridge’s packing material any time, without disturbing the packing bed. Now you can easily monitor visual contaminant build-up, and change your guard cartridge before it’s too late!

If your contaminants are colorless, replace the cartridge as often as needed to maintain chromatographic performance.

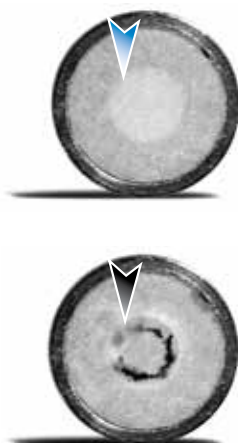

CLEAN

If it looks clean, the cartridge may be reinserted for further use.

DIRTY

If either discoloration or particle build-up is observed, it’s time to replace the cartridge.

“The SecurityGuard is easy to use and cartridge replacement is simple.”

F. Shakir, Sheffield Pharmaceuticals

“We didn’t see any change in retention time or difference in the peaks. The SecurityGuard has increased the life of the column.”

B. Dietz, ADM

The opinions stated herein are solely those of the individual and not necessarily those of any company or organization.

Analytical HPLC/SFC Holder Kit and Replacement Accessories

For 2.0 and 3.0 mm ID cartridges, use with 2.0 to 8.0 mm ID columns

Ordering Information


Analytical Kit

Part No.	Description
KJO-4282	SecurityGuard Standard Kit* (includes holder)

Replacement Parts and Accessories

Part No.	Description	Unit
AJ0-4283	PEEK Ferrules	3/pk
AJ0-4285	Stacking Rings	2/pk
AQ0-1389	PEEK Fingertight Fittings	10/pk
AJ0-4284	SecurityGuard Wrenches	2/pk

Compare, Virtually No Change

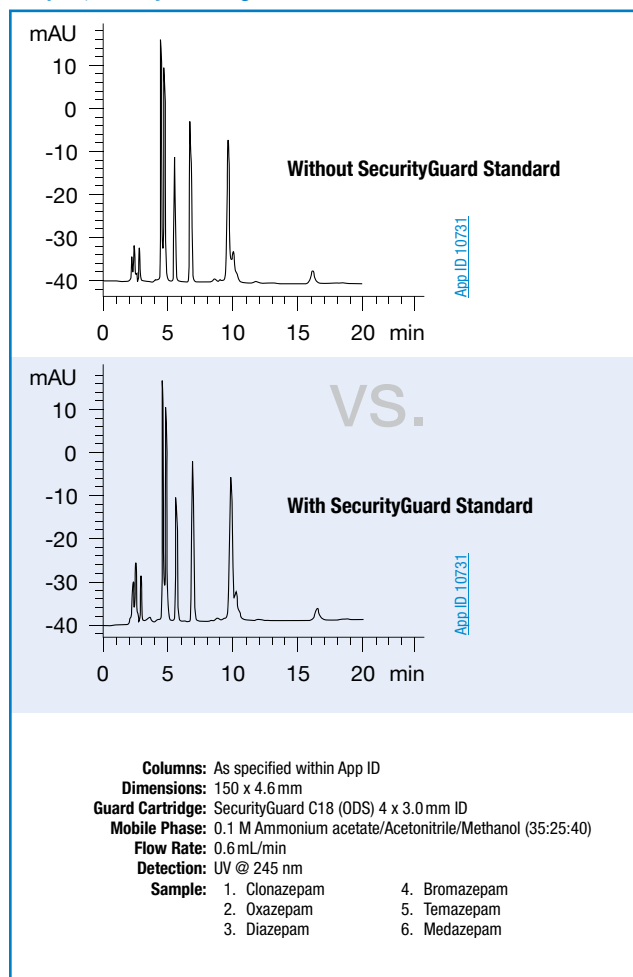

*Kit KJO-4282 Includes:



SecurityGuard™ PREP HPLC/SFC Column Protection

Semi-Preparative HPLC/SFC Holder

For 10.0 mm ID cartridges, use with 9 to 16 mm ID columns

Ordering Information

SecurityGuard SemiPrep Guard Cartridge Holder

Part No.	Description	Unit
AJ0-9281	Holder for 10.0 mm ID cartridges	ea

Accessories

Part No.	Description	Unit
----------	-------------	------

Nut and Ferrule

AQ0-3018	10-32 Threaded Male Nut and Ferrule Set for 1/16 in. OD capillary tubing	ea
--------------------------	--	----

Sure-Lok™ Fingertight Fittings

AQ0-1388	PEEK Sure-Lok Male Nut	ea
--------------------------	------------------------	----

AQ0-1389	PEEK Sure-Lok Male Nut	10/pk
--------------------------	------------------------	-------

Sure-Lok™ Couplers

AQ0-1392	PEEK Sure-Lok Coupler	ea
--------------------------	-----------------------	----

AQ0-1393	PEEK Sure-Lok Coupler	10/pk
--------------------------	-----------------------	-------

Column Sealing Plugs

AQ0-0217	Column Sealing Plug, 10-32 Thread size	10/pk
--------------------------	--	-------



For Semi-Preparative and Preparative Cartridges, see pp. 329-330

Preparative HPLC/SFC Holder (Two Sizes)

For 21.2 mm ID cartridges, use with 18 to 29 mm ID columns

Ordering Information

SecurityGuard Prep Guard Cartridge Holders

Part No.	Description	Unit
----------	-------------	------

AJ0-8223	HPLC Holder Kit for 21.2 mm ID cartridges, includes column coupler	ea
--------------------------	--	----

AJ0-8617	SFC Holder Kit for 21.2 mm ID cartridges, includes column coupler	ea
--------------------------	---	----

For 30.0 mm ID cartridges, use with 30 to 49 mm ID columns

Ordering Information

SecurityGuard Prep Guard Cartridge Holder

Part No.	Description	Unit
----------	-------------	------

AJ0-8277	HPLC Holder Kit for 30.0 mm ID cartridges, includes column coupler	ea
--------------------------	--	----

AJ0-8618	SFC Holder Kit for 30.0 mm ID cartridges, includes column coupler	ea
--------------------------	---	----

Replacement Parts and Accessories

Part No.	Description	Unit
----------	-------------	------

AQ0-8376	PREP Coupler, SS Tube, Nuts, and Ferrules, 10-32 Threads, 1/16 in. OD x 0.030 in. ID	ea
--------------------------	--	----

AQ0-8222	PREP Replacement O-Rings, Kalrez® For 15 x 21.2 mm SG HPLC Holder, Size 2-021	2/pk
--------------------------	---	------


AQ0-8318	PREP Replacement O-Rings, Kalrez® For 15 x 30 mm SG HPLC Holder, Size 2-025	2/pk
--------------------------	---	------

AQ0-8500	PREP Replacement O-Rings, Teflon® For 15 x 21.2 mm SG SFC Holder, Size 2-021	2/pk
--------------------------	--	------

AQ0-8501	PREP Replacement O-Rings, Teflon® For 15 x 30 mm SG SFC Holder, Size 2-025	2/pk
--------------------------	--	------

AT0-0465	Capillary S.S. Tubing, 0.020 in. ID x 0.062 in. (1/16 in.) OD x 10 cm length	5/pk
--------------------------	--	------

AT0-0466	Capillary S.S. Tubing, 0.020 in. ID x 0.062 in. (1/16 in.) OD x 20 cm length	5/pk
--------------------------	--	------

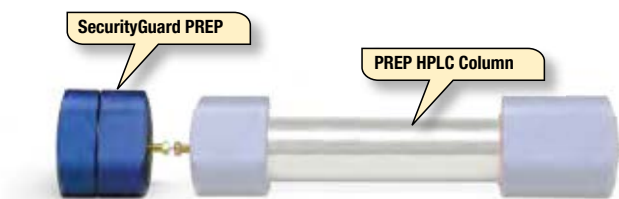

Holders		Cartridges
PREP	SFC	

21.2 mm ID HPLC Holder	21.2 mm ID SFC Holder	Cartridge (15 x 21.2 mm ID)

30 mm ID HPLC Holder	30 mm ID SFC Holder	Cartridge (15 x 30.0 mm ID)

O-Rings	Coupler	
---------	---------	--


Kalrez O-Rings	Teflon O-Rings	PREP Coupler

If the SecurityGuard Cartridge System does not provide at least an equivalent performance as compared to a competing guard cartridge system, return the product with the comparative data within 45 days for a FULL REFUND.

Cartridges and Holders

Step 1: Choose column ID

Step 2: Match column phase

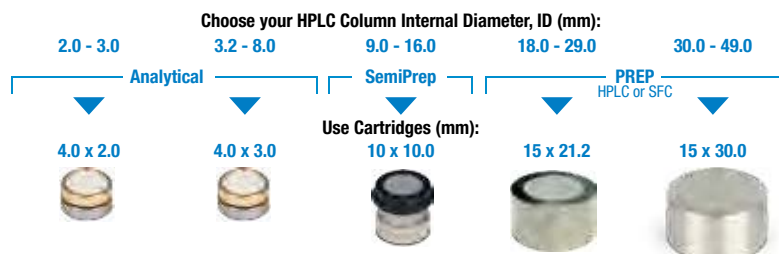

Ordering Information

Material	Description	pH Stability	Analytical		SemiPrep	PREP HPLC or SFC	
Cartridges for General Purpose/Pharmaceutical			/10pk	/10pk	/3pk	ea	ea
C18	(ODS, Octadecyl)	1.5 - 10	AJ0-4286	AJ0-4287	AJ0-7221	AJ0-7839	AJ0-8301
C12	(Dodecyl)	1.5 - 10	AJ0-6073	AJ0-6074	AJ0-7275	AJ0-7842	AJ0-8304
C8	(MOS, Octyl)	1.5 - 10	AJ0-4289	AJ0-4290	AJ0-7222	AJ0-7840	AJ0-8302
C5	(Pentyl)	1.5 - 10	AJ0-4292	AJ0-4293	AJ0-7372	—	—
C1	(TMS)	2 - 9	AJ0-4298	AJ0-4299	—	—	—
Silica	—	—	AJ0-4347	AJ0-4348	AJ0-7223	AJ0-7229	AJ0-8312
HILIC	(HILIC)	1.5 - 8	AJ0-8328	AJ0-8329	AJ0-8902	—	—
NH ₂	(Amino, Aminopropyl)	1.5 - 11	AJ0-4301	AJ0-4302	AJ0-7364	AJ0-8162	AJ0-8309
CN	(Cyano, Cyanopropyl)	2 - 7.5	AJ0-4304	AJ0-4305	AJ0-7313	AJ0-8220	AJ0-8311
Phenyl	(Phenylhexyl)	1.5 - 10	AJ0-4350	AJ0-4351	AJ0-7314	AJ0-7841	AJ0-8303
PFP(2)	(Pentafluorophenyl)	1.5 - 8	AJ0-8326	AJ0-8327	AJ0-8376	AJ0-8377	AJ0-8378
SCX	(SA, Strong Cation Exchanger)	2.5 - 7.5	AJ0-4307	AJ0-4308	—	AJ0-8595	AJ0-8596
SAX	(SB, Strong Anion Exchanger)	2.5 - 7.5	—	AJ0-4311	AJ0-7370	—	—
RP-1	(Reversed Phase - Polymer)	0 - 14	AJ0-5808	AJ0-5809	AJ0-7368	AJ0-8358	—
Polar-RP	(Ether-linked Phenyl)	1.5 - 7	AJ0-6075	AJ0-6076	AJ0-7276	AJ0-7845	AJ0-8307
Fusion-RP	(C18 Polar Embedded)	1.5 - 10	AJ0-7556	AJ0-7557	AJ0-7558	AJ0-7844	AJ0-8306
AQ C18	(Polar Endcapped C18)	1.5 - 7.5	AJ0-7510	AJ0-7511	AJ0-7512	AJ0-7843	AJ0-8305
Gemini [®] NX-C18	(C18 Twin-NX™ Technology)	1 - 12	AJ0-8367	AJ0-8368	AJ0-8369	AJ0-8370	AJ0-8371
Gemini C18	(C18 Twin™ Technology)	1 - 12	AJ0-7596	AJ0-7597	AJ0-7598	AJ0-7846	AJ0-8308
Gemini C6-Phenyl	(C6-Phenyl Twin Technology)	1 - 12	AJ0-7914	AJ0-7915	AJ0-9156	AJ0-9157	AJ0-9158
Luna [®] Omega Polar C18	(Polar Functional C18)	1.5 - 10	AJ0-7600	AJ0-7601	AJ0-9519	AJ0-7603	AJ0-7604
Luna [®] Omega PS C18	(Mixed-Mode C18)	1.5 - 10	AJ0-7605	AJ0-7606	AJ0-9520	AJ0-7608	AJ0-7609
Cartridges for Chiral			/10pk	/10pk	/3pk	ea	ea
<i>For use with chiral columns, such as Lux[®] Cellulose-1, -2, -3, -4, i-Cellulose-5, i-Amylose-1, & Amylose-1, -2 (Phenomenex); CHIRALCEL[®] OD-H[®], OJ-H[®] & CHIRALPAK[®] AD[®]-H, IC (DAICEL Corporation)</i>							
Lux i-Amylose-1	Amylose tris (3, 5-dimethylphenylcarbamate)	2 - 9	AJ0-8640	AJ0-8641	AJ0-8642	AJ0-8643	AJ0-8644
Lux i-Cellulose-5	Cellulose tris (3, 5-dichlorophenylcarbamate)	2 - 9	AJ0-8631	AJ0-8632	AJ0-8633	AJ0-8634	AJ0-8635
Lux Cellulose-1	Cellulose tris (3, 5-dimethylphenylcarbamate)	2 - 9	AJ0-8402	AJ0-8403	AJ0-8404	AJ0-8405	AJ0-8406
Lux Cellulose-2	Cellulose tris (3-chloro-4-methylphenylcarbamate)	2 - 9	AJ0-8398	AJ0-8366	AJ0-8399	AJ0-8400	AJ0-8401
Lux Cellulose-3	Cellulose tris (4-methylbenzoate)	2 - 9	AJ0-8621	AJ0-8622	AJ0-8623	AJ0-8624	AJ0-8625
Lux Cellulose-4	Cellulose tris (4-chloro-3-methylphenylcarbamate)	2 - 9	AJ0-8626	AJ0-8627	AJ0-8628	AJ0-8629	AJ0-8630
Lux Amylose-1	Amylose tris (3, 5-dimethylphenylcarbamate)	2 - 9	AJ0-9337	AJ0-9336	AJ0-9344	AJ0-9338	AJ0-9339
Lux Amylose-2	Amylose tris (5-chloro-2-methylphenylcarbamate)	2 - 9	AJ0-8471	AJ0-8470	AJ0-8472	AJ0-8473	AJ0-8474
Lux AMP	—	1 - 11.5	AJ0-8475	AJ0-8476	—	—	—

HPLC Guard Cartridge Holders (one-time purchase only)	/kit	/holder	/kit	/kit
Reusable Holder	KJ0-4282	AJ0-9281	AJ0-8223	AJ0-8277
SFC Guard Cartridge Holders	/holder	/kit	/kit	
Reusable Holder	AJ0-9281	AJ0-8617	AJ0-8618	

*For all core-shell and/or < 3µm particle columns use 2.1 to 4.6mm ID SecurityGuard ULTRA Holder and Cartridges, see page 331


Continued on next page

If the SecurityGuard Cartridge System does not provide at least an equivalent performance as compared to a competing guard cartridge system, return the product with the comparative data within 45 days for a FULL REFUND.

Cartridges and Holders (cont'd)

Step 1: Choose column ID

Step 2: Match column phase

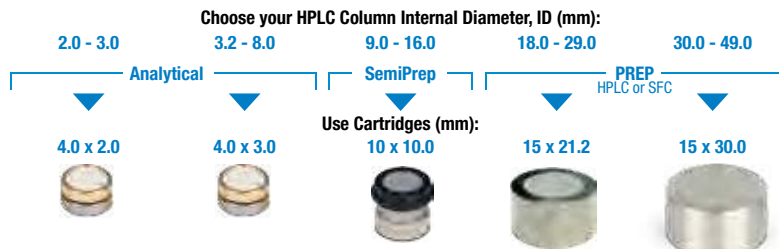

Ordering Information (continued)

Material	Description	pH Stability					
Cartridges for Core-Shell Media			—	—	/3pk	ea	ea
<i>For core-shell media columns, such as Kinetex® and Aeris™ (Phenomenex).</i>							
EVO C18	(ODS, Octadecyl)	1 - 12	*	*	AJO-9306	AJO-9304	AJO-9305
C18	(ODS, Octadecyl)	1.5 - 8.5	*	*	AJO-9278	AJO-9145	AJO-9204
C8	(MOS, Octyl)	1.5 - 8.5	*	*	—	AJO-9205	AJO-9217
PFP	(Pentafluorophenyl)	1.5 - 8.5	*	*	—	AJO-9146	—
F5	(Pentafluorophenylpropyl)	1.5 - 8.5	*	*	AJO-9323	AJO-9324	AJO-9325
Phenyl-Hexyl	(Phenylhexyl)	1.5 - 9	*	*	—	AJO-9147	AJO-9216
Biphenyl	(Biphenyl)	1.5 - 8.5	*	*	AJO-9280	AJO-9272	AJO-9273
HILIC	(HILIC)	2 - 7.5	*	*	—	AJO-9277	—
C18-Peptide	(ODS, Octadecyl)	1.5 - 9	*	*	AJO-9317	AJO-9318	AJO-9319
Cartridges for Protein and Polypeptide Reversed Phase			/10pk	/10pk	/3pk	ea	ea
<i>For use with silica columns for separation of proteins & peptides, such as Jupiter® (Phenomenex) and other widepore or 300 Å brands.</i>							
Widepore C18	(ODS, Octadecyl)	1.5 - 10	AJO-4320	AJO-4321	AJO-7224	AJO-7230	AJO-8313
Widepore C5	(Pentyl)	1.5 - 10	AJO-4326	AJO-4327	AJO-7371	—	—
Widepore C4	(Butyl)	1.5 - 10	AJO-4329	AJO-4330	AJO-7225	AJO-7231	AJO-8314
Cartridges for Synthetic DNA / RNA Analysis			/10pk	/10pk	/3pk	ea	ea
<i>For use with columns like Clarity® (Phenomenex).</i>							
Oligo-RP™	(C18 Twin Technology)	1 - 12	AJO-8134	AJO-8135	AJO-8136	AJO-8210	—
Oligo-WAX™	(WA, Weak Anion Exchanger)	1.5 - 11	—	AJO-8324	AJO-8325	AJO-8639	—
Oligo-XT	(ODS, Octadecyl)	1 - 12	*	*	AJO-9516	AJO-9517	AJO-9518
Cartridges for Silica GFC (Gel Filtration Chromatography)			—	/10pk	—	ea	—
<i>(Aqueous SEC) For use with silica GFC columns, such as Yarra™ and BioSep™ (Phenomenex); ZORBAX® GF-Series (Agilent); Bio-Sil® (Bio-Rad®).</i>							
GFC-2000	—	2 - 7.5	—	AJO-4487	—	AJO-8588	—
GFC-3000	—	2 - 7.5	—	AJO-4488	—	AJO-8589	—
GFC-4000	—	2 - 7.5	—	AJO-4489	—	AJO-8590	—
Cartridges for Polymer GPC (Gel Permeation Chromatography)			—	/3pk	—	—	—
<i>(Organic GPC) For use with polymer GPC columns, such as Phenogel™ (Phenomenex); PLgel™ (Agilent®); SDV® (PSS); Styragel® (Waters®); GPC Series (Shodex®); TSKgel® (Tosoh Bioscience®)</i>							
GPC***	—	0 - 14	—	AJO-9292	—	—	—
Cartridges for Carbohydrate/Organic Acid			—	/10pk	—	—	—
<i>For organic acid and carbohydrate analysis, such as Rezex™ (Phenomenex); Aminex® (Bio-Rad); Sugar-Pak™ (Waters).</i>							
Carbo-H+	—	1 - 8	—	AJO-4490	—	—	—
Carbo-Ag ⁺	—	Neutral	—	AJO-4491	—	—	—
Carbo-Pb ⁺²	—	Neutral	—	AJO-4492	—	—	—
Carbo-Ca ⁺²	—	Neutral	—	AJO-4493	—	—	—
HPLC Guard Cartridge Holders (one-time purchase only)			/kit	/holder	/kit	/kit	/kit
Reusable Holder	—	—	KJO-4282	AJO-9281	AJO-8223	AJO-8277	—
SFC Guard Cartridge Holders			—	/holder	/kit	/kit	/kit
Reusable Holder	—	—	—	AJO-9281	AJO-8617	AJO-8618	—

*For all core-shell and/or < 3 µm particle columns use 2.1 to 4.6 mm ID SecurityGuard ULTRA Holder and Cartridges, see page 331

**For use with saccharide and oligosaccharide columns in Ag+ form.

***Not compatible with HFIP solvent.

UHPLC / HPLC / SFC / PREP

Guard Finder

Having a difficult time finding the best column protection device for your specific UHPLC, HPLC, SFC or Prep column?

- Guard Finder matches over 57,000 column part numbers
- Interactive selection tool finds the appropriate column guard in seconds
- Quickly find column protection for any column from any of the top column manufacturers
- Search by brand, part number, technique, or column phase



SecurityGuard™ ULTRA

**SecurityGuard™
ULTRA**
UHPLC Column Protection

guarantee

UHPLC Column Protection

- Extends HPLC, core-shell, and < 3µm particle column lifetime
- Virtually no change in chromatography
- Fits virtually all manufacturers' columns 2.1 to 4.6 mm ID
- Pressure rated to 20000 psi (1378 bar)
- Simple to use


Universal Fit

Use SecurityGuard ULTRA with virtually all UHPLC columns 2.1 to 4.6mm ID. The extremely low dead volume of this unique product minimizes sample peak dispersion. It will efficiently remove microparticulates and chemical contaminants from the flow stream without contributing to system backpressure or dead volume (<0.3µL).

SecurityGuard ULTRA Increases Column Lifetime, Guaranteed!


When contaminants and particulates build up at the head of your column or on the guard cartridge, system backpressures can increase dramatically. By simply replacing the SecurityGuard ULTRA cartridge, instead of your column, you are able to regain normal operating conditions and reclaim original column performance.

Accelerated lifetime test using endogenous biological matrix on Kinetex 2.6µm C18 50 x 4.6 mm ID column

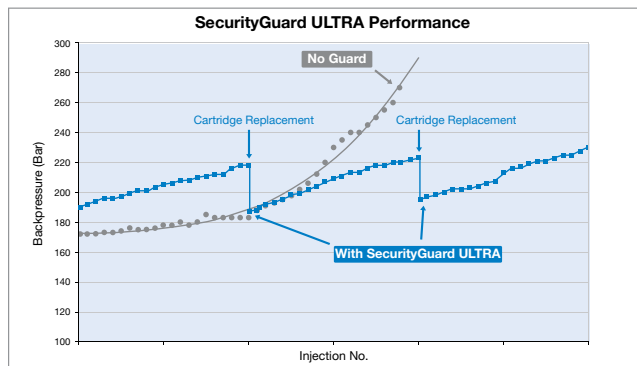

Protects with No Loss of Column Performance!

SecurityGuard ULTRA's unique design minimizes sample peak dispersion to maintain column performance without altering your chromatography results.

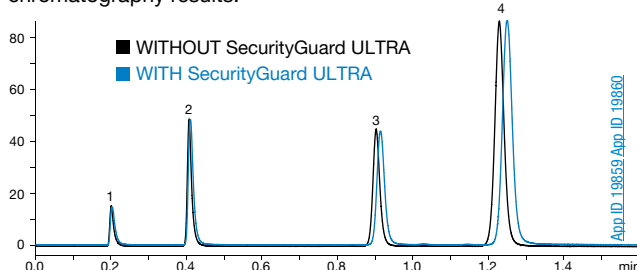

Conditions for both columns:

Column: Kinetex 1.7µm XB-C18

Dimensions: 50 x 2.1 mm

Guard Cartridge: SecurityGuard ULTRA C18 (ODS) 2.1 mm ID

Part No.: [AJ0-8768](#)

Mobile Phase: Acetonitrile / Water (50:50)

Flow Rate: 0.5 mL/min

Detection: UV @ 254 nm

- Sample:
1. Uracil
 2. Acetophenone
 3. Toluene
 4. Naphthalene

2012 R&D 100
Award Recipient



See SecurityGuard ULTRA in action:

www.phenomenex.com/SecurityGuardULTRA



Holder with cartridge, assembled



Holder

SecurityGuard ULTRA Cartridge Holder

Ordering Information

Part No.	Description	Unit
AJ0-9000	SecurityGuard ULTRA Cartridge Holder	ea

SecurityGuard ULTRA Cartridges

Ordering Information

Material	Description	pH Stability	Column ID (mm)		
			2.1	3.0	4.6
Cartridges for General Purpose/ Pharmaceutical					
			/3pk	/3pk	/3pk
EVO C18	(ODS, Octadecyl)	1.0 – 12.0	AJ0-9298	AJ0-9297	AJ0-9296
C18	(ODS, Octadecyl)	1.5 – 8.5*	AJ0-8782	AJ0-8775	AJ0-8768
C8	(MOS, Octyl)	1.5 – 8.5*	AJ0-8784	AJ0-8777	AJ0-8770
PFP	(Pentafluorophenyl)	1.5 – 8.5	AJ0-8787	AJ0-8780	AJ0-8773
F5	(Pentafluorophenyl)	1.5 – 8.5	AJ0-9322	AJ0-9321	AJ0-9320
Biphenyl	(Biphenyl)	1.5 – 8.5*	AJ0-9209	AJ0-9208	AJ0-9207
Phenyl	(Phenylhexyl)	1.5 – 8.5*	AJ0-8788	AJ0-8781	AJ0-8774
HILIC	HILIC	2.0 – 7.5	AJ0-8786	AJ0-8779	AJ0-8772
Polar C18	(Polar Functional C18)	1.5 – 8.5*	AJ0-9532	AJ0-9531	AJ0-9530

Cartridges for General Purpose/Pharmaceutical (Fully Porous Columns)

For fully porous columns like Luna® Omega (Phenomenex)

C18	(ODS, Octadecyl)	1.5 – 8.5*	AJ0-9502	AJ0-9501	AJ0-9500
Polar C18	(ODS, Octadecyl)	1.5 – 8.5*	AJ0-9505	–	–
PS C18	(Mixed-Mode C18)	1.5 – 8.5*	AJ0-9508	–	–

Cartridges for Protein and Peptide Reversed Phase

For use with columns like Aeris™ (Phenomenex)

Widepore C18	(ODS, Octadecyl)	1.5 – 8.5*	AJ0-8783	–	AJ0-8769
Widepore C8	(MOS, Octyl)	1.5 – 8.5*	AJ0-8785	–	AJ0-8771
Widepore C4	(Butyl)	1.5 – 8.5*	AJ0-8899	–	AJ0-8901
Peptide C18	(ODS, Octadecyl)	1.5 – 8.5*	AJ0-8948	AJ0-8947	AJ0-8946

Cartridges for Synthetic DNA / RNA Analysis

For use with columns like Clarity® (Phenomenex)

Oligo-MS C18	(ODS, Octadecyl)	1.5 – 8.5*	AJ0-9068	–	AJ0-9066
Oligo-XT	(ODS, Octadecyl)	1.0 – 12.0	AJ0-9515	–	AJ0-9514

Cartridges for Silica GFC (Gel Filtration Chromatography)

(Aqueous SEC) For use with silica GFC columns such as Yarra™ (Phenomenex)

X150	–	1.5 – 8.5	–	–	AJ0-9512
X300	–	1.5 – 8.5	–	–	AJ0-9513

*pH stable 1.5–8.5 under gradient conditions. pH stable 1.5–10 under isocratic conditions.

[AJ0-9000](#) is the universal holder designed for use with 2.1 mm, 3.0 mm and 4.6 mm ID cartridges.



Initial SecurityGuard ULTRA installation and cartridge replacement, requires 3 wrenches, which must be purchased separately: one 3/8 in. wrench ([AQO-8959](#); fits Kinetex, Aeris, and Oligo-MS column end-fittings), and two 1/8 in. wrenches ([AQO-8903](#); fits ULTRA cartridge and holder). See p. 417

Selectosil™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant.

Shodex®

By Showa Denko K.K.

- High efficiency polymer columns
- Wide application range



Guide for Shodex Column Selection

Solubility	Molecular Weight	Separation Mode	Column	Page
Water-insoluble	over 2000	SEC	GPC KF-803-805	322
	under 2000	SEC	GPC KF-802	322
		RPC	RSpak DE-413, 413L, DM-614	334
Water-soluble	over 2000	SEC	OHpak SB-803-806HQ, SUGAR KS-803-804, PROTEIN KW-802.5-804	333
		IEC	IEC QA-825, DEAE-825, SP-825, CM-825	334
		HIC	HIC PH-814	334
	under 2000	SEC	SB-802-802.5HQ, SUGAR KS-801, 803-804	332
		LEC	SUGAR SC1011, SP0810	334
		IEX	RSpak KC-811, SUGAR SH1011, SUGAR SH1821	333, 334
	IC	IC SI-90 4E, SI-50 4E, IC I-524A, YK-421	334	
	RPC	RSpak DE-613, 413	334	
	NPC	SUGAR SZ5532	334	


Organic GPC Columns

Shodex has a wide variety of columns for GPC (or SEC) using organic solvents. The columns are packed with porous S-DVB gels specially developed for GPC use.

Series Name	In-column Solvent	Applications
GPC KF-800 series	THF (tetrahydrofuran)	General purpose GPC

Calibration Curves for GPC KF-800 Series

Column: Shodex GPC KF-800 series
Dimensions: 8 x 300 mm



App ID: 10766

Ordering Information

Standard Columns

Column Type / Part No.

THF	ID x Length (mm)	Plate Number	Exclusion Limit
GPC KF-802	8 x 300	>16,000	5 x 10 ³
GPC KF-803	8 x 300	>16,000	7 x 10 ⁴
GPC KF-804	8 x 300	>16,000	4 x 10 ⁵
GPC KF-805	8 x 300	>10,000	4 x 10 ⁶

NOTE: Exclusion Limits in parentheses, (), are estimated values.

Note: 803, 804, and 805 are available packed in HFIP.

By Showa Denko K.K.


GFC (Aqueous GPC) Columns

Shodex has a wide variety of columns for GFC. Three types of GFC columns packed with different gel materials are available.

Series Name	Packing Material	Applications
OHpak SB-800HQ	PHM gel	Used for general purpose GFC of water-soluble polymers, proteins and enzymes
SUGAR KS-800	Sulfonated PS gel	Mono, di, tri, oligo and polysaccharides, starches and celluloses
PROTEIN KW-800	Porous silica gel	GFC of proteins, glycoproteins and peptides

Calibration Curves for OHpak SB-800HQ Series

Column: Shodex OHpak SB-800HQ
 Dimensions: 8 x 300 mm
 Eluent: Water
 Sample: 1. P-800
 2. P-400
 3. P-200
 4. P-100
 5. P-50
 6. P-20
 7. P-10
 8. P-5
 9. P-3
 10. P-1
 11. Maltotriose
 12. Maltose
 13. Glucose

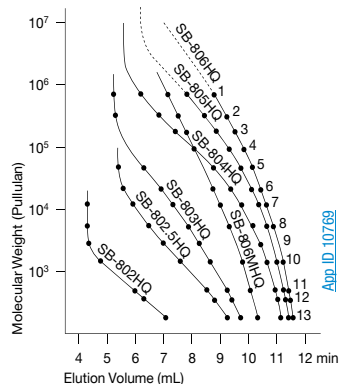

Ordering Information

Aqueous GPC Columns

Column Type/ Part No.	ID x Length (mm)	Plate Number	Exclusion Limit
OHpak SB-802HQ	8 x 300	>10,000	4 x 10 ³
OHpak SB-802.5HQ	8 x 300	>15,000	1 x 10 ⁴
OHpak SB-803HQ	8 x 300	>15,000	1 x 10 ⁵
OHpak SB-804HQ	8 x 300	>15,000	1 x 10 ⁶
OHpak SB-805HQ	8 x 300	>10,000	4 x 10 ⁶
OHpak SB-806HQ	8 x 300	>10,000	(2 x 10 ⁷)
OHpak SB-806MHQ	8 x 300	>10,000	(2 x 10 ⁷)
SUGAR KS-801 (Na ⁺)	8 x 300	>15,000	1 x 10 ³
SUGAR KS-803 (Na ⁺)	8 x 300	>15,000	5 x 10 ⁴
SUGAR KS-804 (Na ⁺)	8 x 300	>15,000	4 x 10 ⁵
PROTEIN KW-802.5	8 x 300	>20,000	5 x 10 ⁴
PROTEIN KW-803	8 x 300	>20,000	1.5 x 10 ⁵
PROTEIN KW-804	8 x 300	>10,000	6 x 10 ⁵

Note: Exclusion Limits in parentheses, (), are estimated values.

Calibration Standards

Ordering Information

Calibration Standards

Standard Type/Part No.	Material	Content	MW Range	Applications
STANDARD P-82	Pullulan	0.2 g x 8 grades	5,000 - 800,000	GFC (aqueous GPC)

Columns for Organic Acids

KC-811 enables an effective organic acids separation using a mixed mode of IEX, SEC and P&A. Organic acids also can be separated by RPC using RSpak DE-613.

Ordering Information

RSpak

Column Type/ Part No.	ID x Length (mm)	Plate Number	Packing Material	Counter Ion
RSpak KC-811	8 x 300	>17,000	S-DVB gel	H+

*Note: RSpak KC-811 was formerly known as Ionpak KC-811.

By Showa Denko K.K.

Ion Chromatography Columns

- Great alternative to Dionex® IonPac® AS4, AS4A, and AS14 columns
- High efficiency, general purpose IC column

Shodex offers an innovative IC column for the suppressor method that improves both the separation speed and resolution of anions in most matrices. With high theoretical plates (>5000/m for Sulfate), the column easily and efficiently separates organic and inorganic anions such as EPA Method 300 analytes, acetate, formate, methacrylate and oxalate. High loading and exceptional resistance to loading combine with features such as improved separation of the fluoride peak from the water dip.

Ordering Information

IC Columns

Column Type/ Part No.	ID x Length (mm)	Plate Number	Packing Material	Functional Group	Applications
IC SI-90 4E	4.0 x 250	>5,000 (S04)	PVA	Quaternary ammonium	Inorganic anions and organic acids
IC SI-90 G	4.6 x 10	(Guard)	—	—	(General purpose)
IC SI-50 4E*	4.0 x 250	>14,000	PVA	Quaternary ammonium	Inorganic anions and organic acids
IC I-524A	4.6 x 100	>2,000	PHM gel	Quaternary ammonium	Inorganic anions
IC YK-421	4.6 x 125	>2,500	Hydrophilic Polymer	Carboxyl Coated Silica	Simultaneous separation of monovalent and divalent cations
IC YS-50 (CH0-8194)	4.6 x 125	>5,500	PVA	Carboxyl	Suppressor and non-suppressor methods
IC YS-G (CH0-8195)	4.6 x 10	(Guard)	—	—	—

*Use IC SI-90G guard.

Columns for Proteins and Nucleic Acids

Ion-Exchange Columns

IEC series columns are suited for the analysis of proteins and nucleic acids.

Ordering Information

IEC Series Columns

Column Type/Part No.	ID x Length (mm)	Plate Number	Packing Material	Functional Group
IEC QA-825	8 x 75	>2,000	PHM gel	Quaternary ammonium (strong anion)
IEC DEAE-825	8 x 75	>2,000	PHM gel	Diethylaminoethyl (weak anion)
IEC SP-825	8 x 75	>2,000	PHM gel	Sulfopropyl (strong cation)
IEC CM-825	8 x 75	>2,000	PHM gel	Carboxymethyl (weak cation)

Other Columns

Column Type/Part No.	ID x Length (mm)	Plate Number	Packing Material	Functional Group	Separation Mode	Applications
HIC PH-814	8 x 75	>2,000	PHM gel	Phenyl	HIC	Proteins

Columns for Sugar Analysis

Ordering Information

Sugar Columns

Column Type/ Part No.	ID x Length (mm)	Plate Number	Exclusion Limit	Packing Material	Counter Ion	Separation Mode
SUGAR SH1011	8 x 300	>15,000	1,000	S-DVB gel	H ⁺	SEC + IEX
SUGAR SH1821	8 x 300	>15,000	10,000	S-DVB gel	H ⁺	SEC + IEX
SUGAR SC1011	8 x 300	>12,000	1,000	S-DVB gel	Ca ²⁺	SEC + IEX
SUGAR SP0810	8 x 300	>10,000	1,000	S-DVB gel	Pb ²⁺	SEC + LEC
SUGAR SC1211	6 x 250	>5,000		S-DVB gel	Ca ²⁺	P&A + LEC
SUGAR SZ5532	6 x 150	>5,000		S-DVB gel	Zn ²⁺	P&A + LEC
SUGAR KS-801	8 x 300	>15,000	1,000	S-DVB gel	Na ⁺	SEC + LEC

Aside from the columns listed here, there are other columns that can be used for sugar separations. SUGAR KS-800 series and OHpak SB-800 HQ series can also be used for sugar separations by SEC.

Polymer-Based Reversed Phase Columns

RSpak

Applications

DE	Suited for wide applications because its characteristics are similar to those of ODS columns.
DM	Suited for analysis of amino acids and polypeptides.

Ordering Information

RSpak Columns

Column Type/Part No.	Plate Number	ID x Length (mm)
RSpak DE-613	>7,000	6.0 x 150
RSpak DE-413	>11,000	4.6 x 150
RSpak DE-413L	>17,000	4.6 x 250
RSpak DE-G (DE-613P)	(guard column)	4.6 x 10
RSpak DM-614	>4,000	6.0 x 150

If SphereClone analytical columns do not provide at least an equivalent separation as compared to Spherisorb columns of the same phase, particle size and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Guaranteed Replacement to Spherisorb®

- Highly reproducible
- Long column life
- Mimics performance of Waters® Spherisorb®
- Economically priced

Phenomenex SphereClone columns have been developed to provide chromatographic behavior that mimics that of Waters Spherisorb columns. For comparative applications, please contact your local Phenomenex representative.

SphereClone™


VS.

Spherisorb®†


Material Characteristics

SphereClone™		Spherisorb®†	
3, 5, 10 µm	Particle Size	3, 5, 10 µm	
80 Å	Pore Size	80 Å	
200 m ² /g	Surface Area	200 m ² /g	
Carbon Load			
—	Silica	—	
6%	C6	6%	
6%	C8	6%	
7%	ODS(1)	6.2%	
12%	ODS(2)	12%	
2%	NH ₂	2%	

SEM of Base Silica




Surface
15,000x Magnification




Physical Mass Distribution and Shape
4,000x Magnification

SEM of Base Silica




Surface
15,000x Magnification




Physical Mass Distribution and Shape
4,000x Magnification

Particle Size Distribution

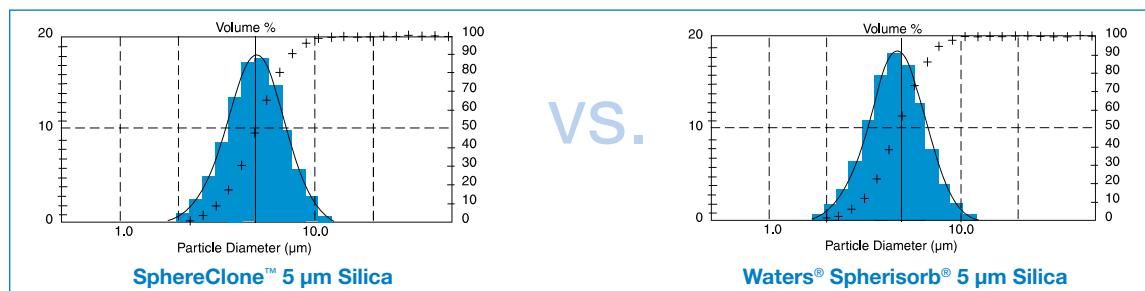

SphereClone Reproducibility

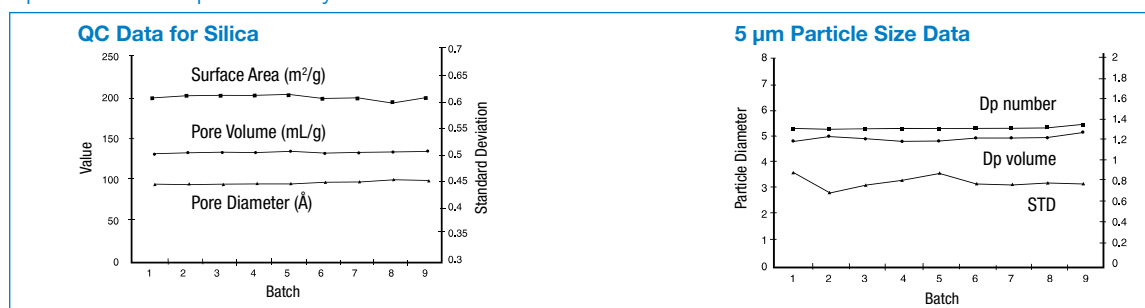

SphereClone™ Guaranteed Replacement to Spherisorb®

guarantee

If SphereClone analytical columns do not provide at least an equivalent separation as compared to Spherisorb columns of the same phase, particle size and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Ordering Information

3 µm Columns (mm)		SecurityGuard™ Cartridges (mm)		
Phases	50 x 4.6	100 x 4.6	150 x 4.6	4 x 3.0
				/10pk
C8	—	00D-4133-E0	—	AJ0-4290
ODS(1)	—	00D-4134-E0	00F-4134-E0	AJ0-4287
ODS(2)	00B-4135-E0	00D-4135-E0	00F-4135-E0	AJ0-4287
NH ₂	—	—	00F-4137-E0	AJ0-4302

for ID: 3.2-8.0 mm

5 µm Columns (mm)		SecurityGuard™ Cartridges (mm)	
Phases	150 x 4.6	250 x 4.6	4 x 3.0
			/10pk
Silica	00F-4139-E0	00G-4139-E0	AJ0-4348
C6	00F-4141-E0	00G-4141-E0	—
C8	00F-4142-E0	00G-4142-E0	AJ0-4290
ODS(1)	00F-4143-E0	00G-4143-E0	AJ0-4287
ODS(2)	00F-4144-E0	00G-4144-E0	AJ0-4287
NH ₂	00F-4147-E0	00G-4147-E0	AJ0-4302
SAX	00F-4149-E0	00G-4149-E0	AJ0-4311

for ID: 3.2-8.0 mm

SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)

10 µm Columns (mm)		SecurityGuard™ Cartridges (mm)	
Phases	250 x 4.6	4 x 3.0	
			/10pk
ODS(2)	00G-4156-E0	AJ0-4287	
SAX	00G-4160-E0	AJ0-4311	

for ID: 3.2-8.0 mm

*Comparative separations may not be representative of all applications.
*Spherisorb columns used for comparison studies were purchased from manufacturer.

Spherex™

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/spherex

Spherisorb®

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/spherisorb
- See SphereClone for a cost effective, guaranteed replacement to Spherisorb



For SecurityGuard Cartridge Holders and Cartridges, see p. 326

If STAR-ION™ A300 does not produce at least equivalent separation as compared to a competing column of a similar type*, simply send us comparative data with the STAR-ION™ A300 column within 45 days for a FULL REFUND.

* Suppressed mode ion columns.


Suppressed Mode Anion Analysis for EPA Method 300

- Excellent separation of inorganic anions and some common organic anions
- High resolution and peak symmetry
- An alternative to Dionex® IonPac® AS4A

EPA Method 300

Column: STAR-ION A300
Dimensions: 100 x 4.6 mm
Part No.: [00D-4090-E0-BV](#)
Eluent: 1.7 mM NaHCO₃ / 1.8 mM Na₂CO₃
Flow Rate: 2.0 mL/min
Detection: Suppressed Conductivity
Injection Volume: 20 µL
Sample:

1. Fluoride	2 mg/L
2. Chloride	20 mg/L
3. Nitrite	2 mg/L
4. Bromide	2 mg/L
5. Nitrate	10 mg/L
6. Phosphate	2 mg/L
7. Sulfate	60 mg/L

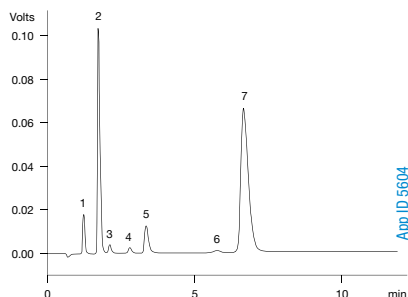

Material Specifications

Material Type	PSDVB with quaternary amine functionality
Mode of IC	Suppressed (optimized)
Max. Temperature	45 °C
Max. Pressure	1000 psi without guard column 1200 psi with guard column
Solvent Limitations	No organic solvents are recommended for use with STAR-ION

Ordering Information

Suppressed Mode Anion Analysis for EPA Method 300

Part No.	Description	Dimensions (mm)	Unit
00D-4090-E0-BV	STAR-ION A300 Anion column (PEEK)	100 x 4.6	ea
00D-4090-N0-BV	STAR-ION A300 Anion column (PEEK)	100 x 10	ea
ALO-3420	STAR-ION A300 Test Mix		ea
AQO-3351	PEEK ¼ in. - 28 to 10-32 Adapter to connect STAR-ION A300 analytical column to Dionex IC systems (use 2 fittings, one for each end of column)		ea
AQO-1388	PEEK long-nut fitting		ea
ATO-1107	PEEK capillary tubing ¼ in. OD x 0.010 in. D x 5 ft. L		ea
ATO-1110	Polymer tubing cutter		ea



For HPLC Column Heater (25-90°C), see p. 408

Sumichiral OA™

By Sumika Chemical Analysis Service, Ltd.

- For Availability and Ordering Information please contact your Phenomenex Technical Consultant or Visit: www.phenomenex.com/sumichiral

Full Range Selectivity for Reversed Phase Separation


Many different mechanisms of retention are utilized within reversed phase chromatography in order to retain and separate target analytes. Whether your compounds are hydrophobic or polar, Synergi columns provide you with a full range of selectivity, ensuring separation of extremely challenging and complex mixtures.

Synergi Polar-RP

Phenyl Ether-Linked

For polar and aromatic mixtures

Ether linkage increases aromaticity of the phenyl group and also provides $\pi-\pi$ interactions with conjugated compounds

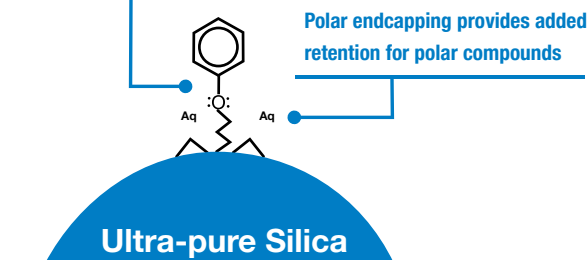


Synergi Fusion-RP

C18 Polar Embedded

Balanced non-polar and polar performance

Embedded polar group complements C18 ligand with balanced polar selectivity

TMS endcapping ensures sharp peaks

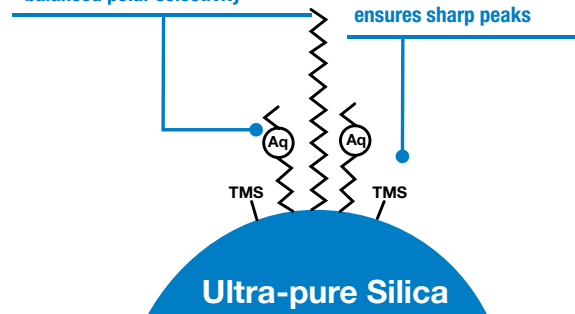


Synergi Hydro-RP

C18 Polar Endcapped

Strong non-polar and polar retention

Polar endcapping provides added retention for polar compounds

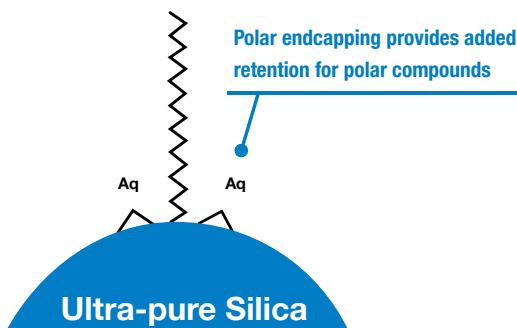


Synergi Max-RP

C12 TMS Endcapped

Excellent for basic compounds at neutral pH

High density ligands and extensive endcapping ensure sharp peaks

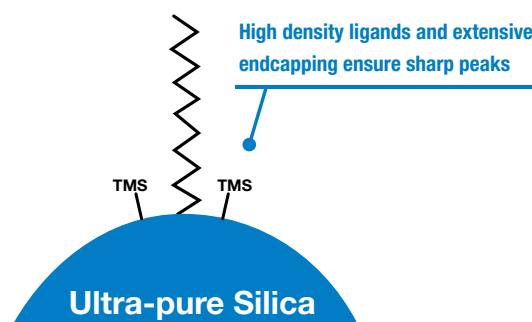


Material Characteristics

Packing Material	Particle Shape/Size (µm)	Pore Size (Å)	Pore Volume (mL/g)	Surface Area (m ² /g)	Carbon Load %	Calculated Bonded Phase Coverage (µmole/m ²)	End Capping
Synergi Max-RP	Spher. 2.5	100	—	400	17	—	TMS
Synergi Hydro-RP	Spher. 2.5	100	—	400	19	—	Hydrophilic
Synergi Polar-RP	Spher. 2.5	100	—	400	11	—	Hydrophilic
Synergi Fusion-RP	Spher. 2.5	100	—	400	12	—	TMS
Synergi Max-RP	Spher. 4, 10	80	1.05	475	17	3.21	TMS
Synergi Hydro-RP	Spher. 4, 10	80	1.05	475	19	2.45	Hydrophilic
Synergi Polar-RP	Spher. 4, 10	80	1.05	475	11	3.15	Hydrophilic
Synergi Fusion-RP	Spher. 4, 10	80	1.05	475	12	N/A	TMS

If Synergi analytical columns do not provide at least an equivalent separation as compared to a competing column of similar particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Synergi Polar-RP

An Ether-linked Phenyl Column with Polar Endcapping

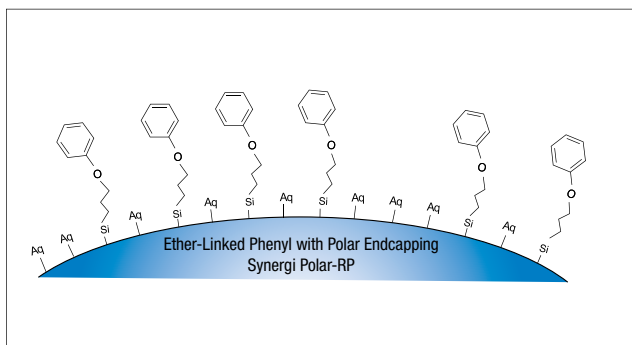

Synergi Polar-RP

USP: L11

pH Stability: 1.5 – 7.0

Particle Size: 2.5 μm, 4 μm, and 10 μm

Phase: Ether-linked phenyl with polar endcapping

Application: For extreme retention of polar and aromatic compounds

Strength: Improved peak shape for acidic and basic analytes and aromatic selectivity with methanol containing mobile phases


Sample Challenge:

You need greater separation between polar and aromatic compounds with only slight differences chemically or structurally.

Selectivity Solution:


The slightest variations in polarity and aromaticity are exploited by Synergi Polar-RP in order to achieve the greatest separation between polar and/or aromatic compounds.

Increased resolution of polar compounds with Synergi Polar-RP compared to traditional C18 phases

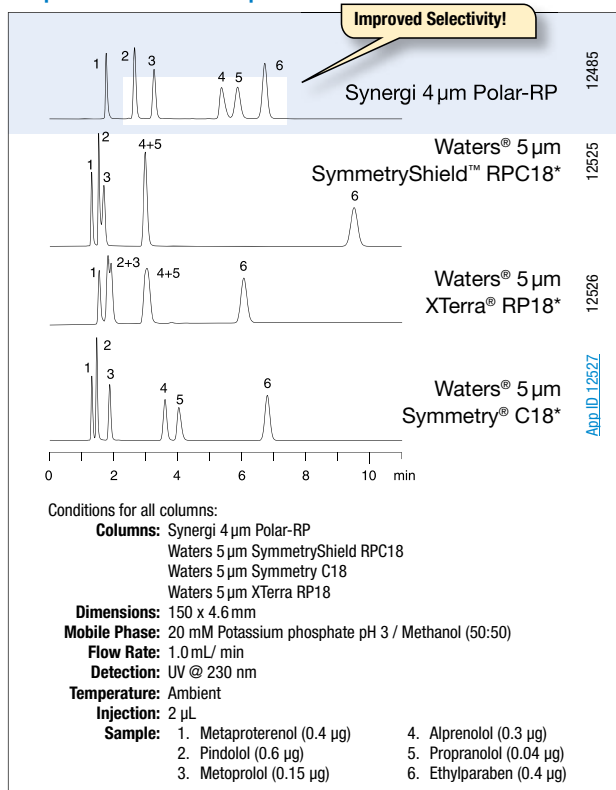


*See p. 342 for disclaimer information. Comparative separations may not be representative of all applications.

Improve peak symmetry of polar compounds with Synergi Polar-RP compared to other phenyl phases

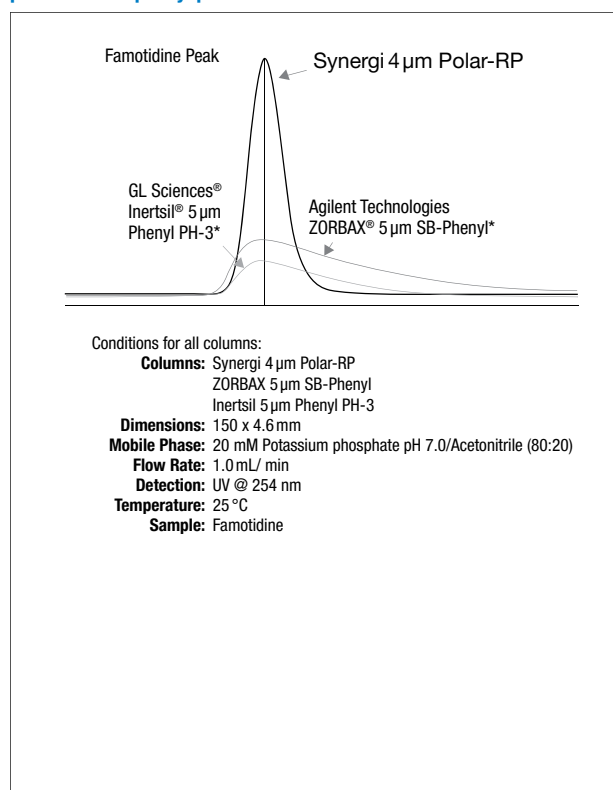

Synergi Polar-RP (cont'd)

Synergi Polar-RP is highly reproducible

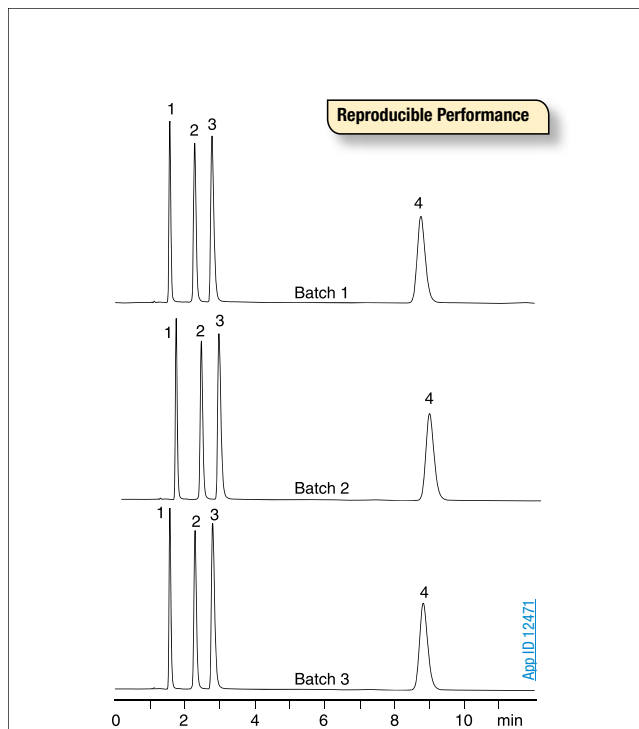

Conditions for all columns:

Column: Synergi 4 µm Polar-RP

Dimensions: 150 x 4.6 mm

Part No.: [00F-4336-E0](#)

Guard Cartridge: [AJ0-6076](#)

Guard Holder: [KJ0-4282](#)

Mobile Phase: Methanol/20 mM Potassium Phosphate pH 6.5 (35:65)

Flow Rate: 1.5 mL/min

Detection: UV @ 210 nm

Vial: [AR0-9925-13](#)


Filter: [AF0-8103-52](#)

Injection: 1 µL

Temperature: 22 °C

- Sample:**
1. Phenylephrine (1 µg)
 2. Phenylpropanolamine (1 µg)
 3. Pseudoephedrine (1 µg)
 4. Methylparaben (1 µg)

The selectivity of Synergi Polar-RP can provide differences in peak elution order for confirmation or better separation

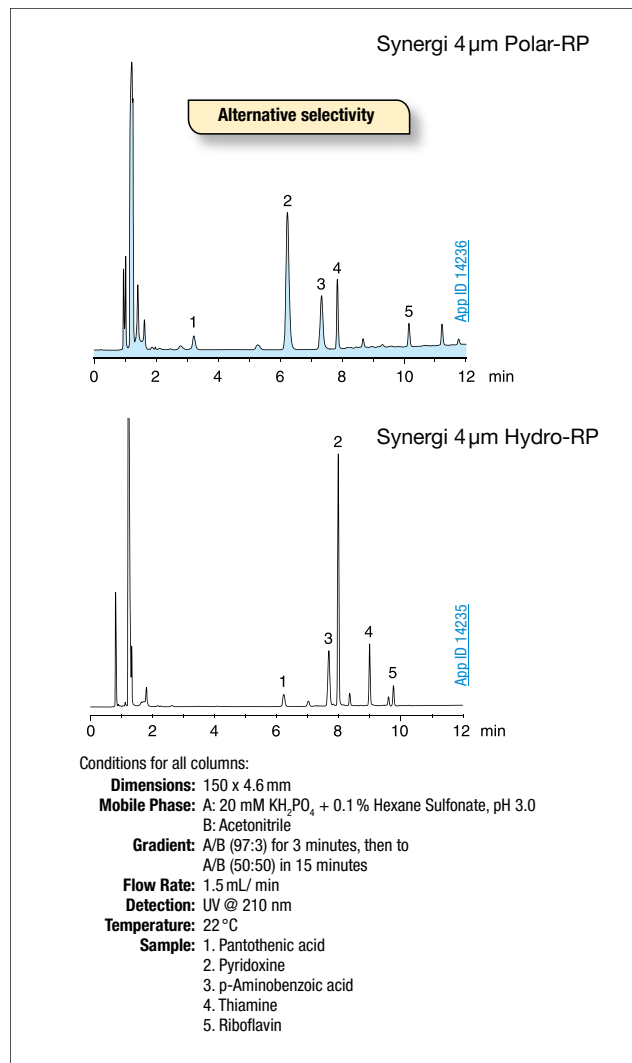

Conditions for all columns:

Dimensions: 150 x 4.6 mm

Mobile Phase: A: 20 mM KH_2PO_4 + 0.1% Hexane Sulfonate, pH 3.0

B: Acetonitrile

Gradient: A/B (97:3) for 3 minutes, then to

A/B (50:50) in 15 minutes


Flow Rate: 1.5 mL/min

Detection: UV @ 210 nm

Temperature: 22 °C

- Sample:**
1. Pantothenic acid
 2. Pyridoxine
 3. p-Aminobenzoic acid
 4. Thiamine
 5. Riboflavin

100% buffer mobile phase stability allows for separation of extremely polar compounds, like nucleic acid bases, on Synergi Polar-RP

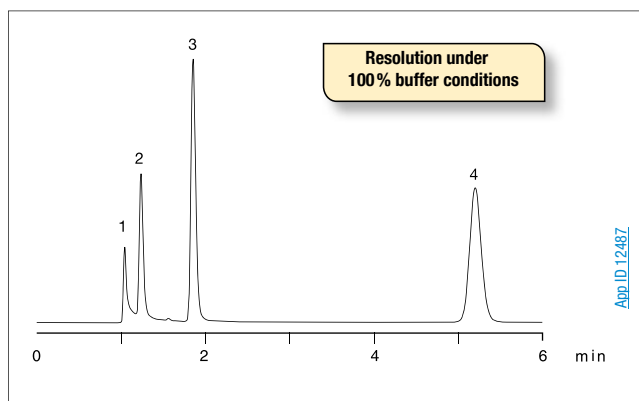

Nucleic Acid Bases

Column: Synergi 4 µm Polar-RP

Dimensions: 150 x 4.6 mm

Part No.: [00F-4336-E0](#)

Guard Cartridge: [AJ0-6076](#)

Guard Holder: [KJ0-4282](#)

Mobile Phase: 20 mM Potassium phosphate pH 2.7

Flow Rate: 2.0 mL/min

Detection: UV @ 254 nm

Vial: [AR0-9925-13](#)

Filter: [AF0-8103-52](#)


Injection: 2.5 µL

Temperature: 22 °C

- Sample:**
1. Thymidine triphosphate (TTP) (1.25 µg)
 2. Thymidine diphosphate (TDP) (1.25 µg)
 3. Thymidine monophosphate (TMP) (1.25 µg)
 4. Thymidine (1.25 µg)

If Synergi analytical columns do not provide at least an equivalent separation as compared to a competing column of similar particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Synergi Fusion-RP A Polar Embedded C18 Column

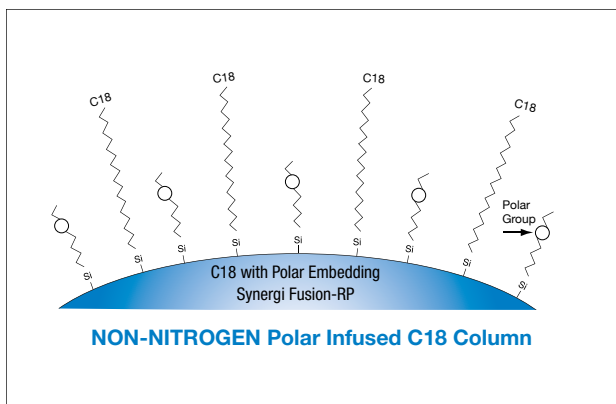

Synergi Fusion-RP

USP: L1

LC-MS
Certified

pH Stability: 1.5 – 9.0**

Particle Size: 2.5 µm, 4 µm, and 10 µm

Phase: Polar embedded C18

Application: For a balanced retention of polar, basic compounds and moderate retention of hydrophobics over a broad pH range

Strength: Analysis of polar, basic compounds with little or no MS phase bleed

** pH range is 1.5 - 10.0 under isocratic conditions.
pH range is 1.5 - 9 under gradient conditions.

Sample Challenge:


You need greater separation of compounds that exhibit moderately polar and hydrophobic characteristics.

Selectivity Solution:


Offering a balanced combination of hydrophobic and polar selectivity, Synergi Fusion-RP will allow you to separate compounds exhibiting polar and hydrophobic characteristics.

Balanced Polar and Hydrophobic Retention Allows for Superior Selectivity

Hydrophobic Basic Compounds

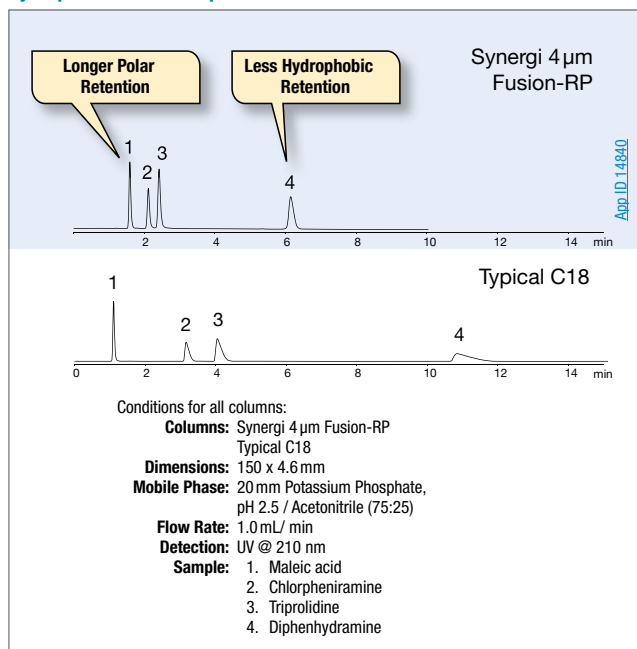


Antihistamines

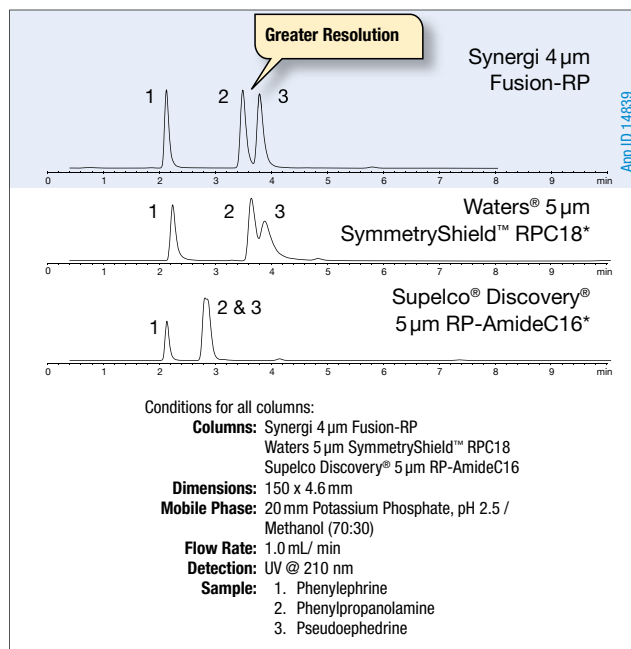


*See p. 342 for disclaimer information. Comparative separations may not be representative of all applications.

Synergi Fusion-RP (cont'd)


Synergi Fusion-RP has negligible MS bleed compared to other polar modified C18 columns

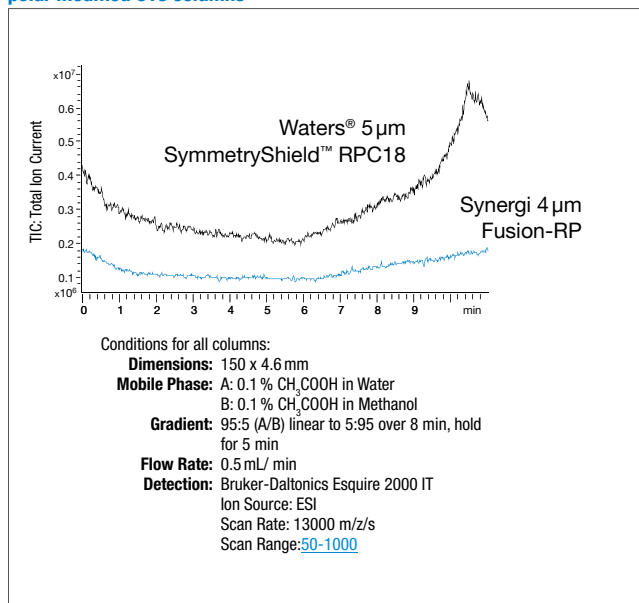

100% aqueous stable for added method flexibility

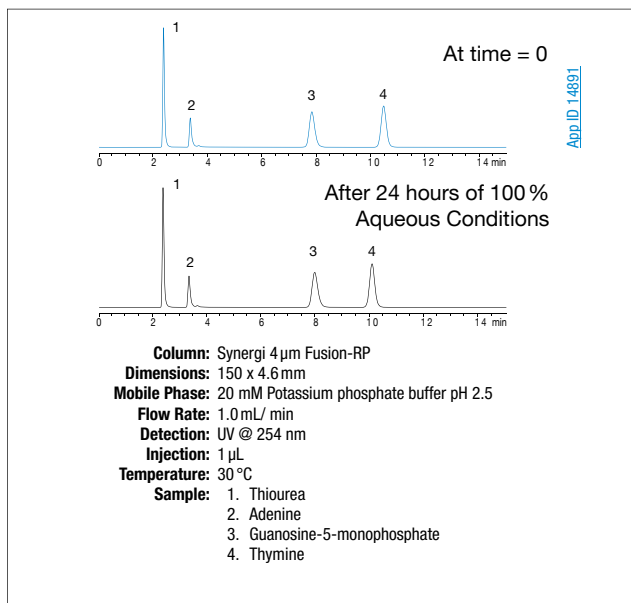

Excellent Multi-Compound Screening Ability

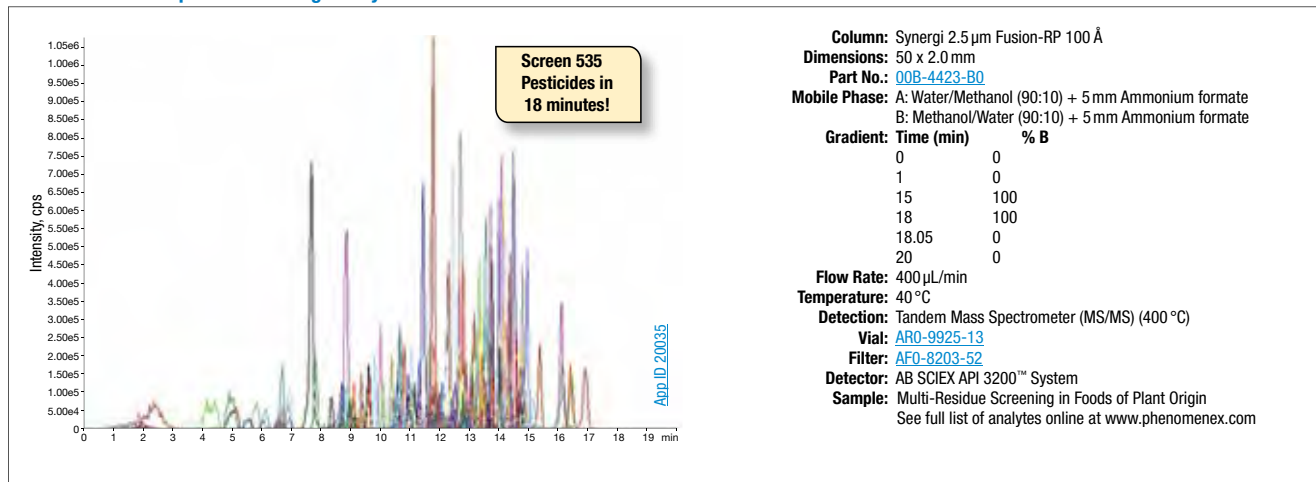


*Comparative separations may not be representative of all applications.

Columns used for comparison studies were manufactured by and purchased from Agilent Technologies Inc., Waters Corporation, GL Sciences Inc., Macherey-Nagel, and Sigma-Aldrich Co., LLC.



If Synergi analytical columns do not provide at least an equivalent separation as compared to a competing column of similar particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Synergi Hydro-RP A Polar Endcapped C18 Column

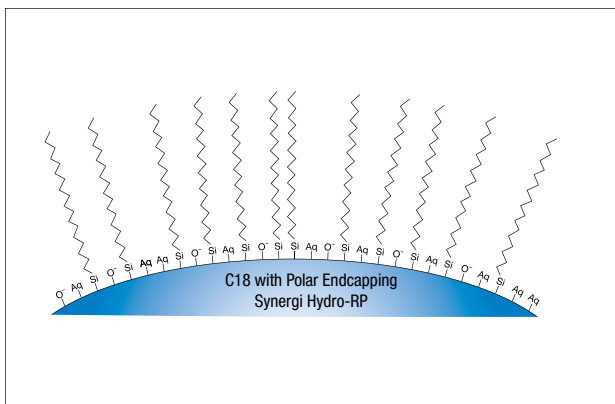

Sample Challenge:

Your sample contains multiple analytes with only slight variations in hydrophobicity.

Selectivity Solution:

The extreme hydrophobic selectivity offered by Synergi Hydro-RP is needed to amplify the small differences in selectivity and get greater separation.

Synergi Hydro-RP

USP: L1

pH Stability: 1.5 – 7.5


Particle Size: 2.5 μm, 4 μm, and 10 μm

Phase: C18 with polar endcapping

Application: For extreme retention of non-polar and extremely polar alkyl compounds

Strength: Resolution of highly polar compounds under 100% buffer mobile phase conditions


Extreme hydrophobic retention relative to other hydrophobic selectivity phases

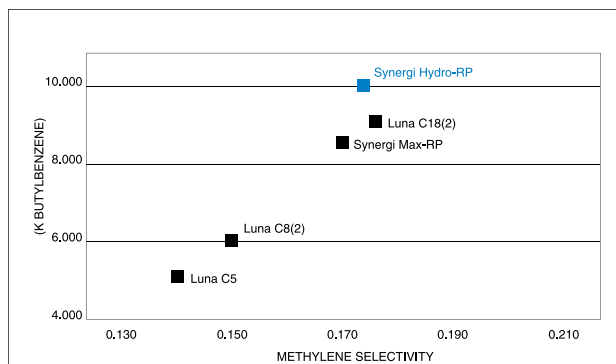

Conditions for all columns:
Dimensions: 150 x 4.6 mm
Mobile Phase: Acetonitrile/20 mM Potassium phosphate pH 7.0 (65:35)
Flow Rate: 1.5 mL/min
Temperature: Ambient
Sample: 1. Butylbenzene
 2. Amylbenzene


The chart was obtained by plotting hydrophobic retention (k for butylbenzene vs. methylene selectivity (log k for amylbenzene vs the number of methyl groups) under the stated conditions. A column with high hydrophobicity will better resolve two analytes which subtly differ in their overall hydrophobicity than a column with lower hydrophobic selectivity.

Additional polar selectivity provides separation where traditional C18 columns cannot

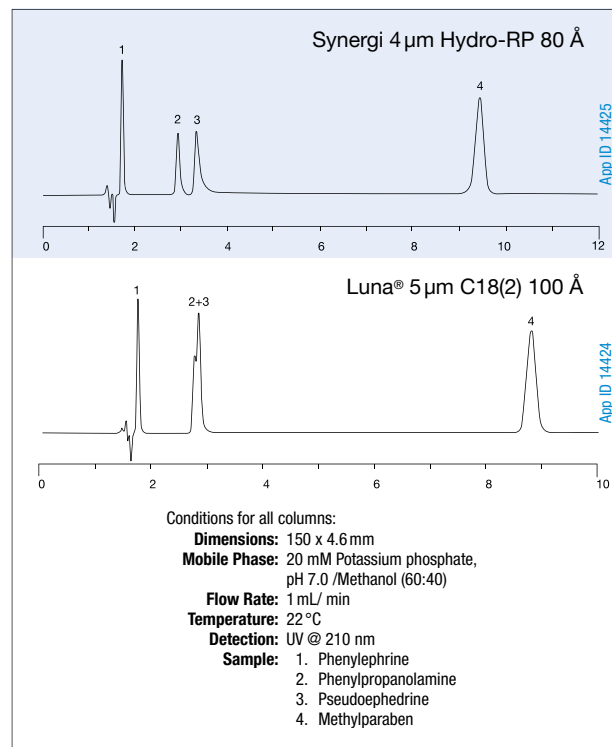


Synergi Hydro-RP (cont'd)

Synergi Hydro-RP is stable in 100% aqueous mobile phase, providing improved retention of extremely polar compounds

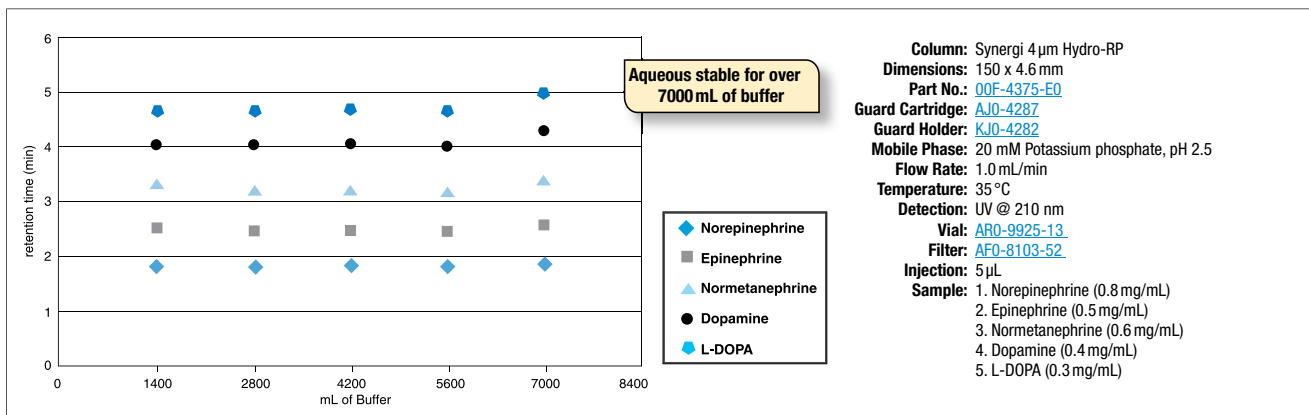


Synergi Hydro-RP is able to separate very polar compounds, as well as, mixtures of polars and non-polars

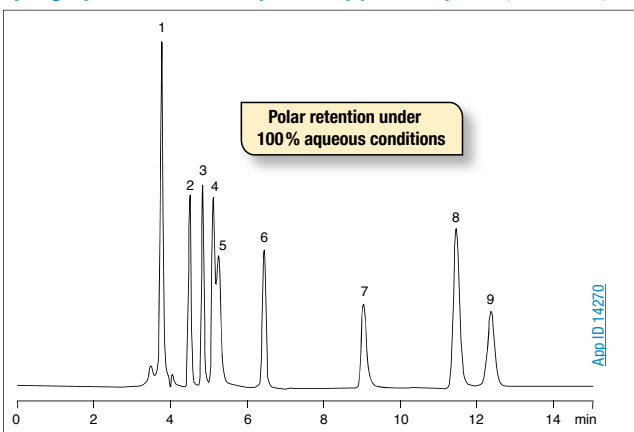

Organic Acids

Column: Synergi 4 µm Hydro-RP
Dimensions: 250 x 4.6 mm
Part No.: [00G-4375-E0](#)
Guard Cartridge: [AJ0-4287](#)
Guard Holder: [KJ0-4282](#)
Mobile Phase: 20 mM Potassium phosphate, pH 2.9
Flow Rate: 0.7 mL/min
Temperature: 22 °C
Detection: UV @ 220 nm
Vial: [AR0-9925-13](#)
Filter: [AF0-8103-52](#)
Sample: 1. Oxalic acid
 2. Tartaric acid
 3. Glycolic acid
 4. Formic acid
 5. Pyruvic acid
 6. Malonic acid
 7. Acetic acid
 8. Maleic acid
 9. Citric acid

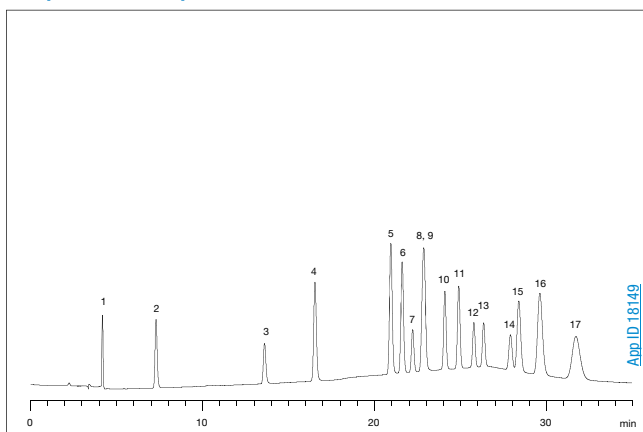

Explosives

Column: Synergi 4 µm Hydro-RP
Dimensions: 250 x 4.6 mm
Part No.: [00G-4375-E0](#)
Mobile Phase: A: Methanol
 B: Water
Gradient:


Time (min)	% B
0	45
2	45
22	25
22.01	45
25	45

Flow Rate: 1 mL/min
Temperature: 22 °C
Detection: UV @ 254 nm / 220 nm (ambient)
Sample: 1. Octahydro-1,3,5,7-tetranitro-1,3,5,7-tetrazocine (HMX)
 2. Hexahydro-1,3,5-trinitro-1,3,5-triazine (RDX)
 3. 1,3,5-Trinitrobenzene
 4. Methyl-2,4,6-trinitrophenylnitramine (Tetryl)
 5. 1,3-Dinitrobenzene
 6. Nitrobenzene
 7. Nitroglycerin
 8. 2,4,6-Trinitrotoluene (TNT)
 9. 3,5-Dinitroaniline
 10. 4-Amino-2,6 dinitrotoluene
 11. 2-Amino-4,6 dinitrotoluene
 12. 2,6-Dinitrotoluene
 13. 2,4-Dinitrotoluene
 14. Pentaerythritol tetranitrate (PETN)
 15. 2-Nitrotoluene
 16. 4-Nitrotoluene
 17. 3-Nitrotoluene



If Synergi analytical columns do not provide at least an equivalent separation as compared to a competing column of similar particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Synergi Max-RP A Reversed Phase C12 Column

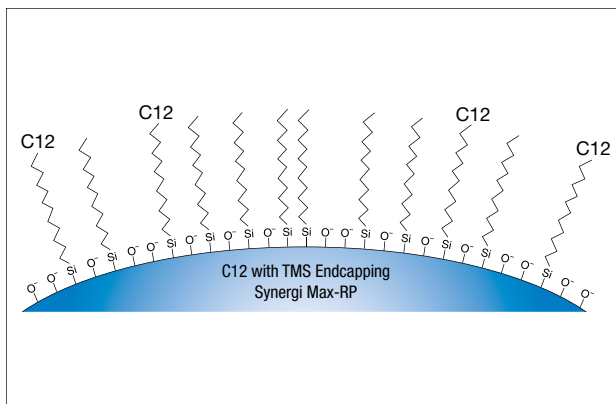

Synergi Max-RP

USP: L87

LC-MS
Certified

pH Stability: 1.5 – 9.0**

Particle Size: 2.5 μm, 4 μm, and 10 μm

Phase: Reversed phase C12

Application: For hydrophobic, non-polar compounds over a wide pH range, with little or no MS phase bleed

Strength: Sharp peak shape for basic compounds at neutral pH

**pH range is 1.5 - 10.0 under isocratic conditions.
pH range is 1.5 - 9 under gradient conditions.


Sample Challenge:

You need to retain compounds based on hydrophobic selectivity exclusively, but cannot accomplish peak separation with C18 column.

Selectivity Solution:

The C12 ligands on Synergi Max-RP give a hydrophobic selectivity that may separate peaks where C18 columns cannot.

Hydrophobic Retention: Synergi Max-RP (C12) Performs Like a C18*

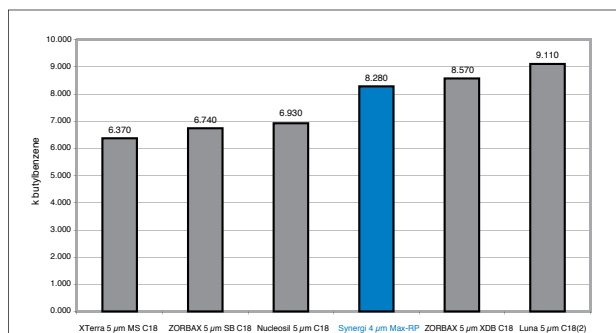

Conditions for all columns:

Columns: Waters XTerra 5 μm MS C18
Agilent Technologies ZORBAX 5 μm SB C18
Macherey Nagel Nucleosil 5 μm C18
Synergi 4 μm Max-RP
Agilent Technologies ZORBAX 5 μm XDB C18
Luna 5 μm C18(2)

Dimensions: 150 x 4.6 mm

Mobile Phase: Acetonitrile/Water (80:20)

Flow Rate: 1 mL/min


Detection: UV @ 254 nm

Injection: 1 μL

Temperature: Ambient

Sample: Butylbenzene

Silanol Activity at Low pH: C12 vs. C18 Phases

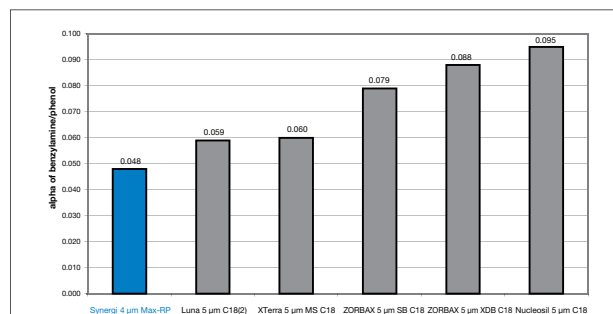

Conditions for all columns:

Columns: Waters XTerra 5 μm MS C18
Agilent Technologies ZORBAX 5 μm SB C18
Macherey Nagel Nucleosil 5 μm C18
Synergi 4 μm Max-RP
Agilent Technologies ZORBAX 5 μm XDB C18
Luna 5 μm C18(2)

Dimensions: 150 x 4.6 mm

Mobile Phase: Methanol/20 mM Potassium phosphate, pH 2.5 (30:70)

Flow Rate: 1 mL/min

Detection: UV @ 254 nm

Injection: 5 μL

Temperature: Ambient



Sample: 1. Benzylamine
2. Phenol

*See p. 342 for disclaimer information. Comparative separations may not be representative of all applications.

Synergi Max-RP (cont'd)

Sharper Peaks


The Synergi Max-RP C12 ligands are densely bound to silica surface, significantly decreasing the number of active silanol groups, which cause peak tailing

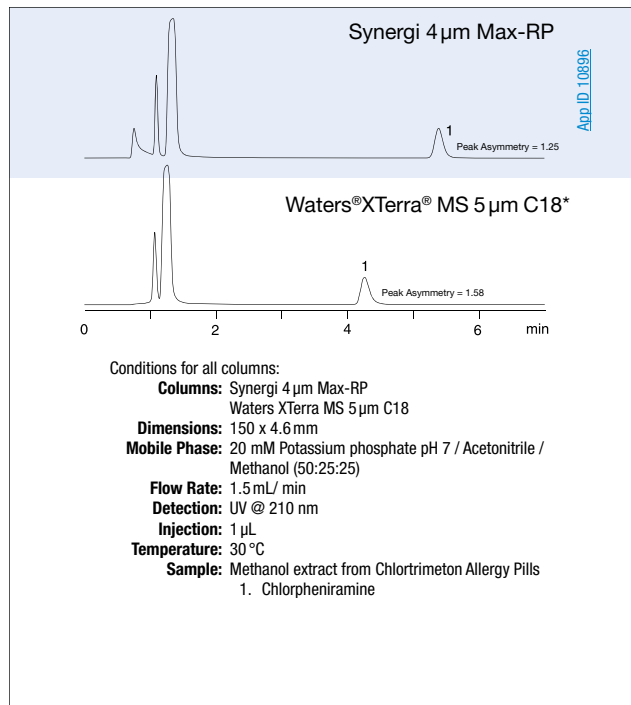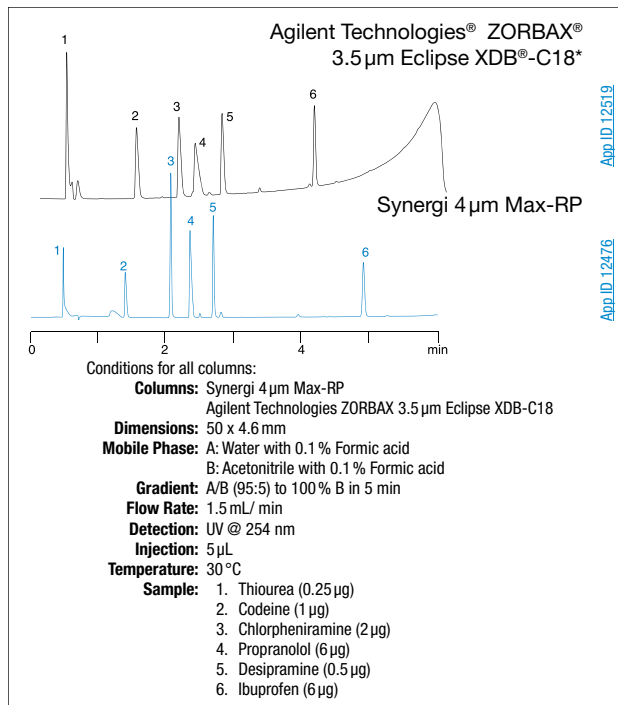


*See p. 342 for disclaimer information. Comparative separations may not be representative of all applications.

Achieve Reproducibility and Long Column Lifetimes Even at pH Extremes with Synergi Max-RP

Stability @ pH 1.5

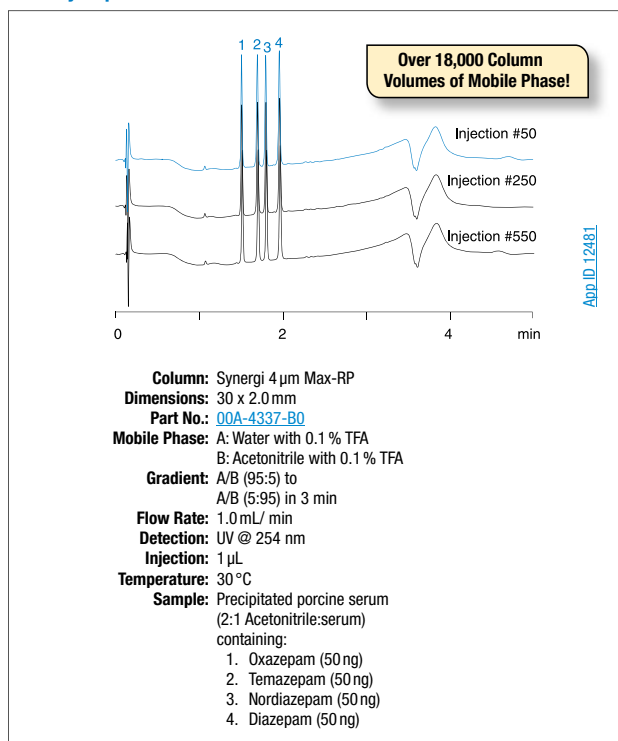

Stability @ pH 10.0

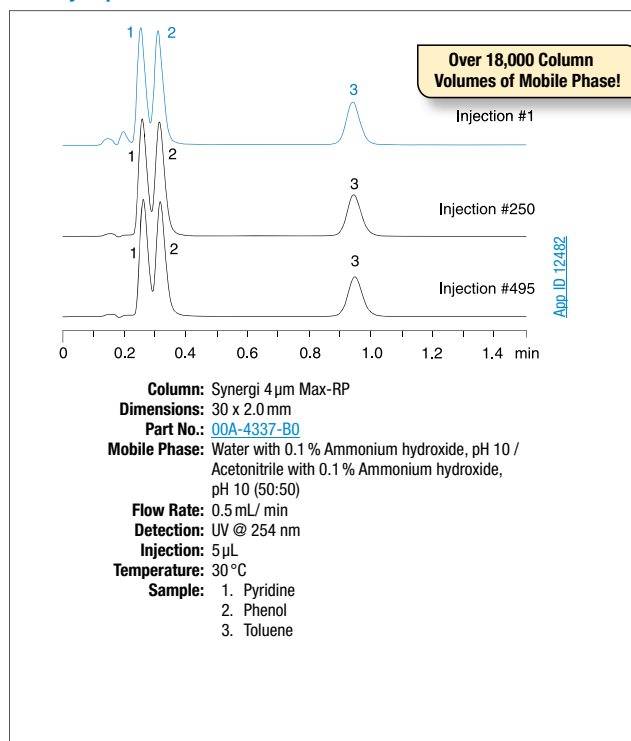

If Synergi analytical columns do not provide at least an equivalent separation as compared to a competing column of similar particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Fast LC Solutions

Ordering Information

2.5 µm High Speed Technology (HST) Columns (mm)						
Phases	30 x 2.0	50 x 2.0	100 x 2.0	50 x 3.0	100 x 3.0	50 x 4.6
Max-RP	00A-4372-B0	00B-4372-B0	00D-4372-B0	00B-4372-Y0	00D-4372-Y0	00B-4372-E0
Hydro-RP	00A-4387-B0	00B-4387-B0	00D-4387-B0	00B-4387-Y0	00D-4387-Y0	00B-4387-E0
Polar-RP	00A-4371-B0	00B-4371-B0	00D-4371-B0	00B-4371-Y0	00D-4371-Y0	00B-4371-E0
Fusion-RP	00A-4423-B0	00B-4423-B0	00D-4423-B0	00B-4423-Y0	00D-4423-Y0	00B-4423-E0



For information about HST Columns, contact your Phenomenex technical consultant or local distributor.

Ordering Information

2.5 µm MercuryMS LC-MS Cartridges (mm)					Columns (mm)	
Phases	10 x 2.0	10 x 4.0	20 x 2.0	20 x 4.0	20 x 2.0	20 x 4.0
Max-RP	00N-4372-B0-CE	—	00M-4372-B0-CE	00M-4372-D0-CE	—	—
Hydro-RP	00N-4387-B0-CE	00N-4387-D0-CE	00M-4387-B0-CE	—	—	—
Polar-RP	00N-4371-B0-CE	00N-4371-D0-CE	00M-4371-B0-CE	—	00M-4377-B0	—
Fusion-RP	00N-4423-B0-CE	—	00M-4423-B0-CE	00M-4423-D0-CE	00M-4423-B0	00M-4423-D0

MercuryMS™ Cartridge Holders



Direct-Connect Holder



Standard Holder

Ordering Information

Direct-Connect Cartridge Holders

Part No.	Description
CHO-7187	10 mm direct-connect holder
CHO-7188	20 mm direct-connect holder

Standard Cartridge Holders

Part No.	Description
CHO-5846	10 mm standard holder
CHO-5845	20 mm standard holder

Capillary Columns

Ordering Information

4 µm Synergi Capillary Columns (mm)					Guard Columns (mm)
Phases	50 x 0.30	150 x 0.30	150 x 0.50	250 x 0.50	20 x 0.30
Max-RP	00B-4337-AC	—	—	—	03M-4337-AC
Hydro-RP	00B-4375-AC	00F-4375-AC	—	00G-4375-AF	03M-4375-AC
Fusion-RP	00B-4424-AC	00F-4424-AC	00F-4424-AF	—	03M-4424-AC

If Synergi analytical columns do not provide at least an equivalent separation as compared to a competing column of similar particle size, similar phase and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

HPLC Columns

Ordering Information

4 µm Microbore and Minibore Columns (mm)								SecurityGuard™ Cartridges (mm)
Phases	50 x 1.0	150 x 1.0	30 x 2.0	50 x 2.0	75 x 2.0	150 x 2.0	250 x 2.0	4 x 2.0* /10pk
Max-RP	00B-4337-AO	00F-4337-AO	00A-4337-BO	00B-4337-BO	00C-4337-BO	00F-4337-BO	00G-4337-BO	AJO-6073
Hydro-RP	00B-4375-AO	00F-4375-AO	00A-4375-BO	00B-4375-BO	00C-4375-BO	00F-4375-BO	00G-4375-BO	AJO-7510
Polar-RP	00B-4336-AO	00F-4336-AO	00A-4336-BO	00B-4336-BO	00C-4336-BO	00F-4336-BO	00G-4336-BO	AJO-6075
Fusion-RP	00B-4424-AO	00F-4424-AO	00A-4424-BO	00B-4424-BO	00C-4424-BO	00F-4424-BO	00G-4424-BO	AJO-7556

for ID: 2.0-3.0 mm

4 µm MidBore™ Columns (mm)					SecurityGuard™ Cartridges (mm)
Phases	30 x 3.0	50 x 3.0	150 x 3.0	250 x 3.0	4 x 2.0* /10pk
Max-RP	—	00B-4337-YO	00F-4337-YO	00G-4337-YO	AJO-6073
Hydro-RP	—	00B-4375-YO	00F-4375-YO	00G-4375-YO	AJO-7510
Polar-RP	00A-4336-YO	00B-4336-YO	00F-4336-YO	00G-4336-YO	AJO-6075
Fusion-RP	—	00B-4424-YO	00F-4424-YO	00G-4424-YO	AJO-7556

for ID: 2.0-3.0 mm

4 µm Analytical Columns (mm)						SecurityGuard™ Cartridges (mm)
Phases	30 x 4.6	50 x 4.6	75 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0* /10pk
Max-RP	00A-4337-E0	00B-4337-E0	00C-4337-E0	00F-4337-E0	00G-4337-E0	AJO-6074
Hydro-RP	00A-4375-E0	00B-4375-E0	00C-4375-E0	00F-4375-E0	00G-4375-E0	AJO-7511
Polar-RP	00A-4336-E0	00B-4336-E0	00C-4336-E0	00F-4336-E0	00G-4336-E0	AJO-6076
Fusion-RP	—	00B-4424-E0	00C-4424-E0	00F-4424-E0	00G-4424-E0	AJO-7557

for ID: 3.2-8.0 mm

Preparative Columns

Ordering Information

Axia™ Packed Preparative Columns (mm)					SecurityGuard™ Cartridges (mm)
Phases	50 x 21.2	100 x 21.2	150 x 21.2	250 x 21.2	15 x 21.2**
4 µm					
Max-RP	—	—	00F-4337-PO-AX	00G-4337-PO-AX	AJO-7842
Hydro-RP	00B-4375-PO-AX	—	00F-4375-PO-AX	00G-4375-PO-AX	AJO-7843
Polar-RP	00B-4336-PO-AX	00D-4336-PO-AX	00F-4336-PO-AX	00G-4336-PO-AX	AJO-7845
Fusion-RP	—	00D-4424-PO-AX	00F-4424-PO-AX	00G-4424-PO-AX	AJO-7844
10 µm					
Hydro-RP	—	—	Inquire	00G-4376-PO-AX	AJO-7843
Polar-RP	—	—	Inquire	00G-4351-PO-AX	AJO-7845
Fusion-RP	—	—	00F-4425-PO-AX	00G-4425-PO-AX	AJO-7844

for ID: 18-29 mm

Ordering Information

Axia™ Packed Preparative Columns (mm) continued		SecurityGuard™ Cartridges (mm)
Phases	250 x 30	15 x 30.0*
4 µm		
Max-RP	00G-4337-UO-AX	AJO-8304

for ID: 30-49 mm

Ordering Information

4 µm Semi-Prep Columns (mm)		SecurityGuard™ Cartridges (mm)
Phases	250 x 10	10 x 10†
4 µm		
Max-RP	00G-4337-NO	AJO-7275
Hydro-RP	00G-4375-NO	AJO-7512
Polar-RP	00G-4336-NO	AJO-7276
Fusion-RP	00G-4424-NO	AJO-7558

for ID: 9-16 mm

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJO-4282](#)

†SemiPrep SecurityGuard™ Cartridges require holder, Part No.: [AJO-9281](#)

**PREP SecurityGuard™ Cartridges require holder, Part No.: [AJO-8223](#)

*PREP SecurityGuard™ Cartridges require holder, Part No.: [AJO-8277](#)



For more dimensions and phases of Axia packed preparative columns, see pp. 381-382, or contact your Phenomenex Technical Consultant

Pilot Scale Columns and Bulk Material

Ordering Information

10 µm Analytical and Semi-Prep Columns (mm)				SecurityGuard™ Cartridges (mm)
Phases	250 x 4.6	250 x 10	4 x 3.0*	10 x 10†
10 µm				
Hydro-RP	00G-4376-E0	00G-4376-NO	AJO-7511	AJO-7512
Polar-RP	00G-4351-E0	00G-4351-NO	AJO-6076	AJO-7276
Fusion-RP	00G-4425-E0	00G-4425-NO	AJO-7557	AJO-7558

for ID: 3.2-8.0 mm 9-16 mm

10 µm Bulk Packings

Phases	100 g	1 kg
Max-RP	04G-4350	04K-4350
Hydro-RP	04G-4376	04K-4376
Polar-RP	04G-4351	04K-4351
Fusion-RP	04G-4425	04K-4425

Larger quantities of bulk media available upon request.

Synergi Bulk Media

Beyond our largest preparative column dimensions, Synergi phases are available in bulk quantities for HPLC purification at the process, pilot, and commercial scale. These medias offer a complementary selectivity to the standard C18, C8, or Silica phases traditionally employed in larger scale HPLC. Additionally, due to the diverse chemical properties of each of the Synergi phases, dramatic differences in chromatographic parameters such as retention time, selectivity, and resolution are often observed. For those challenging purifications where chromatography still makes the most sense, the Synergi family offers an excellent alternative to evaluate! Get your Synergi preparative scout column(s) and evaluate these phases today!



Ultracarb™

- Excellent peak shape for basic compounds, free fatty acids, triglycerides, fat-soluble vitamins, and other lipophilic compounds

Ultracarb C8 offers a high carbon load material with somewhat different selectivity than the two Ultracarb ODS phases.

Ordering Information

Minibore and MidBore™ Columns (mm)		SecurityGuard™ Cartridges (mm)
Phases	150 x 2.0	4 x 2.0
		/10pk
5 µm ODS (30)	00F-0351-B0	AJ0-4286 for ID: 2.0-3.0 mm

Analytical Columns (mm)					SecurityGuard™ Cartridges (mm)
Phases	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	4 x 3.0
					/10pk
3 µm ODS (20)	00B-0205-E0	00D-0205-E0	00F-0205-E0	—	AJ0-4287
5 µm C8	—	—	00F-2134-E0	00G-2134-E0	AJ0-4290
5 µm ODS (20)	—	—	00F-0206-E0	00G-0206-E0	AJ0-4287
5 µm ODS (30)	—	00D-0351-E0	00F-0351-E0	00G-0351-E0*	AJ0-4287

for ID: 3.2-8.0 mm



*IMPORTANT: Phenomenex highly recommends the use of 150 mm column length, as opposed to the “traditional” 250 mm column length, when the 5 µm ODS (30) phase is desired. In those cases when the additional retention and resolution of a 250 mm column is desired, please be aware that column backpressure with Ultracarb 5 µm ODS (30) can be 50 to 100 % higher than that experienced with “standard” ODS columns. This relatively high backpressure is a function of the hydrophobicity of the 5 µm ODS (30) phase; higher backpressure is completely “natural” with this phase and will have no ill consequence for the column.

SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)

Ultremex™

- For all new methods we recommend Luna columns
- Spherical, silica material

Ordering Information

5 µm Analytical Columns (mm)			SecurityGuard™ Cartridges (mm)
Phases	150 x 4.6	250 x 4.6	4 x 3.0
			/10pk
C8	00F-0047-E0	00G-0047-E0	AJ0-4290
C18	00F-0048-E0	00G-0048-E0	AJ0-4287

for ID: 3.2-8.0 mm

SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)

Ultron® ES

Manufactured by Shinwa Chemical Industries, Ltd.

- Two complementary protein-based chiral stationary phases
- Easy to use with reversed-phase mobile phases
- Racemic separation without derivatization
- pH range from 3.0 to 7.5

Ordering Information

Column	µm	Size (mm)	ES-OVM
Analytical	5	150 x 4.6	702111651
Analytical & Guard	5	150 x 4.6	702111651A



Protect your valuable column investment with the disposable KrudKatcher™ pre-column filter, see p. 17
For In-line Filters specifically designed to protect your chiral column investment, see p. 17



For Chiral Column Performance Check Standards, see p. 415



For HPLC Column Heater System (25-90 °C), see p. 408

If Yarra analytical columns do not provide you with at least an equivalent separation as any other GFC column of similar porosity, type, and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Affordable, Ultra-High Resolution Size Exclusion Chromatography for HPLC/UHPLC Systems

- Save money with extremely affordable prices
- Achieve better results through larger exclusion ranges and higher efficiencies
- Enhance recovery using more inert Yarra particles and Bio-Inert hardware
- Gain time with faster, more productive HPLC/UHPLC runs
- Feel at ease knowing you have an unmatched product guarantee


Minimize Adsorption with Bio-Inert Hardware!

Yarra vs. Waters® BEH SEC

Yarra 1.8 µm 150 x 4.6 mm		vs.	Waters 1.7 µm 150 x 4.6 mm	
			BEH125 SEC	BEH200 SEC
1.8	1.8	Particle Size (µm)	1.7	1.7
150	300	Pore Size (Å)	125	200
1K - 450 K	10K-700K	MW Range in native conditions (Da)	1 K - 80 K	10K - 450 K
>30,000	>30,000	Efficiency (plates/column)	>30,000	>30,000

*Waters specifications taken from Waters website.


Better Recovery with Greater Inertness

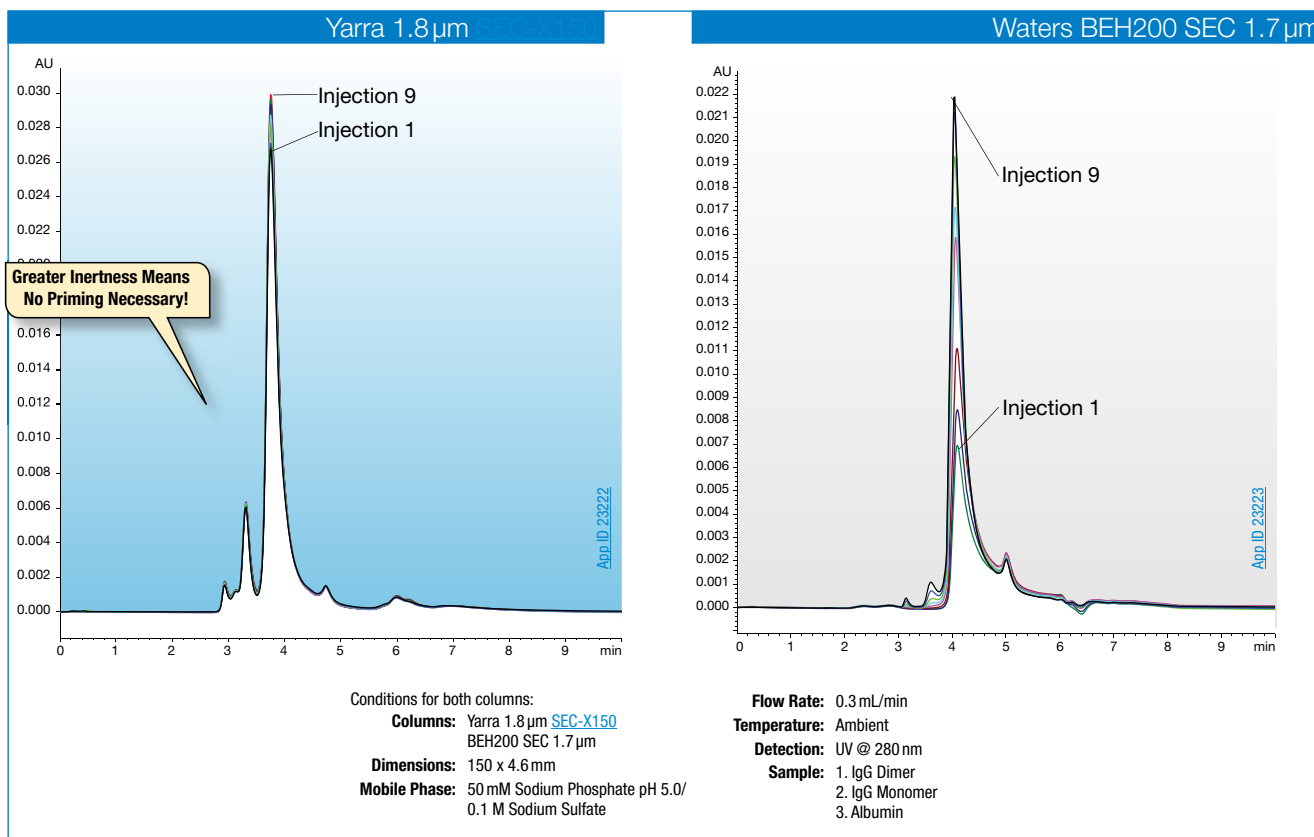

Comparative separations may not be representative of all applications.


Exceptional Separation Power—Low MW

Degraded Human Insulin

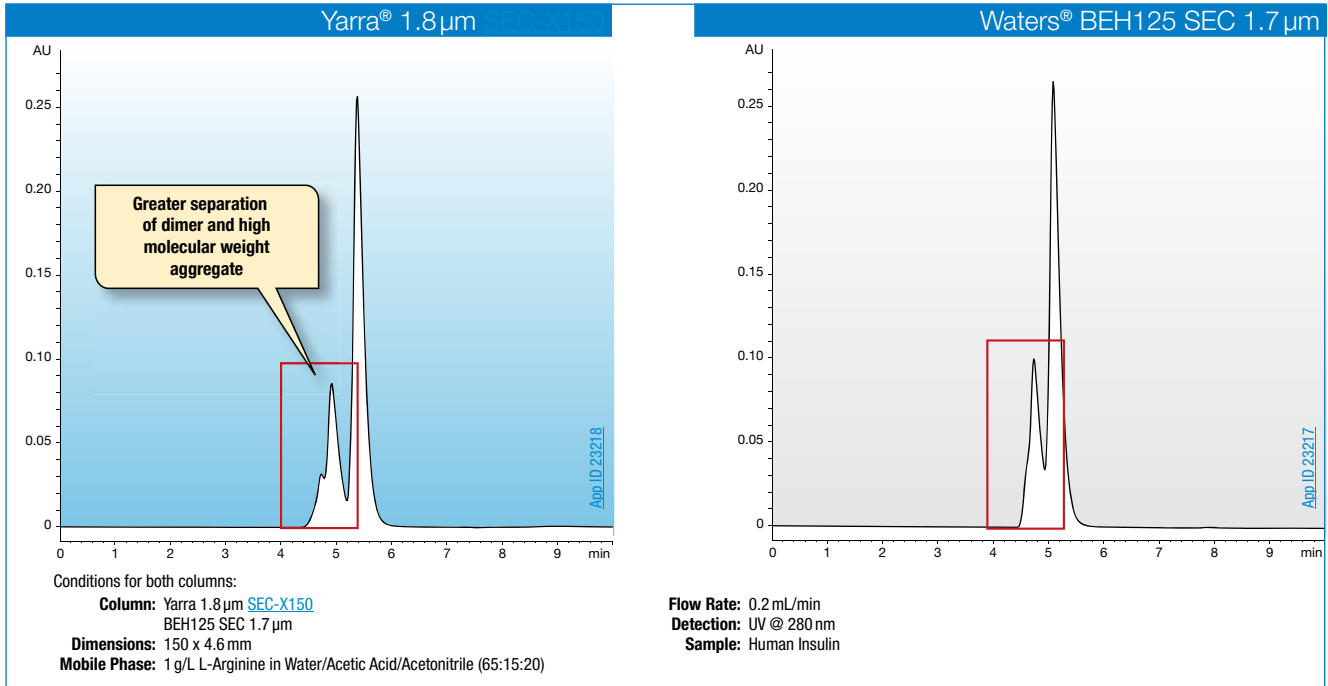

Comparative separations may not be representative of all applications.

Expanded Resolution of Recombinant Human Insulin

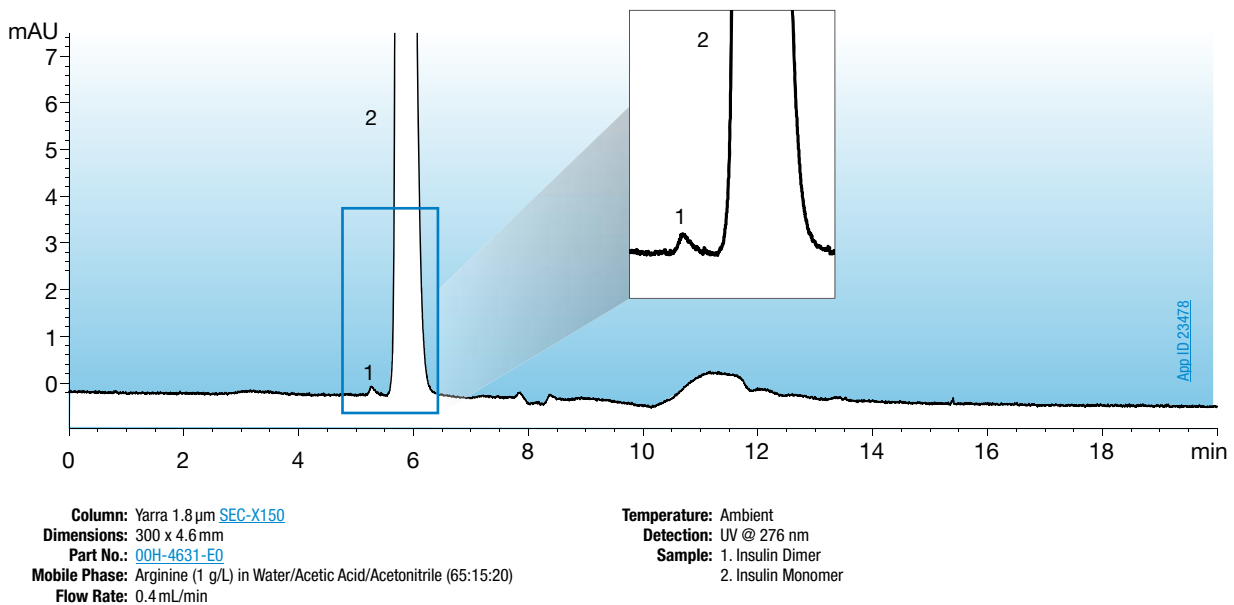


Yarra™ 1.8 μm Aqueous GFC/SEC Columns

Exceptional Separation Power—High MW

The large separation range of the Yarra [SEC-X300](#) makes it good for high molecular weight aggregation studies of monoclonal antibodies. While the smaller MW focus of the [SEC-X150](#) allows for excellent identification and separation of a mAb and its variable region fragments.

Mouse mAb (monoclonal antibody)

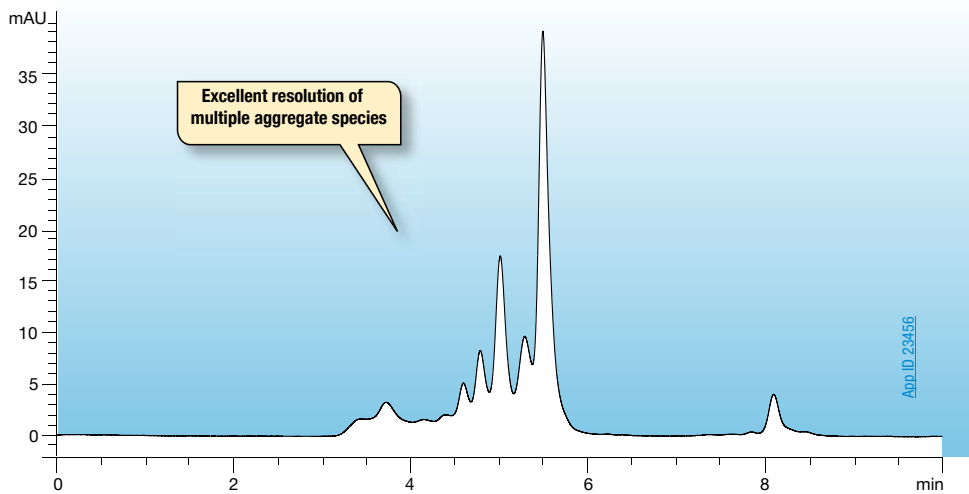

Column: Yarra 1.8 μm [SEC-X300](#)

Dimensions: 150 x 4.6 mm

Part No.: [00F-4743-E0](#)

Mobile Phase: 0.1 M Sodium Phosphate in Water (pH 6.8)

Flow Rate: 0.35 mL/min

Temperature: Ambient

Detection: UV @ 280 nm

Sample: Mouse Monoclonal Antibody

Fast GFC/SEC Methods on your HPLC or UHPLC

Utilize the high performance of the new Yarra 1.8 μm [SEC-X150](#) on the system(s) that you know and are comfortable with! The amazing separation power of the Yarra 1.8 μm [SEC-X150](#) can easily be utilized on any HPLC and UHPLC system.

PROTEINS/PEPTIDES | YARRA | HPLC/UHPLC



Shimadzu® Nexera®



Waters® ACQUITY® UPLC®



Agilent® 1200



Questions About LC System Compatibility?
Contact your local Phenomenex representative for guidance!

Yarra™ 1.8 μm Aqueous GFC/SEC Columns


guarantee

If Yarra analytical columns do not provide you with at least an equivalent separation as any other GFC column of similar porosity, type, and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Excellent Stability and Lifetime


The great care exhibited in both engineering and packing of Yarra columns can produce stable performance over longer lifetimes than other size exclusion columns on the market. By gaining extended lifetime with Yarra columns, you save significant time and money for your lab.

Increased Lifetime Under Extreme Conditions (10% IPA and higher flow rate)

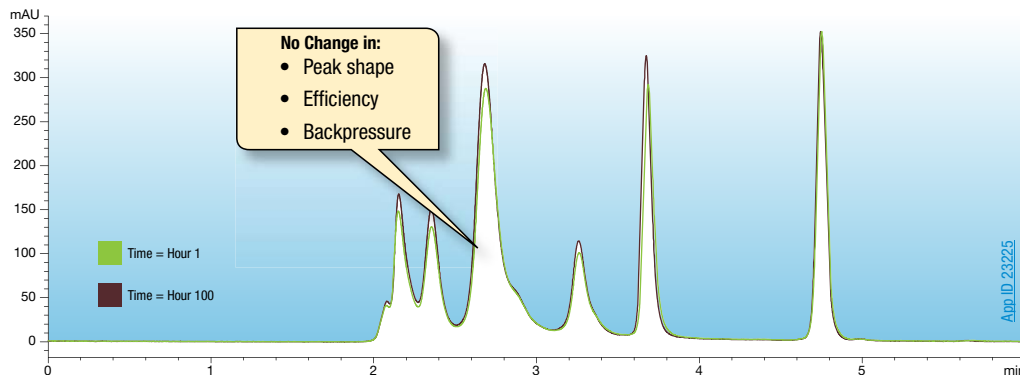

Column: Yarra 1.8 μm [SEC-X150](#)
Dimension: 150 x 4.6 mm
Part No.: [00F-4631-E0](#)
Mobile Phase: 100 mM Sodium Phosphate in Water pH 6.8 + 0.025% NaN₃ + **10% IPA**
Flow Rate: **0.4 mL/min**
Temperature: Ambient
Detection: UV @ 280 nm
Sample: 1. Thyroglobulin (669 kDa)
 2. IgA (300 kDa)
 3. IgG (150 kDa)
 4. Ovalbumin (44 kDa)
 5. Myoglobin (17 kDa)
 6. Uridine

Molecular Weight (MW) Separation Ranges

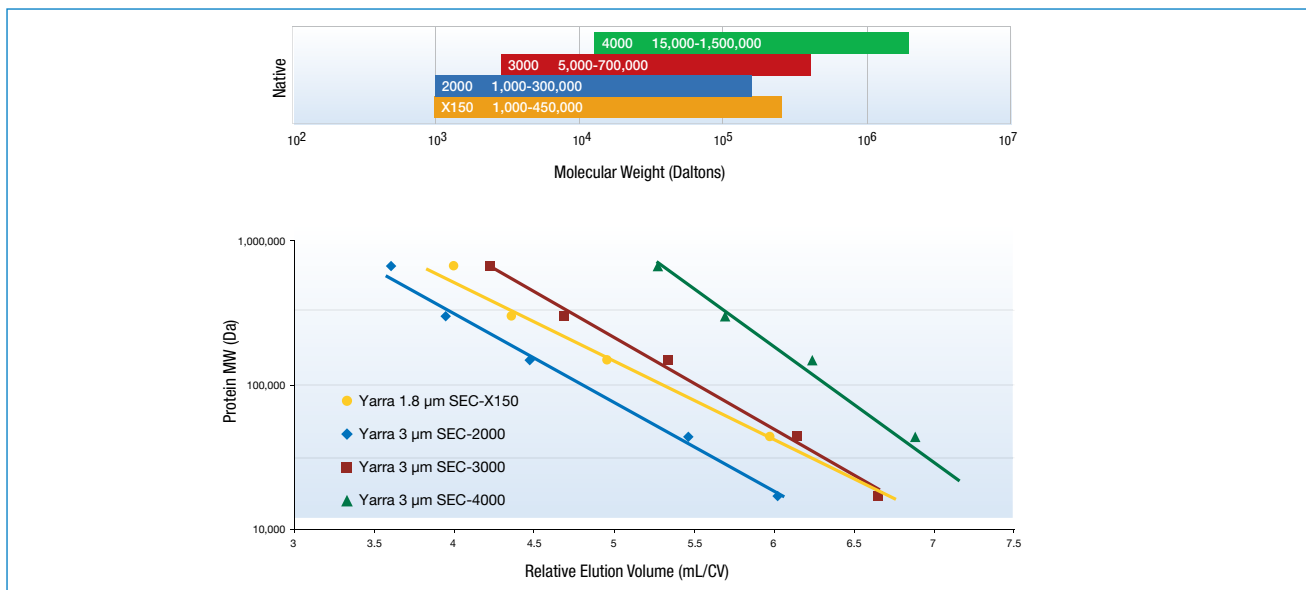

Bio-Inert Hardware

In addition to a highly inert particle chemistry, Yarra 1.8 μm [SEC-X150](#) and [SEC-X300](#) columns utilize a Bio-Inert hardware to further ensure accurate recoveries.

Ordering Information

Yarra 1.8 μm SEC Bio-Inert Columns (mm)		
Phases	150 x 4.6	300 x 4.6
Yarra 1.8 μm SEC-X150	00F-4631-E0	00H-4631-E0
Yarra 1.8 μm SEC-X300	00F-4743-E0	00H-4743-E0

Yarra 1.8 μm SEC Stainless Steel Columns (mm)			SecurityGuard ULTRA Cartridges***
Phases	150 x 4.6	300 x 4.6	3/pk
Yarra 1.8 μm SEC-X150	00F-4631-E0-SS	00H-4631-E0-SS	AJ0-9512
Yarra 1.8 μm SEC-X300	00F-4743-E0-SS	00H-4743-E0-SS	AJ0-9513

For Stainless Steel Only

***SecurityGuard ULTRA cartridges require holder, Part No.: [AJ0-9000](#)


Bio-Inert Hardware

Yarra® 1.8 μm



Conventional Hardware

Waters® BEH200 SEC 1.7 μm



If Yarra analytical columns do not provide you with at least an equivalent separation as any other GFC column of similar porosity, type, and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

High Resolution Size Exclusion for Biomolecules

- Extremely high efficiency 3 μm particle
- Huge cost savings
- Extreme surface inertness


Starting with 3 μm ultra-pure silica, Yarra particles are densely bonded with a proprietary hydrophilic surface chemistry. Coupled with tight particle and pore size distribution as well as strict packing and QC specifications, Yarra columns allow for very high efficiency and resolution.

Higher Efficiency, Much Lower Price Compared to TSKgel® – GUARANTEED!

Yarra			VS.	TSKgel*†		
3	3	3		G2000SWxl	G3000SWxl	G4000SWxl
145	290	500	Particle Size (μm)	5	5	8
1K - 300 K	5K - 700 K	15 K - 1,500 K	Pore Size (Å)	125	250	450
2.5 - 7.5	2.5 - 7.5	2.5 - 7.5	MW Range in native conditions (Da)	5K - 150 K	10K - 500 K	20 K - 7,000 K
3000	3000	1700	pH Stability	2.5 - 7.5	2.5 - 7.5	2.5 - 7.5
50	50	50	Maximum Backpressure (psi)	1015	1015	508
1.5	1.5	1.2	Maximum Temperature (°C)	30	30	30
48,000	48,000	38,000	Maximum Flow Rate (mL/min)	1.2	1.2	1.2
			Efficiency (minimum theoretical plates)	20,000	20,000	16,000

*Also guaranteed against other aqueous GFC columns 3 μm or above.

Compare Yarra's Resolving Power to TSKgel's

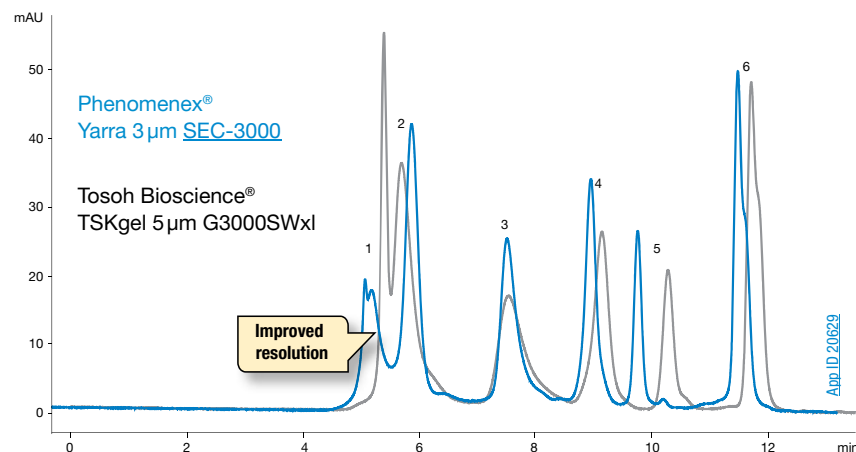

Conditions for both columns:

Columns: Yarra 3 μm SEC-3000
TSKgel 5 μm G3000SWxl

Dimensions: 300 x 7.8 mm

Mobile Phase: 50 mM Sodium Phosphate pH 6.8
/ 0.3 M Sodium Chloride

Flow Rate: 1 mL/min

Backpressure: 99 bar

Temperature: Ambient

Detection: UV @ 220 nm

Sample:
1. IgM
2. Thyroglobulin (669 kDa)
3. Beta Amylase
4. Ovalbumin (44 kDa)
5. Myoglobin (17 kDa)
6. Uridine

Comparative separations may not be representative of all applications.

†All TSKgel specifications were taken from Tosoh Bioscience 2004-5 Laboratory Products Catalog


Yarra™ 3 μm Aqueous GFC/SEC Columns

Extreme Surface Inertness for Accurate and Confident Recoveries

Phenomenex's proprietary surface chemistry provides an inertness hard to match by other GFC columns. The result is minimal


adsorption of proteins and other protein aggregates leading to more accurate quantitation.

Minimal "Priming Effect" with Yarra Columns

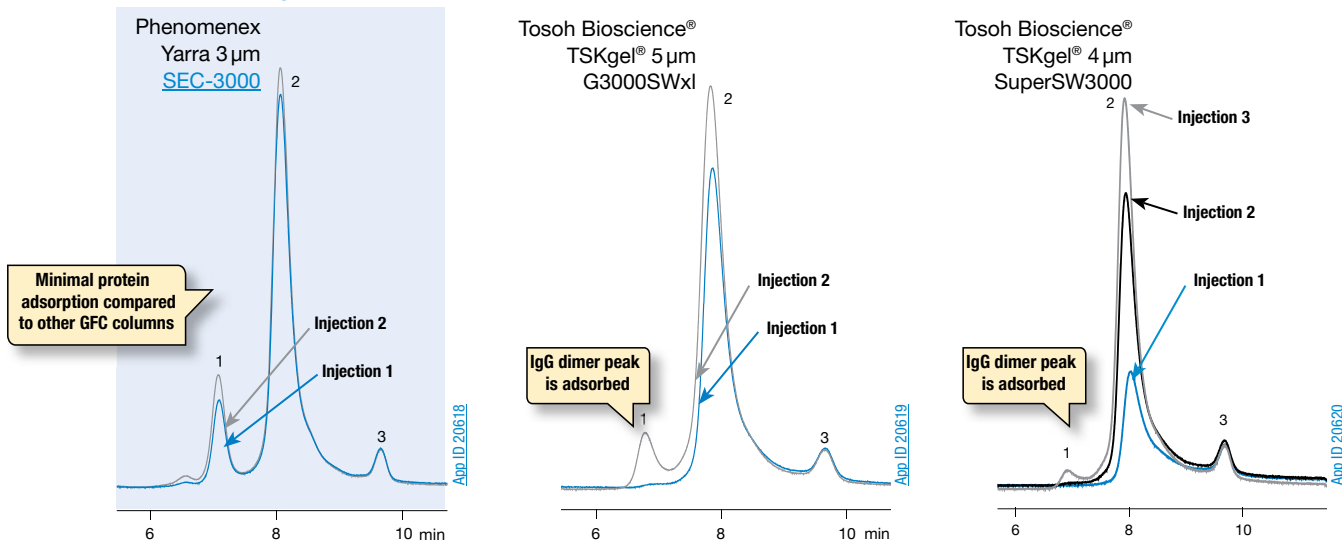

Ultra-High Resolution Size Exclusion for Biomolecules

Yarra 3 μm SEC-3000 vs. 5 μm SEC 3000 Column

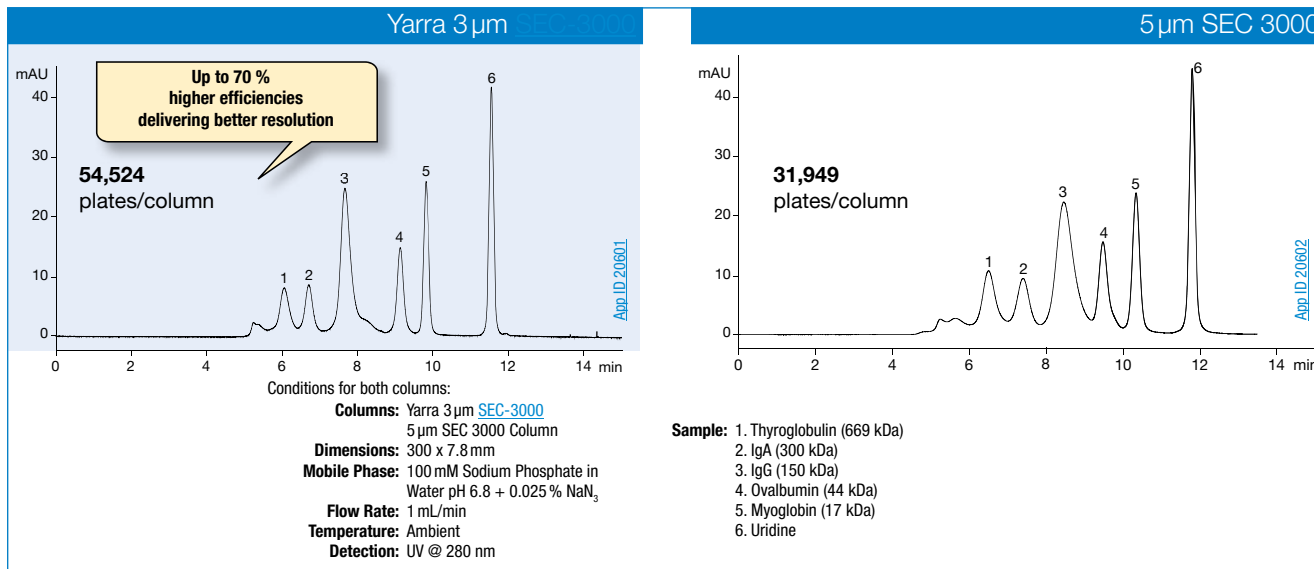


Comparative separations may not be representative of all applications.

Yarra™ 3 μm Aqueous GFC/SEC Columns

Expert Manufacturing for Dependable Performance and Reliability

Reproducible GFC columns require extreme detail in every aspect of the manufacturing and packing process. First, Yarra silica particles are synthesized using narrow tolerances for pore and particle size. Next, bonding of a proprietary hydrophilic ligand is tightly controlled and packing of each column requires validated recipes tested to high specifications.

Batch-to-Batch Reproducibility Yarra 3 μm SEC-3000

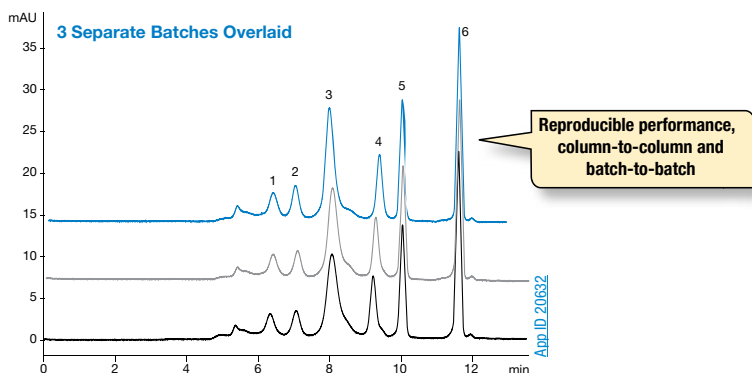


Column: Yarra 3 μm [SEC-3000](#)
Dimensions: 300 x 7.8 mm
Part No.: [00H-4513-K0](#)
Guard Cartridge: [AJ0-4488](#)
Guard Holder: [KJ0-4282](#), SecurityGuard Guard Cartridge Kit
Mobile Phase: 100 mM Sodium Phosphate in Water pH 6.8 + 0.025% Na₃
Flow Rate: 1 mL/min
Detection: UV @ 280 nm
Filter: [AF0-8108-52](#), Phenex-PES 28 mm Syringe Filters 0.45 μm, Non-Sterile, Luer/Slip
Vial: [AR0-9925-13](#), Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: 1. Thyroglobulin (669 kDa)
 2. IgA (300 kDa)
 3. IgG (150 kDa)
 4. Ovalbumin (44 kDa)
 5. Myoglobin (17 kDa)
 6. Uridine

Robust Columns with Long Lifetimes to Get the Most Out of Your Investment

The great care exhibited in both engineering and packing of Yarra columns can produce stable performance over longer lifetimes than other size exclusion columns on the market. Over the course of time, reduced numbers of column replacements add up to significant time and money savings for your lab.

Efficiency and Retention Time Stability on Yarra 3 μm SEC-2000 over 900 Injections

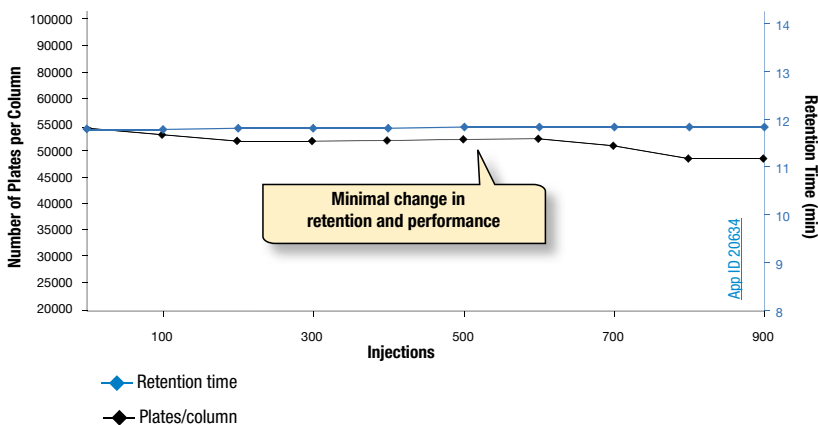

Column: Yarra 3 μm [SEC-2000](#)
Dimensions: 300 x 7.8 mm
Part No.: [00H-4512-K0](#)
Guard Cartridge: [AJ0-4487](#)
Guard Holder: [KJ0-4282](#), SecurityGuard Guard Cartridge Kit
Mobile Phase: 100 mM Sodium Phosphate in Water pH 6.8 + 0.025% Na₃
Flow Rate: 1 mL/min
Detection: UV @ 280 nm
Filter: [AF0-8108-52](#), Phenex-PES 28 mm Syringe Filters 0.45 μm, Non-Sterile, Luer/Slip
Vial: [AR0-9925-13](#), Verex Vial Kit, 9 mm, 2 mL Clear 33 w/ Patch + PTFE/Silicone, preSlit
Sample: 1. Thyroglobulin (669 kDa)
 2. IgA (300 kDa)
 3. IgG (150 kDa)
 4. Ovalbumin (44 kDa)
 5. Myoglobin (17 kDa)
 6. Uridine

Yarra™ 3 μm Aqueous GFC/SEC Columns

guarantee


If Yarra analytical columns do not provide you with at least an equivalent separation as any other GFC column of similar porosity, type, and dimensions, return the column with comparative data within 45 days for a FULL REFUND.

Selecting the Right Yarra Column for Your Application


It is useful to employ the differences in selectivity between Yarra [SEC-2000](#), [SEC-3000](#) and [SEC-4000](#) columns. For molecular weight ranges where overlap occurs, we suggest screening at least two phases to identify the optimal selectivity for your separation.

Use the MW chart and/or calibration curves to select the most appropriate phase(s) to evaluate.

Molecular Weight (MW) Separation Ranges for Yarra

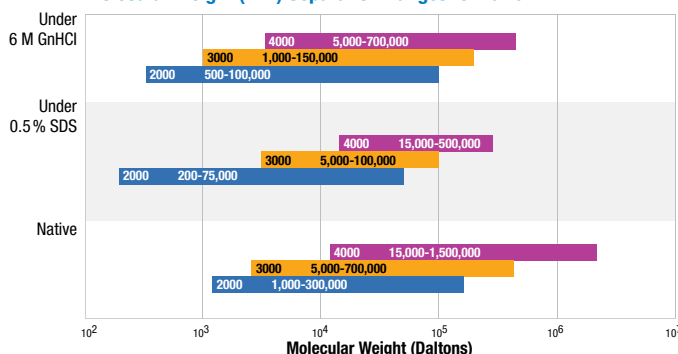

MW Calibration Curves for Protein Separation

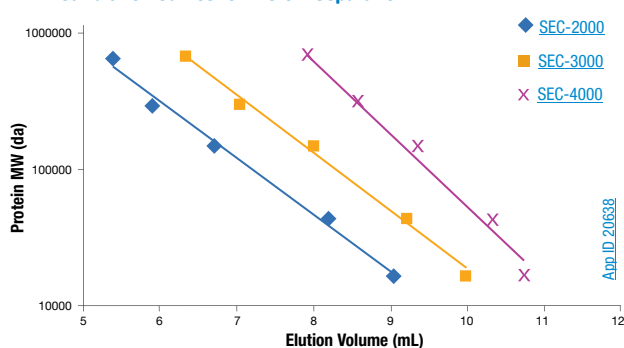

Aqueous SEC 1 Column Check Standard (for Yarra 3 μm SEC and other protein SEC columns)

Part No.: [AL0-3042](#)

Unit quantity: Dry; reconstituted to 2 mL

Contains: Bovine thyroglobulin; Human gamma globulin (contains IgA and IgG); Ovalbumin; Myoglobin; Uridine (reconstitute with 1 mL of 100 mM Sodium phosphate pH 6.8)

Diluent: 100 mM Sodium phosphate pH 6.8

Storage: Add 0.1 % NaNO₂ to the solution and refrigerate

Test Conditions


Mobile phase: 100 mM Sodium phosphate, pH 6.8

Flow rate: 1.0 mL/min for a 300 x 7.8 mm column

Injection volume: 10 μL

Detection: UV @ 280 nm

SEM of Yarra 3 μm Particle



“I was very impressed with the Yarra [SEC-3000](#), 300x7.8 mm column. It provided excellent resolution between the monomer and HMWP peaks, which allowed for consistent integration. The peak shape was greatly improved for all sample components. We immediately revised our test method to include the Yarra [SEC-3000](#) column. This is a column that G.H. Lathe and C.R.J. Ruthven would be proud of!”

Kieran Curley,
Mannkind Corporation, Danbury, CT, USA

Ordering Information

Yarra 3 μm SEC Columns (mm)	Narrow Bore	Analytical	Analytical	SecurityGuard™ Cartridges (mm)
Phases	300 x 4.6	150 x 7.8	300 x 7.8	4 x 3.0*
Yarra 3 μm SEC-2000	00H-4512-E0	00F-4512-K0	00H-4512-K0	AJ0-4487
Yarra 3 μm SEC-3000	00H-4513-E0	00F-4513-K0	00H-4513-K0	AJ0-4488
Yarra 3 μm SEC-4000	00H-4514-E0	—	00H-4514-K0	AJ0-4489

*SecurityGuard™ Analytical Cartridges require holder, Part No.: [KJ0-4282](#)

for ID: 4.6 - 7.8 mm



For information on SecurityGuard column protection, see p. 326


The opinions stated herein are solely those of the speaker and not necessarily those of any company or organization.

Yarra™ 5 μm PREP Aqueous GFC/SEC Columns

Higher Performance for Preparative BioSeparations at a Lower Price

Enjoy the same selectivity and ultra-high efficiency of Yarra 3 μm for your preparative gel filtration applications. Yarra SEC PREP features a 5 μm particle size version of the original Yarra 3 μm particle with the same chemistry on a 21.2 mm ID column for preparative purification, desalting, and characterization of biomolecules. Yarra 5 μm PREP is available at an affordable price while maintaining the high performance given with the analytical columns.

Yarra 5 μm SEC/GFC PREP Column

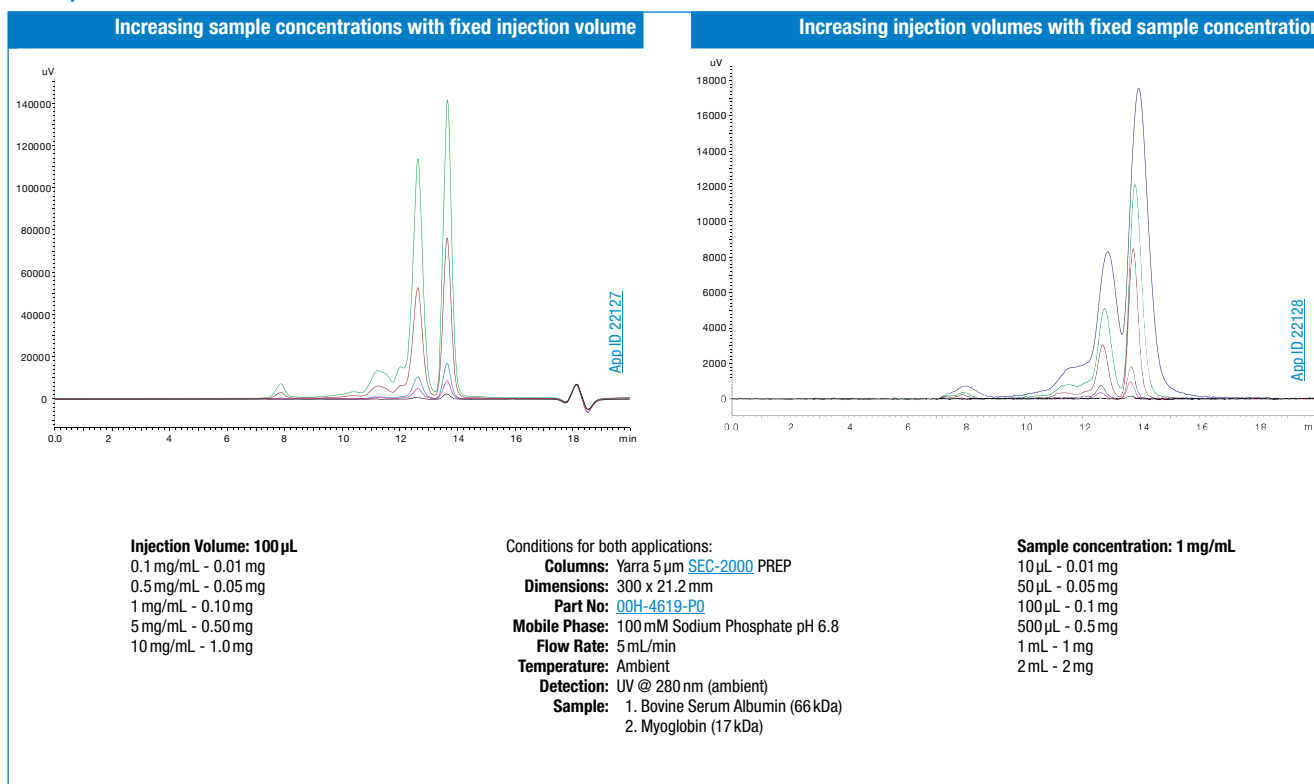

Yarra 5 μm PREP SEC Columns (mm)	Preparative	SecurityGuard™ Cartridges (mm)
Phases	300 x 21.2	15 x 21.2**
		/ea
Yarra 5 μm SEC-2000 PREP	00H-4619-P0	AJ0-8588
Yarra 5 μm SEC-3000 PREP	00H-4620-P0	AJ0-8589
Yarra 5 μm SEC-4000 PREP	00H-4621-P0	AJ0-8590

**PREP SecurityGuard™ Cartridges require holder, Part No.: [AJ0-8223](#) for ID: 18 - 29 mm



Zorbax®

Manufactured by Agilent Technologies®

Ordering Information

Eclipse XDB Columns

Column	µm	Size (mm)	XDB-C18 (L1)	XDB-C8 (L7)
Analytical	5	250 x 4.6	990967-902	990967-906
Analytical	5	150 x 4.6	993967-902	993967-906
Rapid Resolution	3.5	75 x 4.6	966967-902	—

StableBond 80 Å Columns

Column	µm	Size (mm)	SB-C18 (L1)	SB-C8 (L7)	SB-CN (L10)	SB-Phenyl (L11)
Analytical	5	250 x 4.6	880975-902	880975-906	880975-905	880975-912
Analytical	5	150 x 4.6	883975-902	883975-906	883975-905	883975-912
Rapid Resolution	3.5	150 x 4.6	863953-902	863953-906	863953-905	863953-912
Rapid Resolution	3.5	75 x 4.6	—	866953-906	—	—

Rx 80 Å Reversed-Phase HPLC Columns

Column	µm	Size (mm)	Rx-C8 (L7)
Analytical	5	250 x 4.6	880967-901
Analytical	5	150 x 4.6	883967-901
Rapid Resolution	3.5	150 x 4.6	863953-906



StableBond 300 Å (Wide Pore) columns available

Traditional Reversed-Phase Columns

Column	µm	Size (mm)	ODS C18 (L1)	C8 (L7)
Analytical	5	250 x 4.6	880952-702	880952-706
Analytical	5	150 x 4.6	883952-702	—